

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
 Data File : PD060039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 11:16
 Operator : DD\AJ
 Sample : RESC06
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 05:10:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.506	4.024	17210042	60961618	20.083	20.451
2)	SA Decachlor...	8.306	9.112	33153194	97401957	39.901	39.594
Target Compounds							
2)	A alpha-BHC	3.947	4.415	13294710	44314128	10.345	9.948
3)	MA gamma-BHC...	4.234	4.701	12676168	40504050	10.370	10.008
4)	MA Heptachlor	4.541	5.213	12196116	39330096	10.391	9.920
5)	MB Aldrin	4.793	5.520	11872363	37134044	10.341	10.009
6)	B beta-BHC	4.484	4.869	5531271	19090750	10.439	10.273
7)	B delta-BHC	4.693	5.088	12836570	35853136	10.215	9.785
8)	B Heptachlo...	5.240	5.906	10904834	33282478	10.323	10.105
9)	A Endosulfan I	5.583	6.264	10725975	32672381	10.545	10.194
10)	B trans-Chl...	5.469	6.140	10945928	34133351	10.306	9.935
11)	B cis-Chlor...	5.528	6.214	10928738	34404230	10.331	10.020
12)	B 4,4'-DDE	5.693	6.369	21110551	63499756	20.655	19.638
13)	MA Dieldrin	5.828	6.521	22539861	69875802	20.687	20.011
14)	MA Endrin	6.088	6.740	18675360	56027110	20.701	20.009
15)	B Endosulfa...	6.361	6.948	18748774	56705375	20.791	20.060
16)	A 4,4'-DDD	6.212	6.859	18362326	53314059	20.763	19.873
17)	MA 4,4'-DDT	6.456	7.159	18439571	53393774	20.517	19.621
18)	B Endrin al...	6.530	7.072	15680871	49208705	21.064	20.453
19)	B Endosulfa...	6.745	7.295	17890386	58354207	20.472	20.242
20)	A Methoxychlor	7.005	7.616	44410638	144.7E6	104.356	102.915
21)	B Endrin ke...	7.240	7.768	21632206	60550700	21.747	20.763

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 11:16
Operator : DD\AJ
Sample : RESC06
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:10:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

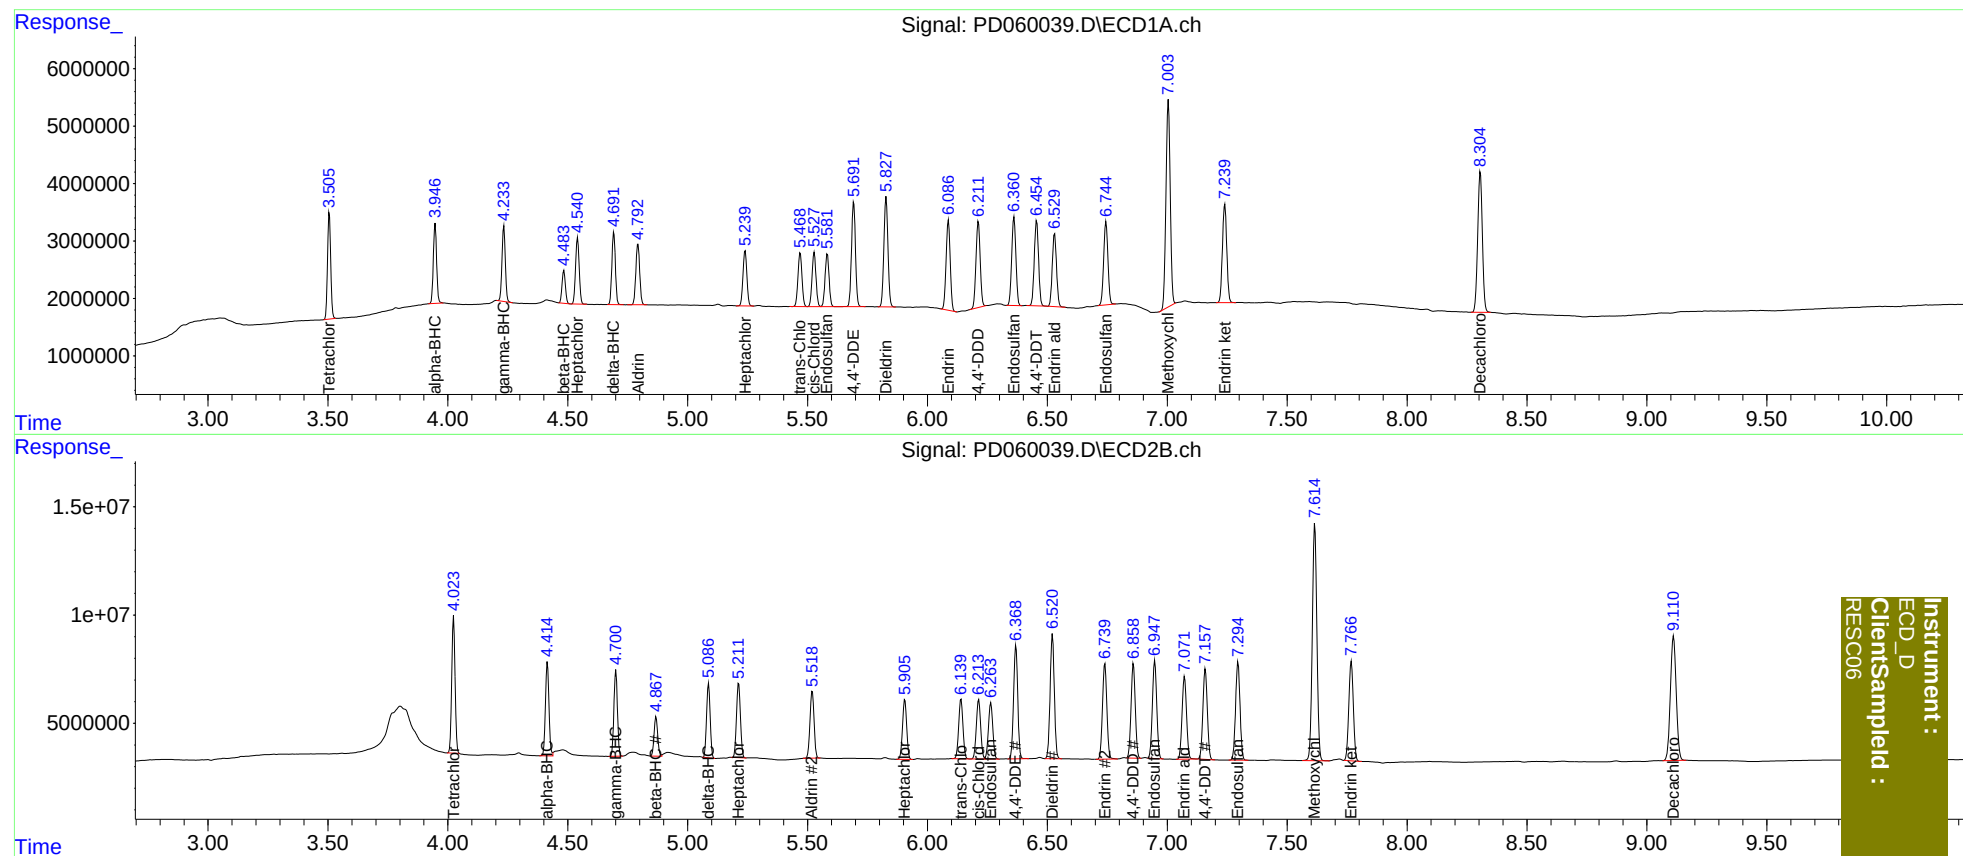

Instrument :
ECD_D
ClientSampled :
RESC06

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060039.D
Acq On : 03 Nov 2020 11:16
Operator : DD\AJ
Sample : RESC06
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Title : GC Extractables
Last Update : Wed Nov 04 04:05:33 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.506	3.948	100.00%
3.948	4.234	100.00%
4.234	4.484	100.00%
4.484	4.541	100.00%
4.541	4.693	100.00%
4.693	4.793	100.00%
4.793	5.240	100.00%
5.240	5.469	100.00%
5.469	5.528	100.00%
5.528	5.583	100.00%
5.583	5.693	100.00%
5.693	5.828	100.00%
5.828	6.088	100.00%
6.088	6.212	100.00%
6.212	6.361	100.00%
6.361	6.456	100.00%
6.456	6.530	100.00%
6.530	6.745	100.00%
6.745	7.005	100.00%
7.005	7.240	100.00%
7.240	8.306	100.00%

Signal #2


4.024	4.415	100.00%
4.415	4.701	100.00%
4.701	4.869	100.00%
4.869	5.088	100.00%
5.088	5.213	100.00%
5.213	5.520	100.00%
5.520	5.906	100.00%
5.906	6.140	100.00%
6.140	6.214	100.00%
6.214	6.264	98.90%
6.264	6.369	100.00%
6.369	6.521	100.00%
6.521	6.740	100.00%
6.740	6.859	100.00%
6.859	6.948	100.00%
6.948	7.072	100.00%
7.072	7.159	100.00%
7.159	7.295	100.00%
7.295	7.616	100.00%
7.616	7.768	100.00%
7.768	9.112	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 11:16
Operator : DD\AJ
Sample : RESC06
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:10:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

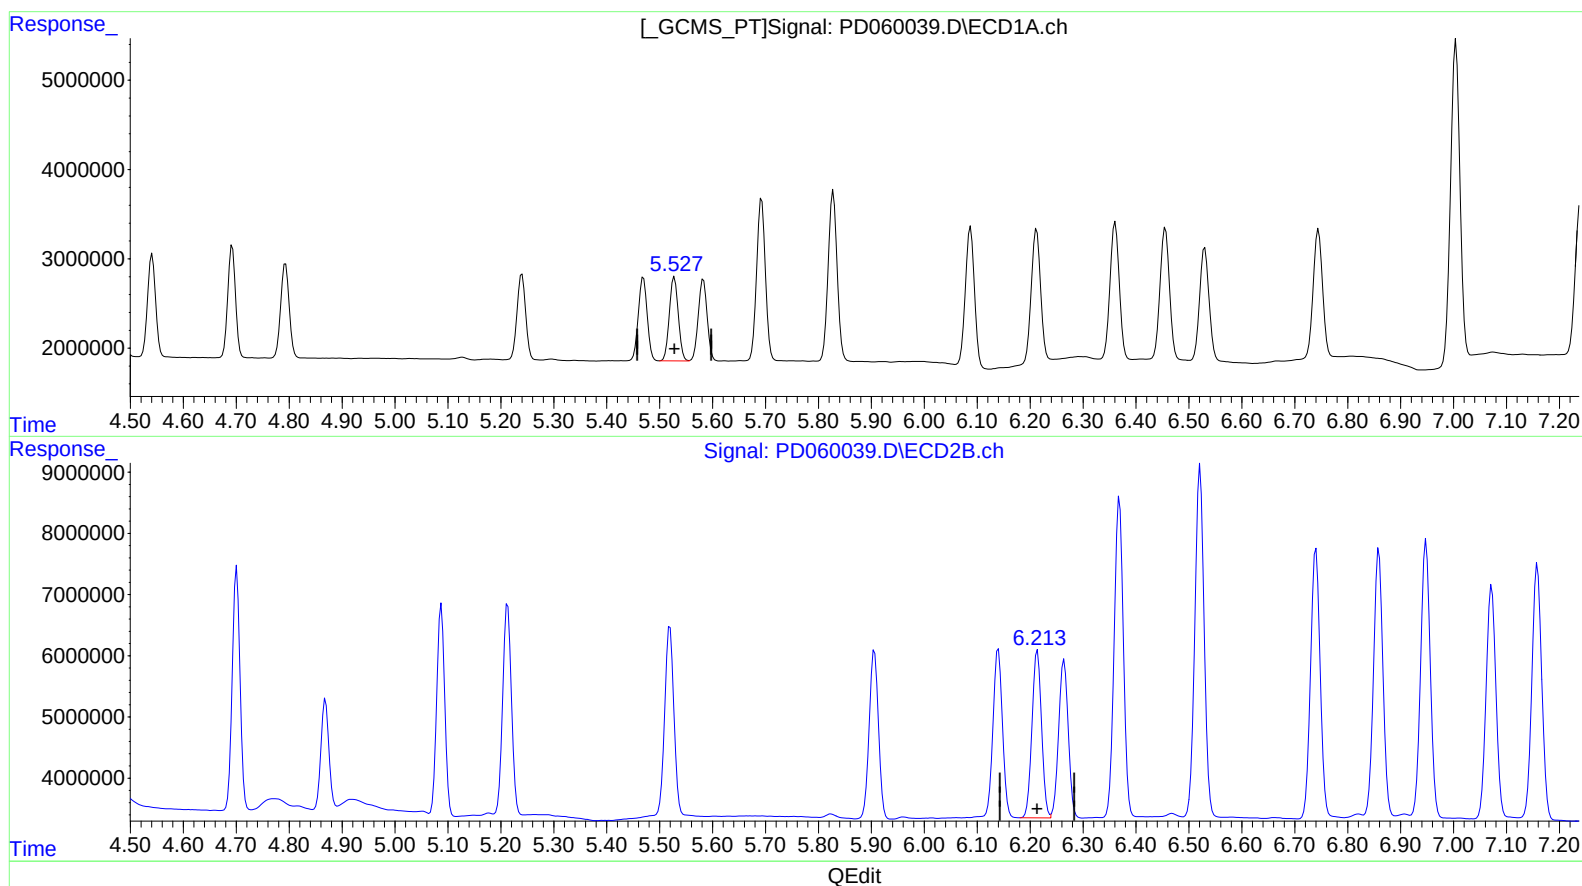

(11) cis-Chlordane (B)

5.528min 10.331 ng/ml

response 10928738

(11) cis-Chlordane #2 (B)

6.214min 10.020 ng/ml

response 34404230