

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110323\
 Data File : PD079377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2023 22:43
 Operator : AR\AJ
 Sample : PB156831BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:16:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.802	26149394	38957360	17.050	17.965
27)	SA Decachlor...	9.112	7.950	38209000	48271743	20.145	20.697
Target Compounds							
3)	MA gamma-BHC...	0.000	3.655	0	107958	N.D.	<MDL
4)	MA Heptachlor	0.000	3.983	0	228175	N.D.	<MDL
5)	MB Aldrin	0.000	4.267	0	269665	N.D.	<MDL
6)	B beta-BHC	0.000	3.896f	0	33304	N.D.	<MDL
9)	A Endosulfan I	0.000	5.132	0	754796	N.D.	0.297
11)	B cis-Chlor...	0.000	5.094	0	591891	N.D.	0.209
13)	MA Dieldrin	0.000	5.447f	0	105879	N.D.	<MDL
15)	B Endosulfa...	0.000	5.924f	0	43685	N.D.	<MDL
20)	A Methoxychlor	0.000	6.661	0	105920	N.D.	<MDL
22)	Toxaphene-1	0.000	5.094f	0	591891	N.D.	38.331
24)	Toxaphene-3	0.000	6.661	0	105920	N.D.	2.024


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110323\
Data File : PD079377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2023 22:43
Operator : AR\AJ
Sample : PB156831BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:16:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

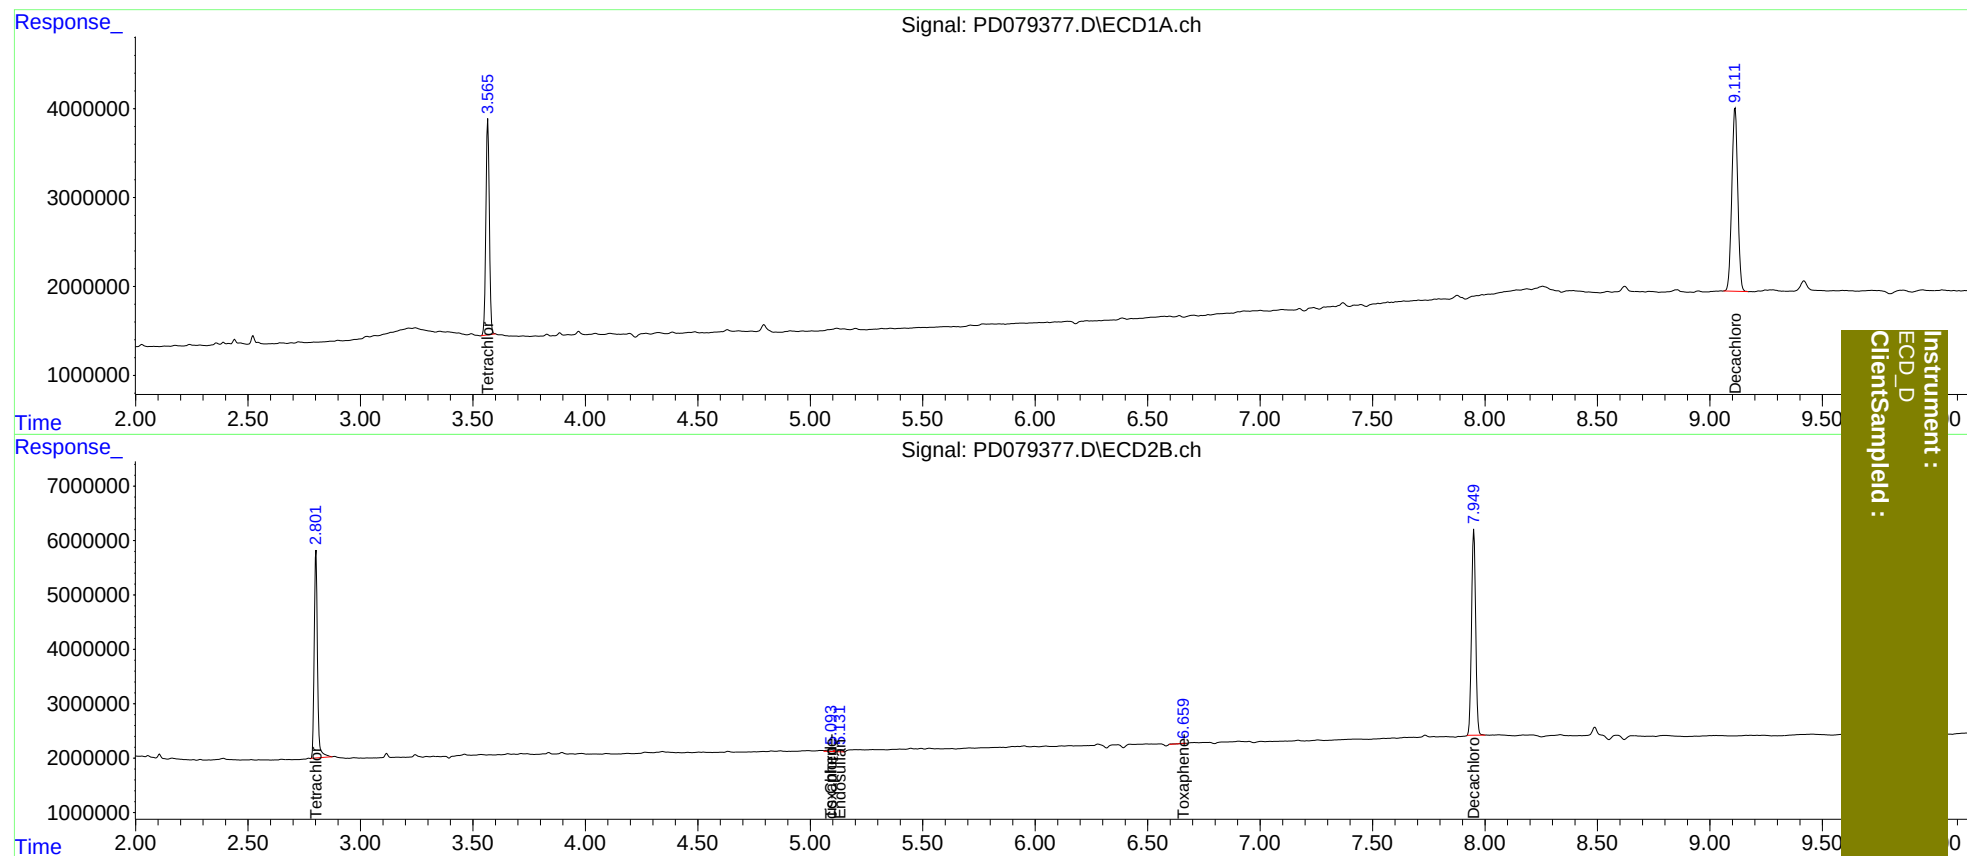


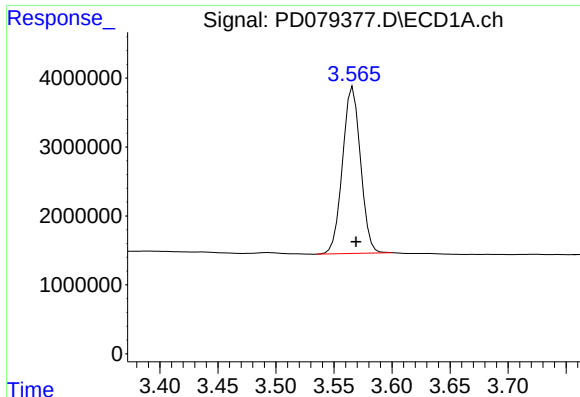

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: -0.003 min
Response: 26149394
Conc: 17.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

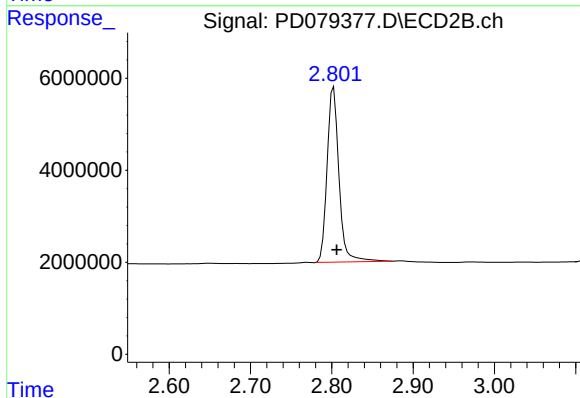


#1 Tetrachloro-m-xylene

R.T.: 2.802 min
Delta R.T.: -0.004 min
Response: 38957360
Conc: 17.96 ng/ml

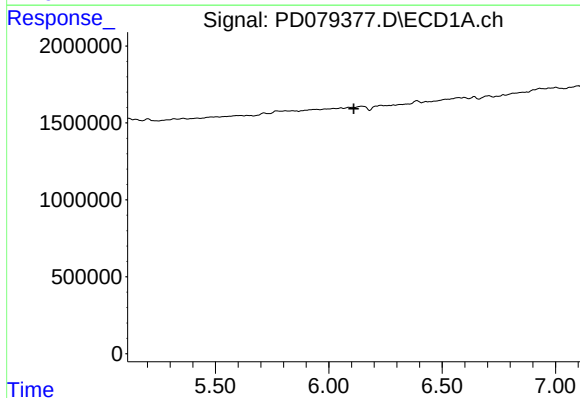


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.110 min
Response: 0
Conc: N.D.

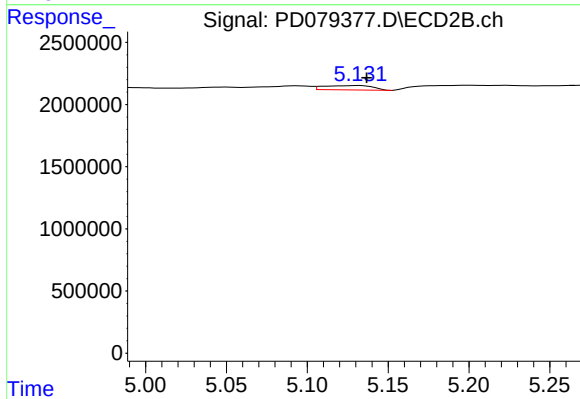

#9 Endosulfan I


R.T.: 5.132 min
Delta R.T.: -0.005 min
Response: 754796
Conc: 0.30 ng/ml

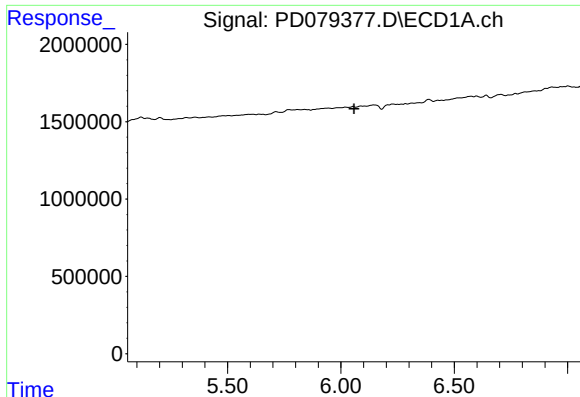

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

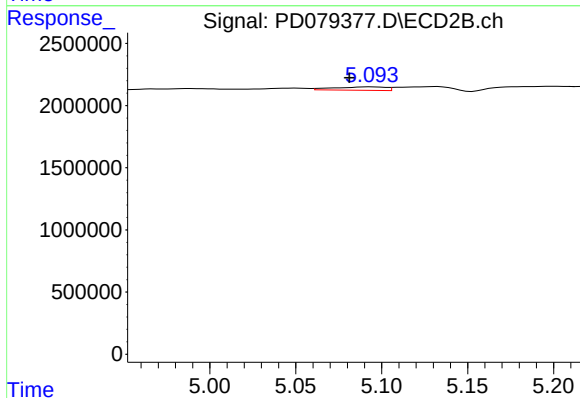


#11 cis-Chlordane

R.T.: 5.094 min
Delta R.T.: 0.013 min
Response: 591891
Conc: 0.21 ng/ml

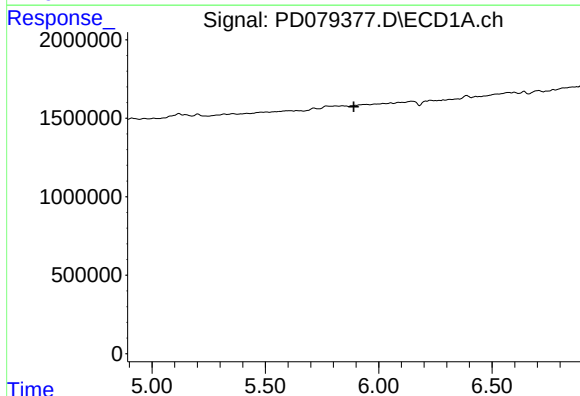


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 5.890 min
Response: 0
Conc: N.D.

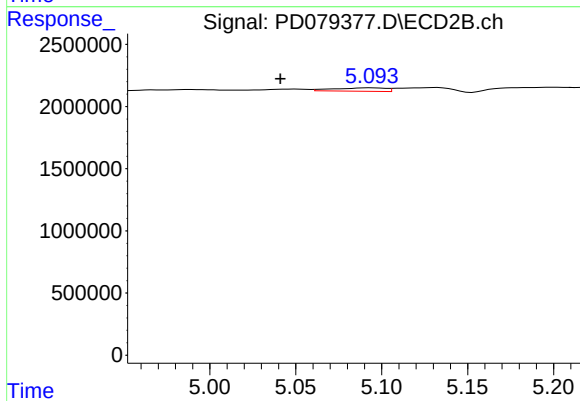

#22 Toxaphene-1


R.T.: 5.094 min
Delta R.T.: 0.053 min
Response: 591891
Conc: 38.33 ng/ml

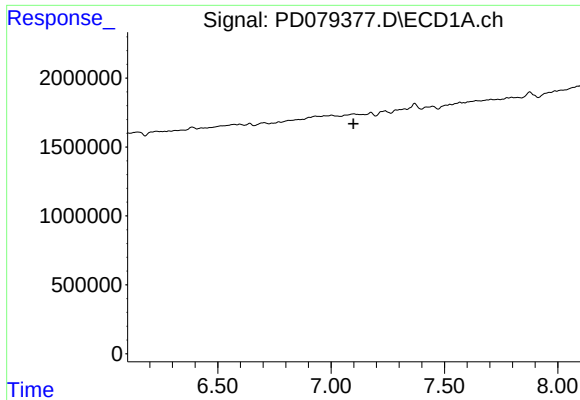

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 7.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

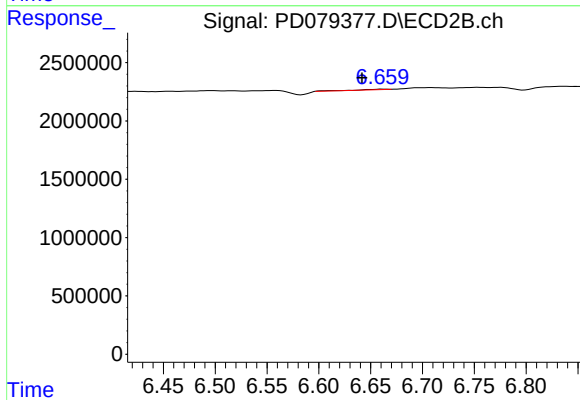


#24 Toxaphene-3

R.T.: 6.661 min
Delta R.T.: 0.020 min
Response: 105920
Conc: 2.02 ng/ml

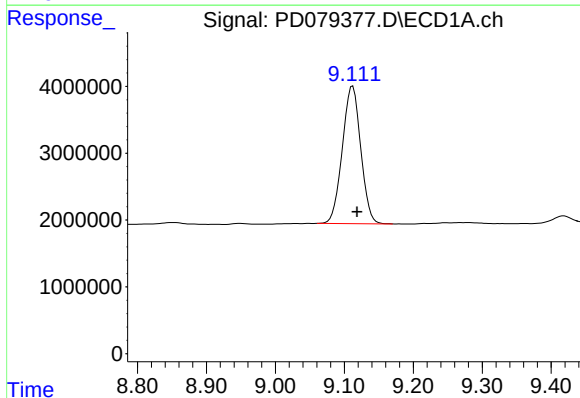

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: -0.006 min
Response: 38209000
Conc: 20.15 ng/ml

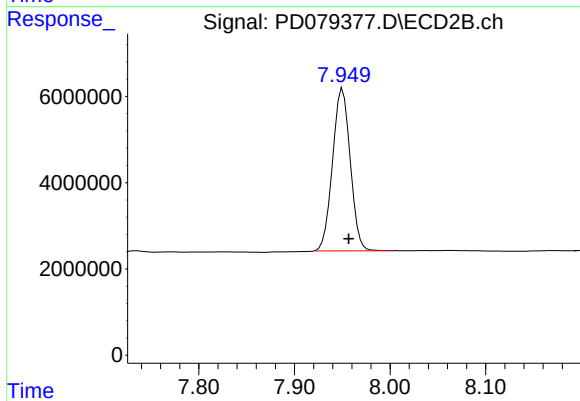

#27 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: -0.006 min
Response: 48271743
Conc: 20.70 ng/ml