

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110323\
 Data File : PD079344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2023 14:35
 Operator : AR\AJ
 Sample : 05057-05MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A4939MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 22:14:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.803	27031493	38671807	17.625	17.833
27)	SA Decachlor...	9.117	7.953	38538703	47438065	20.319	20.340
Target Compounds							
2)	A alpha-BHC	4.025	3.306	123.8E6	176.0E6	47.533	51.606
3)	MA gamma-BHC...	4.358	3.636	115.6E6	159.2E6	46.439	49.256
4)	MA Heptachlor	4.952	3.979	108.4E6	143.5E6	40.678	47.204
5)	MB Aldrin	5.295	4.260	101.7E6	138.6E6	41.145	45.002
6)	B beta-BHC	4.551	3.931	48148943	66163485	42.225	45.746
7)	B delta-BHC	4.801	4.163	118.5E6	162.6E6	45.180	49.571
8)	B Heptachlo...	5.722	4.762	103.6E6	141.9E6	43.139	49.175
9)	A Endosulfan I	6.108	5.133	96867709	131.6E6	45.217	51.839
10)	B trans-Chl...	5.977	5.013	98610831	139.9E6	44.517	50.511
11)	B cis-Chlor...	6.058	5.078	100.4E6	141.8E6	44.168	50.072
12)	B 4,4'-DDE	6.228	5.267	191.7E6	266.5E6	93.051	101.901
13)	MA Dieldrin	6.384	5.398	210.7E6	299.4E6	92.747	101.636
14)	MA Endrin	6.614	5.673	181.6E6	266.6E6	95.903	105.669
15)	B Endosulfa...	6.832	5.966	179.9E6	249.5E6	90.727	104.868
16)	A 4,4'-DDD	6.745	5.820	156.3E6	223.7E6	93.013	101.265
17)	MA 4,4'-DDT	7.061	6.072	170.4E6	236.7E6	95.158	105.056
18)	B Endrin al...	6.962	6.146	131.7E6	179.9E6	86.851	97.079
19)	B Endosulfa...	7.196	6.368	170.9E6	233.4E6	88.936	101.281
20)	A Methoxychlor	7.534	6.648	426.4E6	576.8E6	444.462	473.085
21)	B Endrin ke...	7.684	6.875	182.8E6	270.1E6	87.512	102.326

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110323\
Data File : PD079344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2023 14:35
Operator : AR\AJ
Sample : 05057-05MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 22:14:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

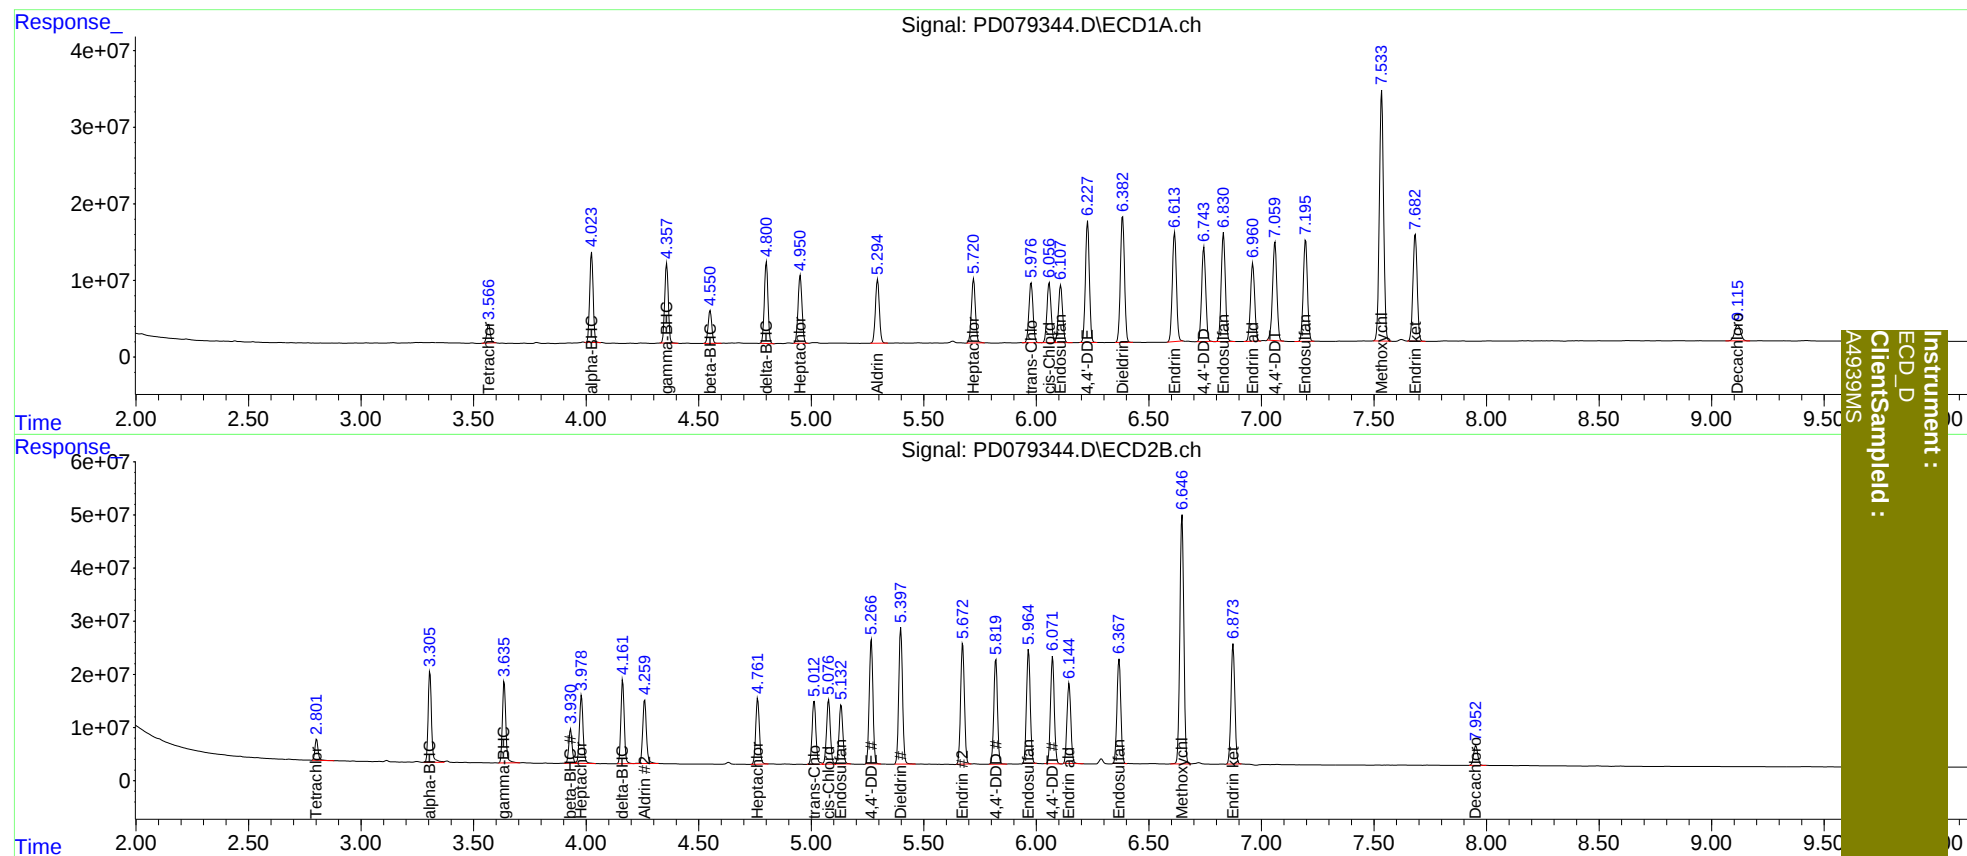

Instrument :
ECD_D
ClientSampled :
A4939MS