

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110323\
 Data File : PD079349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2023 15:46
 Operator : AR\AJ
 Sample : 05013-06MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A49B9MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/02/2023
 Supervised By : mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 22:15:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.803	22902198	34469795	14.933	15.895
27)	SA Decachlor...	9.115	7.952	30849053	39044467	16.265	16.741
Target Compounds							
2)	A alpha-BHC	4.025	3.307	107.5E6	156.5E6	41.242	45.893
3)	MA gamma-BHC...	4.359	3.637	100.5E6	140.5E6	40.400	43.462
4)	MA Heptachlor	4.951	3.980	102.5E6	136.4E6	38.464	44.864
5)	MB Aldrin	5.295	4.261	97787281	124.3E6	39.552	40.352
6)	B beta-BHC	4.551	3.932	44885059	60278528	39.362	41.677
7)	B delta-BHC	4.801	4.163	101.5E6	141.4E6	38.678	43.113
8)	B Heptachlo...	5.721	4.763	92975021	126.7E6	38.716	43.914
9)	A Endosulfan I	6.108	5.134	86978049	118.5E6	40.601	46.650
10)	B trans-Chl...	5.977	5.013	88144161	123.3E6	39.792	44.516
11)	B cis-Chlor...	6.057	5.078	89152695	125.3E6	39.220	44.243
12)	B 4,4'-DDE	6.228	5.267	167.8E6	236.2E6	81.446	90.338
13)	MA Dieldrin	6.383	5.399	188.0E6	265.8E6	82.746	90.228
14)	MA Endrin	6.614	5.674	162.4E6	237.3E6	85.756	94.043
15)	B Endosulfa...	6.832	5.966	161.7E6	222.5E6	81.542	93.528
16)	A 4,4'-DDD	6.745	5.821	138.9E6	196.9E6	82.666	89.139
17)	MA 4,4'-DDT	7.060	6.072	151.5E6	210.2E6	84.598	93.310
18)	B Endrin al...	6.962	6.144	114.3E6	157.4E6	75.332	84.952m
19)	B Endosulfa...	7.197	6.368	154.8E6	207.7E6	80.575	90.100
20)	A Methoxychlor	7.534	6.648	390.1E6	525.9E6	406.660	431.348
21)	B Endrin ke...	7.683	6.874	166.4E6	240.2E6	79.629	91.010

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110323\
Data File : PD079349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2023 15:46
Operator : AR\AJ
Sample : 05013-06MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 22:15:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

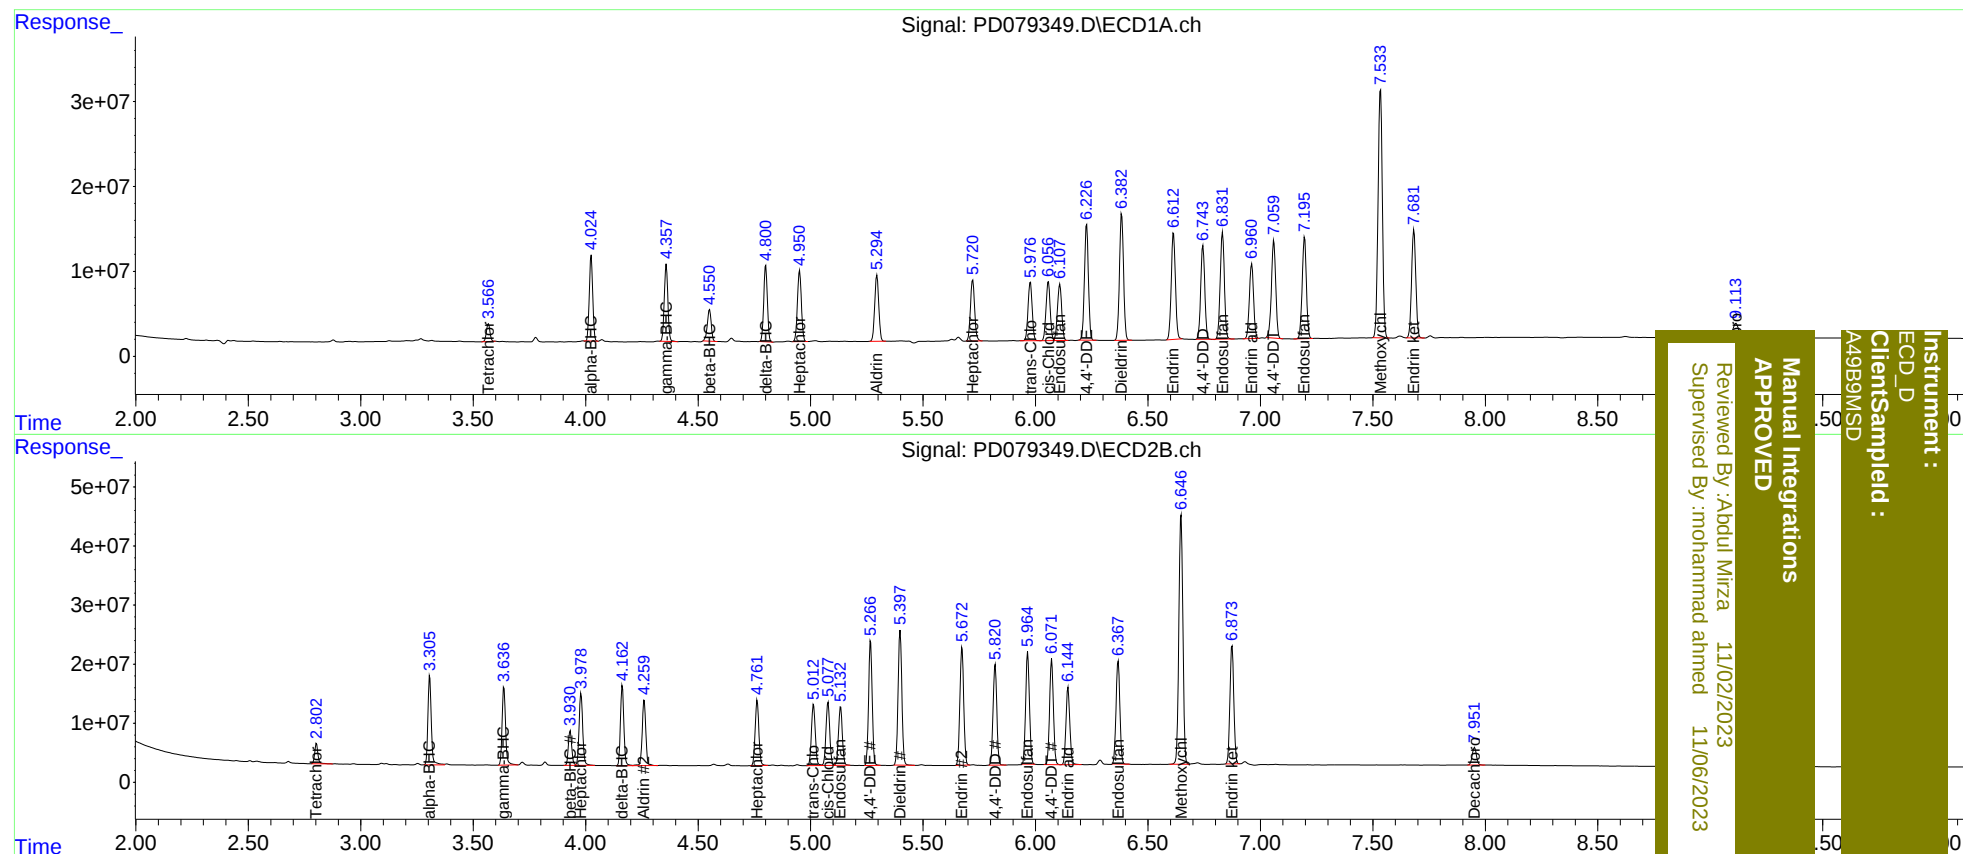

Instrument :
ECD_D
ClientSampled :
A49B9MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 11/02/2023
Supervised By: mohammad ahmed 11/06/2023