

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110419\
 Data File : PD055830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2019 15:02
 Operator : SG\AJ
 Sample : PB124511BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:38:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.296	3.961	18513278	25152773	24.593	24.002
27)	SA Decachlor...	7.972	8.998	37101541	47713435	45.517	42.017
Target Compounds							
19)	B Endosulfa...	0.000	7.243f	0	2569720	N.D.	2.131

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110419\
Data File : PD055830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2019 15:02
Operator : SG\AJ
Sample : PB124511BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:38:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

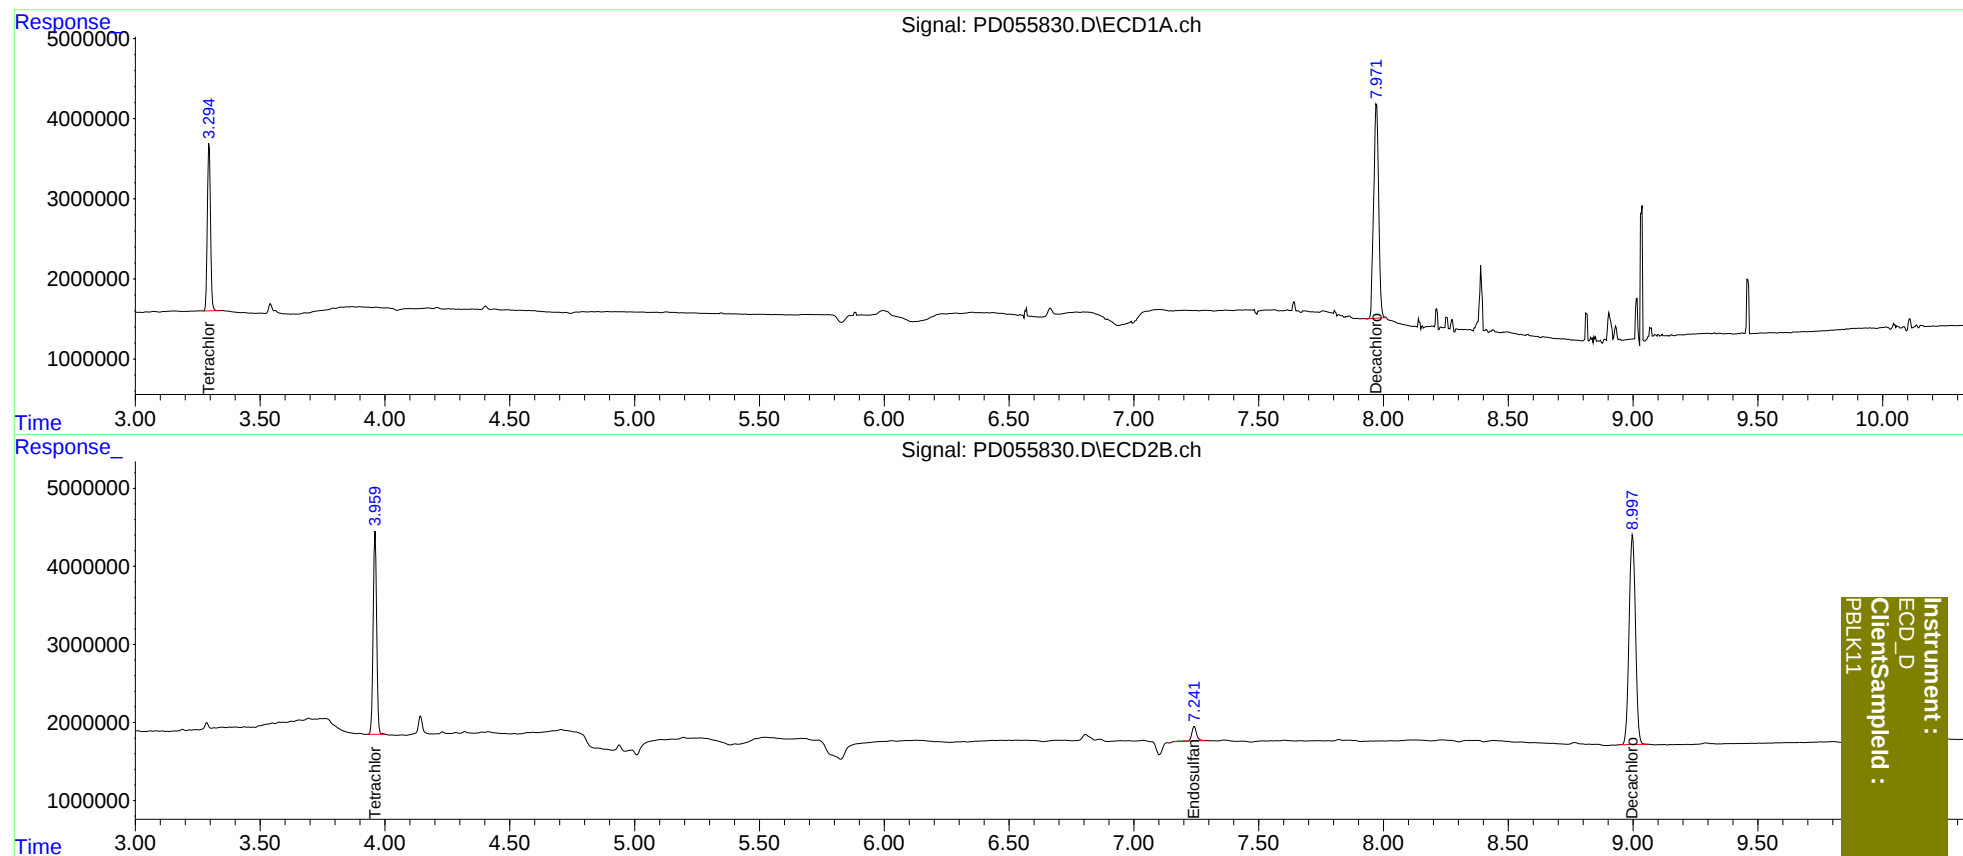


Instrument :
ECD_D
ClientSampleId :
PBLK11

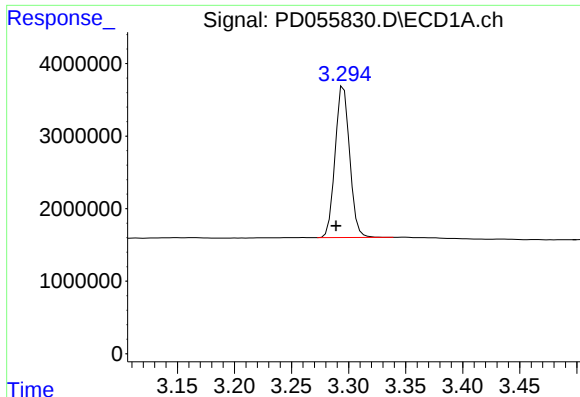

#1 Tetrachloro-m-xylene


R.T.: 3.296 min
Delta R.T.: 0.007 min
Response: 18513278
Conc: 24.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK11

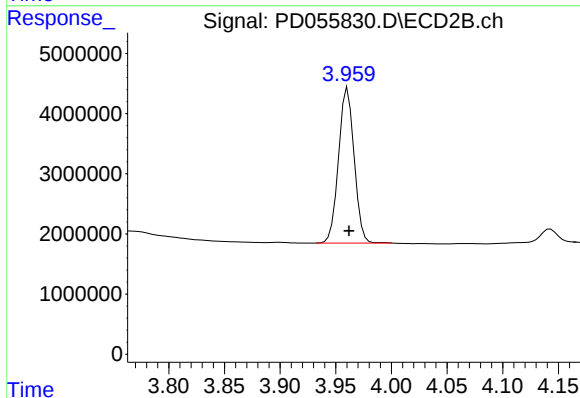


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.001 min
Response: 25152773
Conc: 24.00 ng/ml

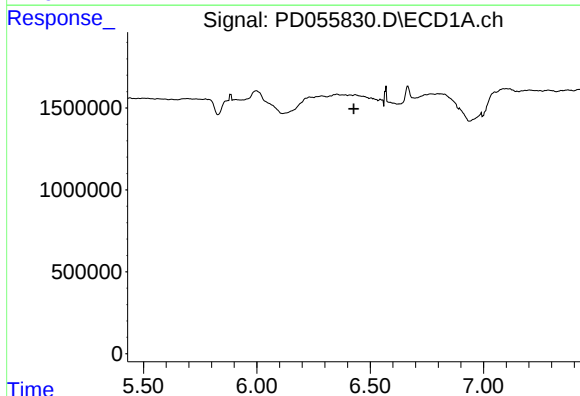


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

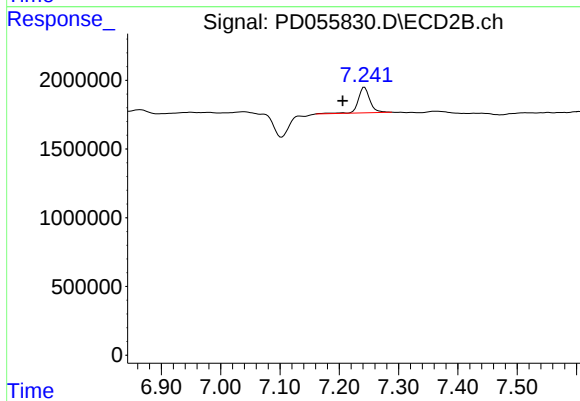

#19 Endosulfan Sulfate


R.T.: 7.243 min
Delta R.T.: 0.037 min
Response: 2569720
Conc: 2.13 ng/ml

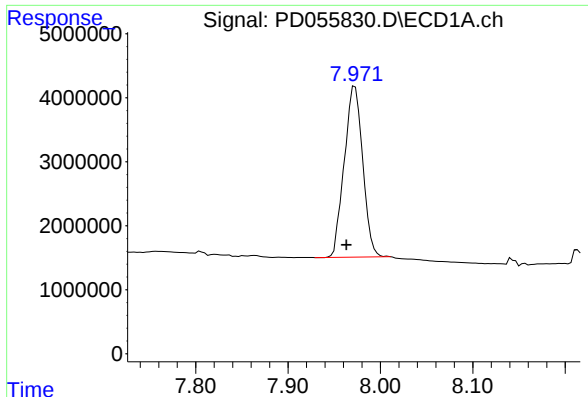

#27 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: 0.009 min
Response: 37101541
Conc: 45.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK11

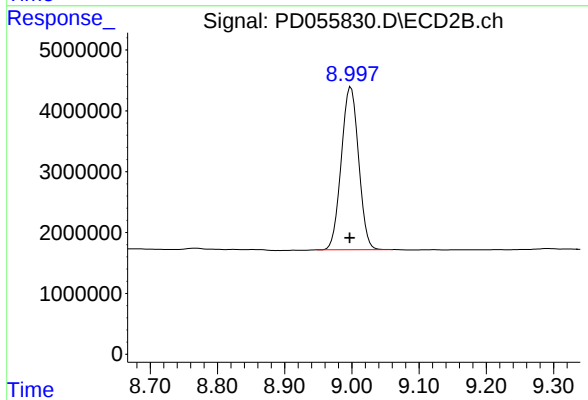

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.002 min
Response: 47713435
Conc: 42.02 ng/ml