

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110419\
 Data File : PD055837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2019 16:40
 Operator : SG\AJ
 Sample : K5629-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5AG7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:39:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	20229122	25003079	26.873	23.859
27)	SA Decachlor...	7.962	8.996	29906296	38770184	36.690	34.142
Target Compounds							
8)	B Heptachlo...	0.000	5.803	0	5343513	N.D.	3.959
15)	B Endosulfa...	0.000	6.868	0	3197642	N.D.	2.469

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110419\
Data File : PD055837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2019 16:40
Operator : SG\AJ
Sample : K5629-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:39:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

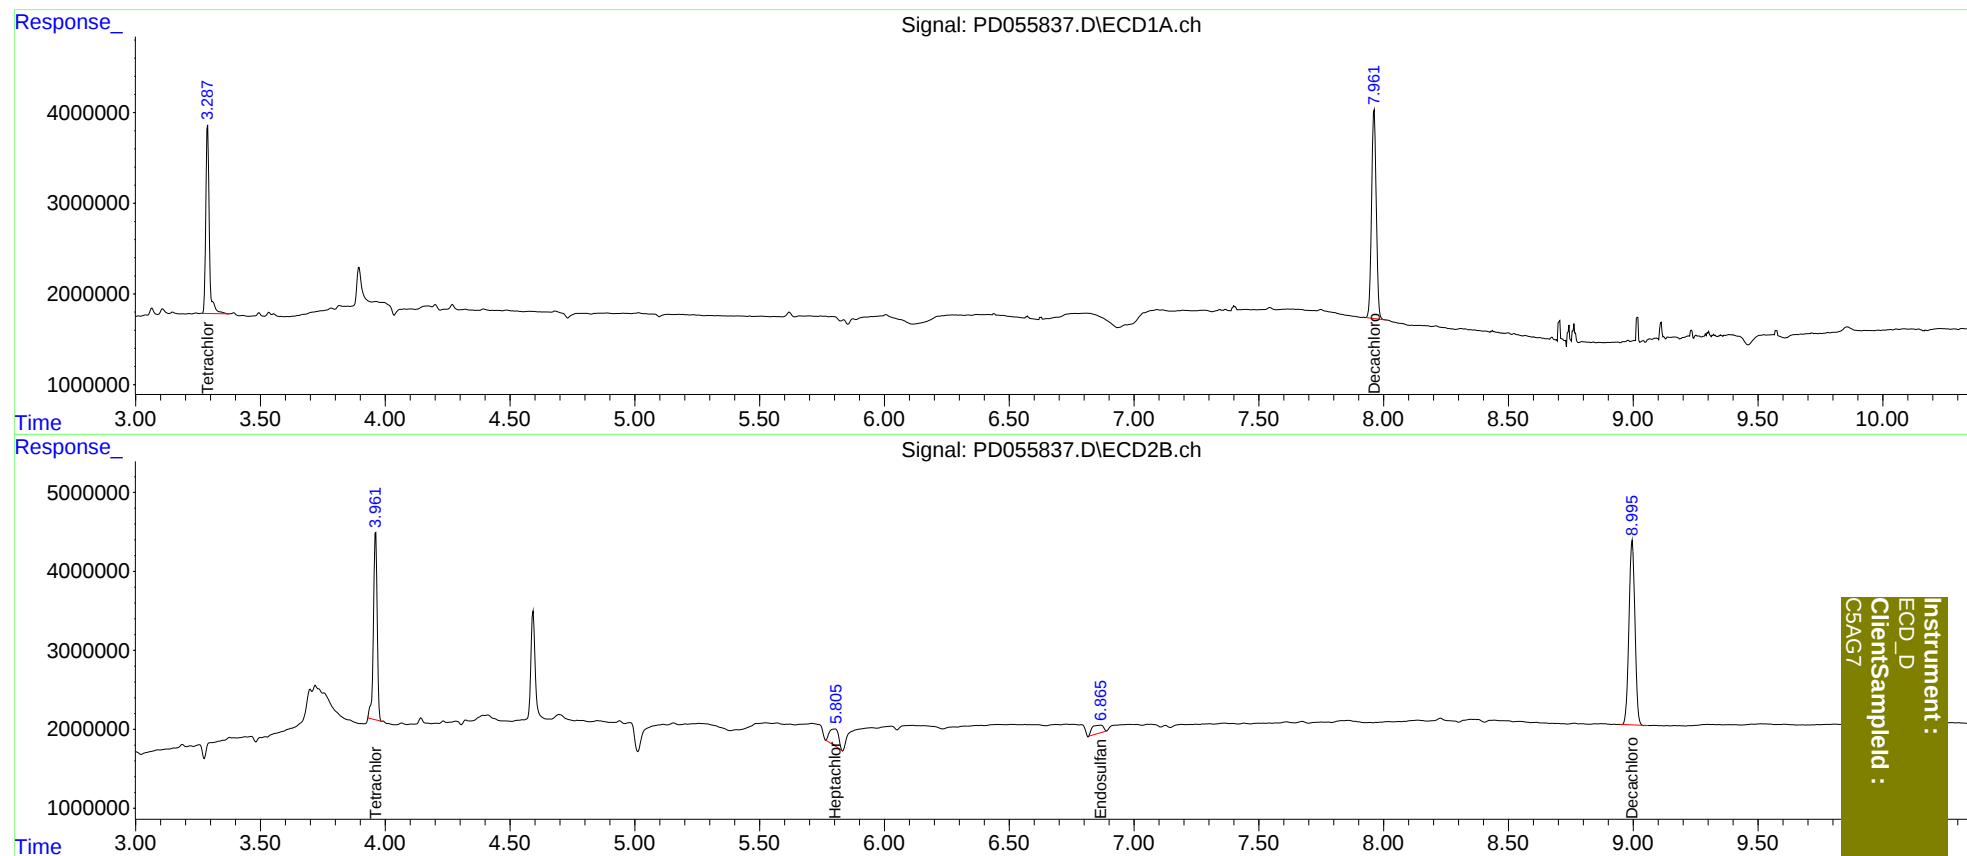


Instrument :
ECD_D
ClientSampleId :
C5AG7

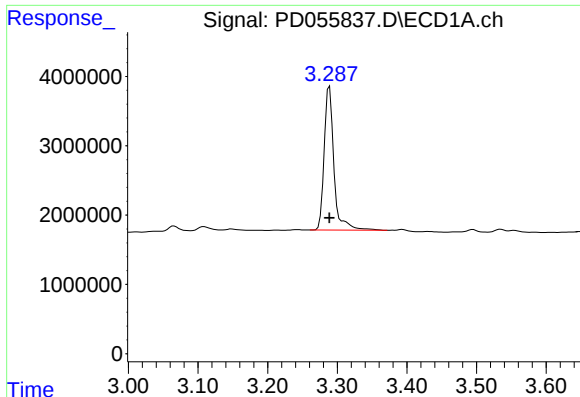

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 20229122
Conc: 26.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AG7

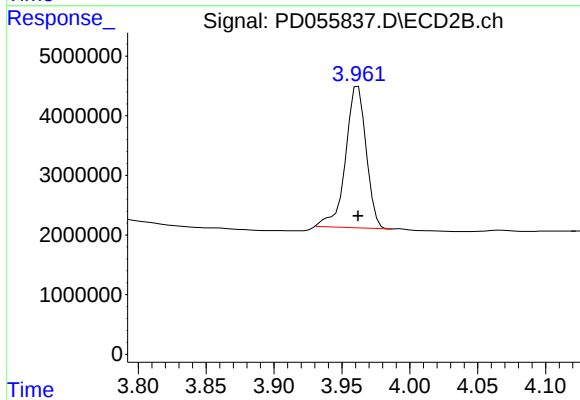


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 25003079
Conc: 23.86 ng/ml

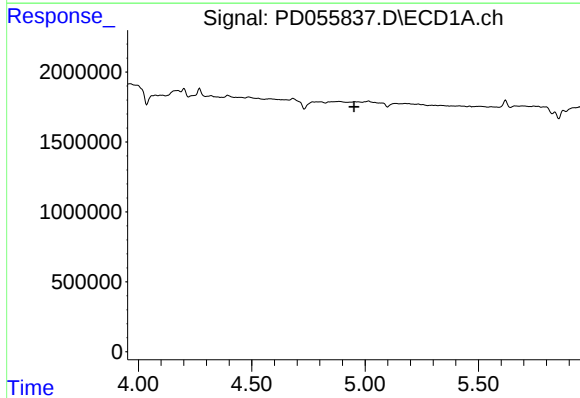


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

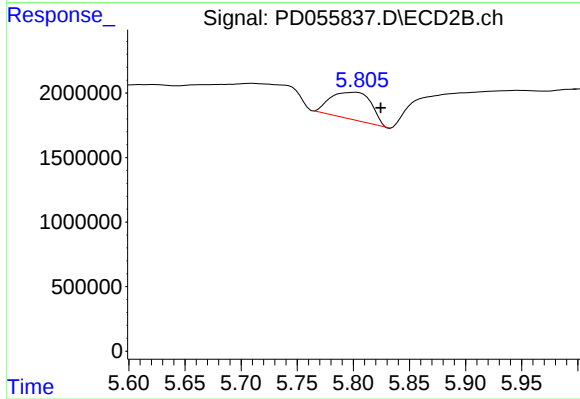

#8 Heptachlor epoxide


R.T.: 5.803 min
Delta R.T.: -0.022 min
Response: 5343513
Conc: 3.96 ng/ml

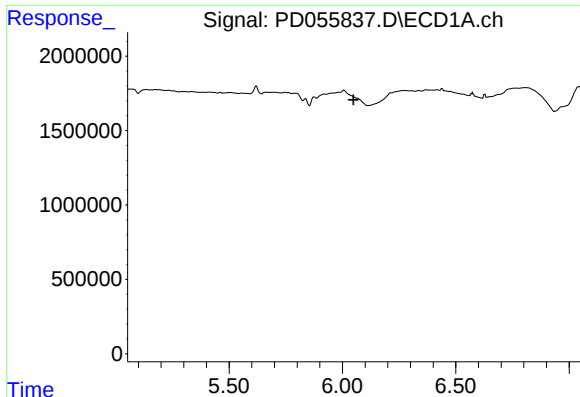

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C5AG7

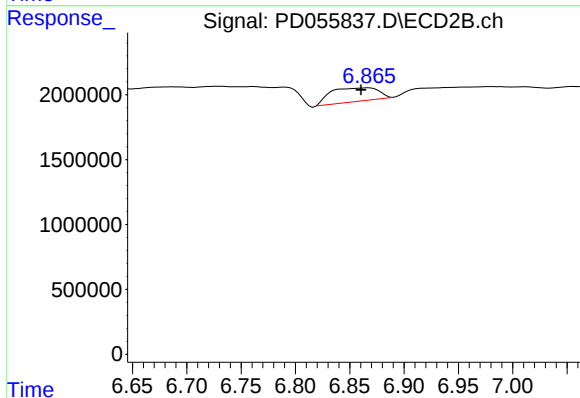


#15 Endosulfan II

R.T.: 6.868 min
Delta R.T.: 0.007 min
Response: 3197642
Conc: 2.47 ng/ml

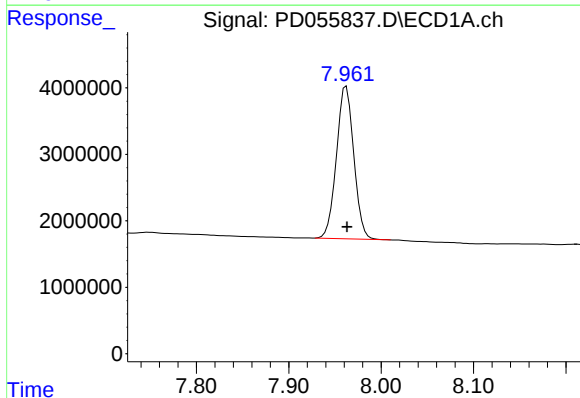

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: 0.000 min
Response: 29906296
Conc: 36.69 ng/ml

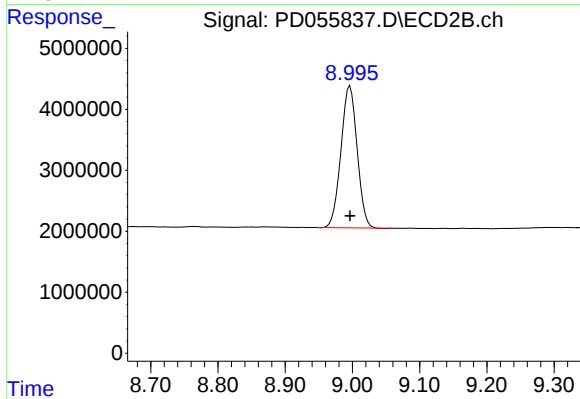

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 38770184
Conc: 34.14 ng/ml