

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110420\
Data File : PD060077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2020 10:30
Operator : DD\AJ
Sample : INDA314
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA314

Manual Integrations
APPROVED

Ankita
11/5/2020 11:26:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:45:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

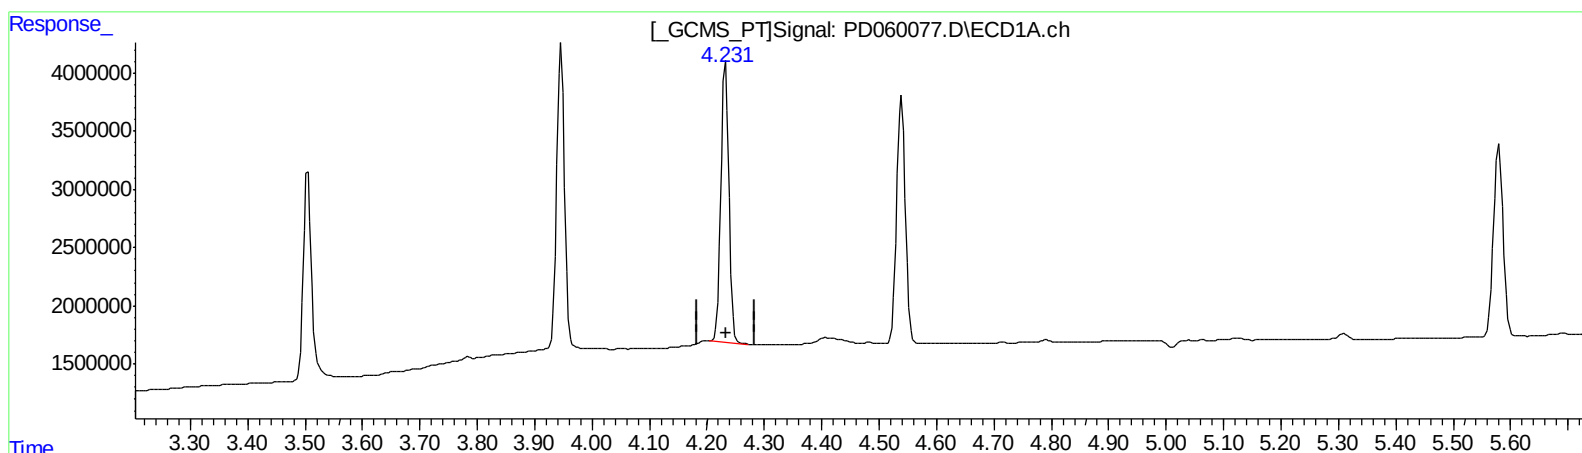

(3) gamma-BHC (Lindane) (MA)

4.233min 19.067 ng/ml

response 23306443

(3) gamma-BHC (Lindane) #2 (MA)

4.699min 17.550 ng/ml

response 71028048

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110420\
Data File : PD060077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2020 10:30
Operator : DD\AJ
Sample : INDA314
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA314

Manual Integrations
APPROVED

Ankita
11/5/2020 11:26:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:45:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

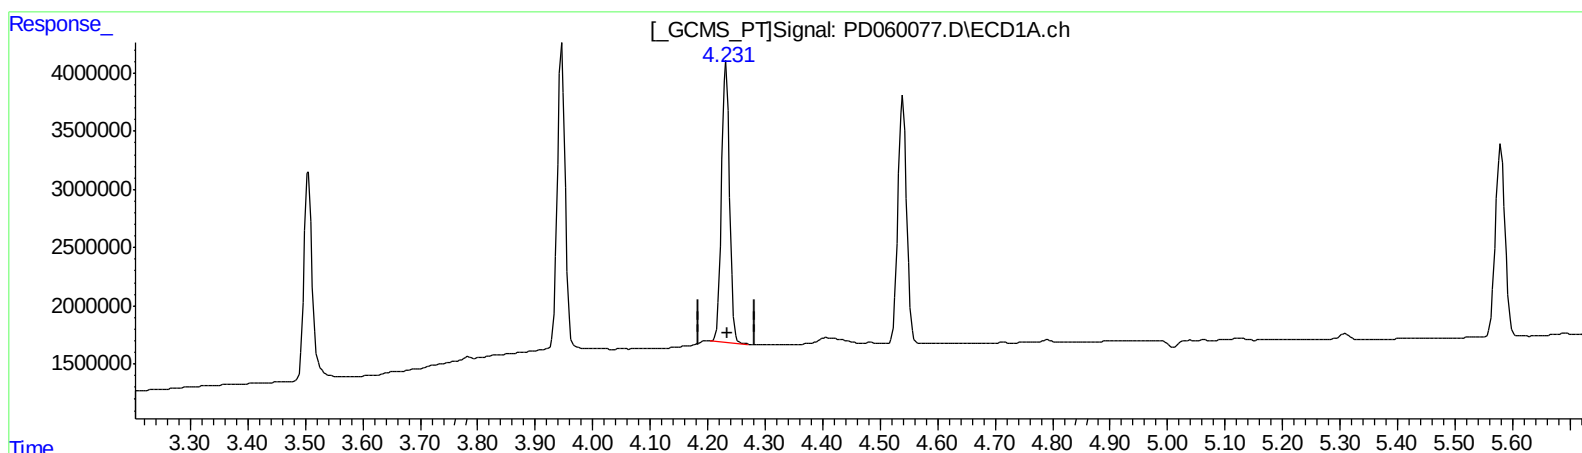

(3) gamma-BHC (Lindane) (MA)

4.233min 19.067 ng/ml

response 23306443

(3) gamma-BHC (Lindane) #2 (MA)

4.698min 19.931 ng/ml m

response 80662669

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110420\
 Data File : PD060077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2020 10:30
 Operator : DD\AJ
 Sample : INDA314
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA314

Manual Integrations
 APPROVED

Ankita
 11/5/2020 11:26:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:45:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.505	4.023	17393641	61527031	20.297	20.640
27) SA Decachlor...	8.301	9.105	30785332	92731714	37.051	37.695
Target Compounds						
2) A alpha-BHC	3.946	4.413	24801511	86761633	19.298	19.478
3) MA gamma-BHC...	4.233	4.698	23306443	80662669	19.067	19.931m
4) MA Heptachlor	4.539	5.210	22545770	77740208	19.209	19.608
9) A Endosulfan I	5.580	6.261	19463837	63576204	19.136	19.836
13) MA Dieldrin	5.826	6.518	41305194	138.0E6	37.910	39.534
14) MA Endrin	6.084	6.736	33868423	104.5E6	37.542	37.335
16) A 4,4'-DDD	6.209	6.855	33342661	107.1E6	37.703	39.905
17) MA 4,4'-DDT	6.453	7.155	33419121	104.9E6	37.183	38.549
20) A Methoxychlor	7.000	7.612	79207949	273.6E6	186.123	194.629

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 11/5/20