

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
 Data File : PD079394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 13:38
 Operator : AR\AJ
 Sample : 04922-10MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAS3MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/03/2023
 Supervised By : mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 21:38:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.800	16750429	23067012	10.922	10.637
27)	SA Decachlor...	9.117	7.950	18851964	17588161	9.939	7.541
Target Compounds							
2)	A alpha-BHC	4.029	3.304	92678980	145.4E6	35.570m	42.642
3)	MA gamma-BHC...	4.363	3.634	81134504	130.5E6	32.599	40.380
4)	MA Heptachlor	4.957	3.977	96736208	135.6E6	36.310	44.596
5)	MB Aldrin	5.300	4.258	92689418	134.3E6	37.490	43.604
6)	B beta-BHC	4.557	3.929	37798275	57027323	33.148	39.429
7)	B delta-BHC	4.806	4.160	68210274	94294915	25.999	28.754
8)	B Heptachlo...	5.727	4.760	81303742	112.3E6	33.856	38.919
9)	A Endosulfan I	6.112	5.131	71244835	103.2E6	33.257	40.636
10)	B trans-Chl...	5.982	5.010	75191992	111.2E6	33.945	40.143
11)	B cis-Chlor...	6.062	5.075	74658555	110.8E6	32.844	39.130
12)	B 4,4'-DDE	6.233	5.263	138.9E6	218.3E6	67.425	83.477m
13)	MA Dieldrin	6.388	5.396	148.9E6	227.6E6	65.532	77.270
14)	MA Endrin	6.618	5.671	127.6E6	202.9E6	67.412	80.423
15)	B Endosulfa...	6.835	5.962	125.3E6	181.3E6	63.213	76.178m
16)	A 4,4'-DDD	6.749	5.818	109.6E6	167.4E6	65.229	75.780
17)	MA 4,4'-DDT	7.064	6.070	118.2E6	167.2E6	66.012	74.193
18)	B Endrin al...	6.965	6.142	89132660	128.3E6	58.766	69.213m
19)	B Endosulfa...	7.200	6.364	109.9E6	158.3E6	57.194	68.667m
20)	A Methoxychlor	7.538	6.645	318.7E6	431.2E6	332.227	353.666
21)	B Endrin ke...	7.686	6.872	131.3E6	181.7E6	62.822	68.832

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 13:38
Operator : AR\AJ
Sample : 04922-10MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:38:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

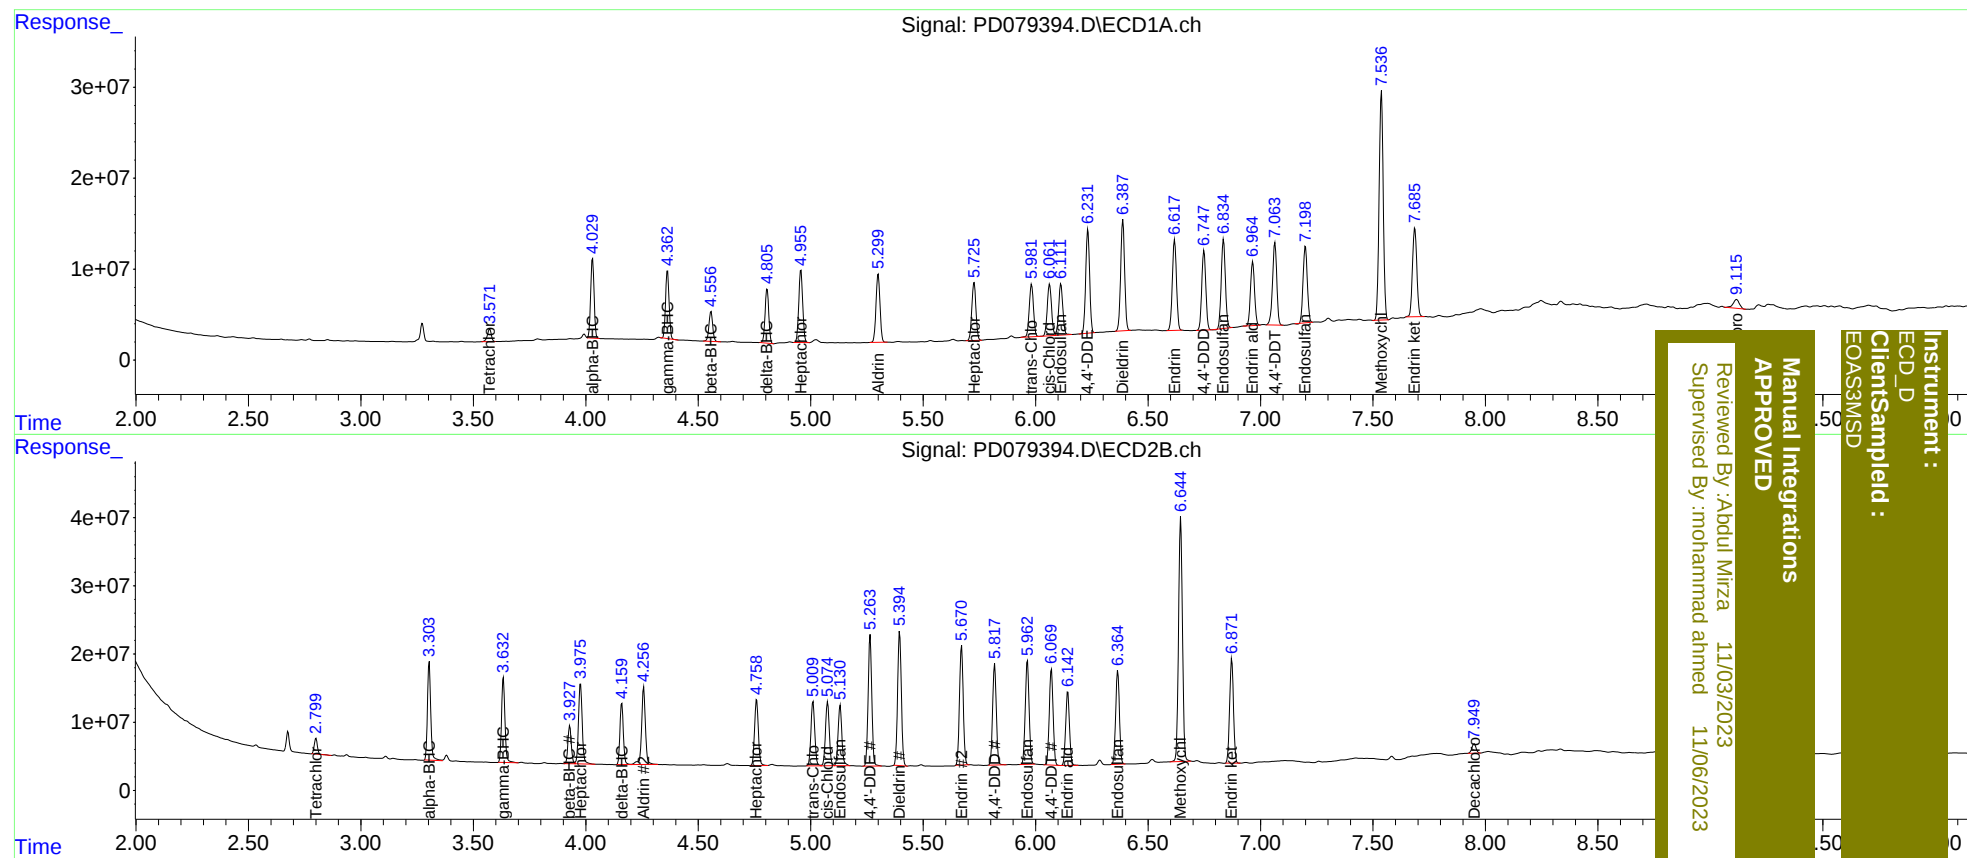

Instrument :
ECD_D
ClientSampled :
EOASMSD
Manual Integrations
APPROVED
Reviewed By: Abdul Miza 11/03/2023
Supervised By: mohammad ahmed 11/06/2023