

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110423\  
Data File : PD079388.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Nov 2023 11:18  
Operator : AR\AJ  
Sample : 04922-01  
Misc :  
ALS Vial : 6 Sample Multiplier: 1


Instrument :  
ECD\_D  
ClientSampleId :  
EOAQ3

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/06/2023  
Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 02 21:30:04 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101723CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 17 09:38:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

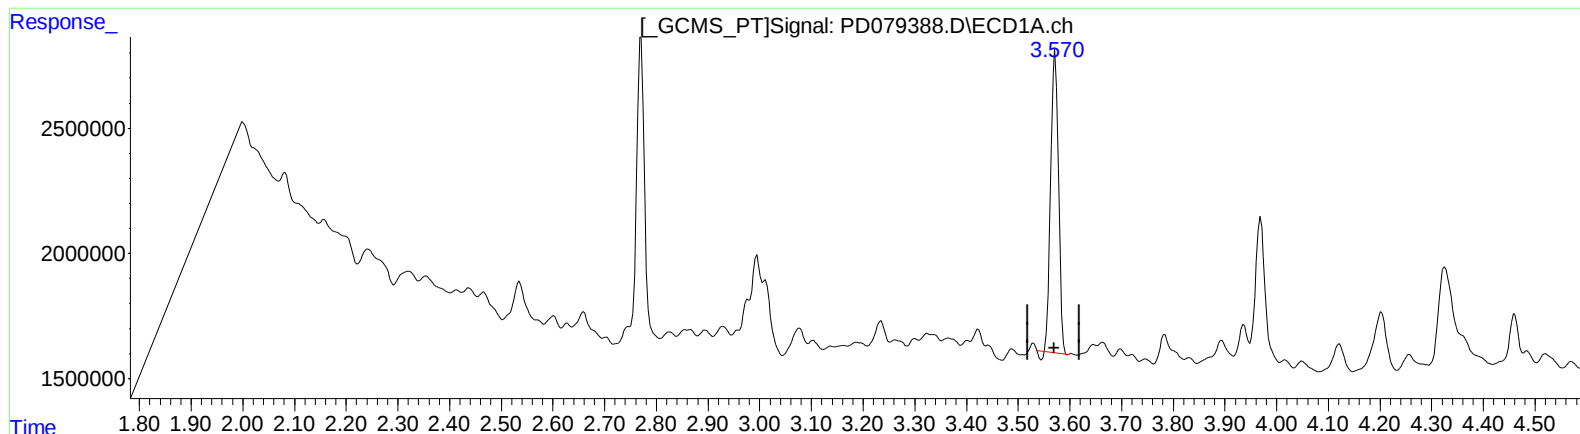

QEdit

(1) Tetrachloro-m-xylene (SA)

3.572min 8.204 ng/ml

response 12581810

(1) Tetrachloro-m-xylene #2 (SA)

2.800min 9.165 ng/ml

response 19873669

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110423\  
Data File : PD079388.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Nov 2023 11:18  
Operator : AR\AJ  
Sample : 04922-01  
Misc :  
ALS Vial : 6 Sample Multiplier: 1



Instrument :  
ECD\_D  
ClientSampleId :  
EOAQ3

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/06/2023  
Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 02 21:30:04 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101723CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 17 09:38:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

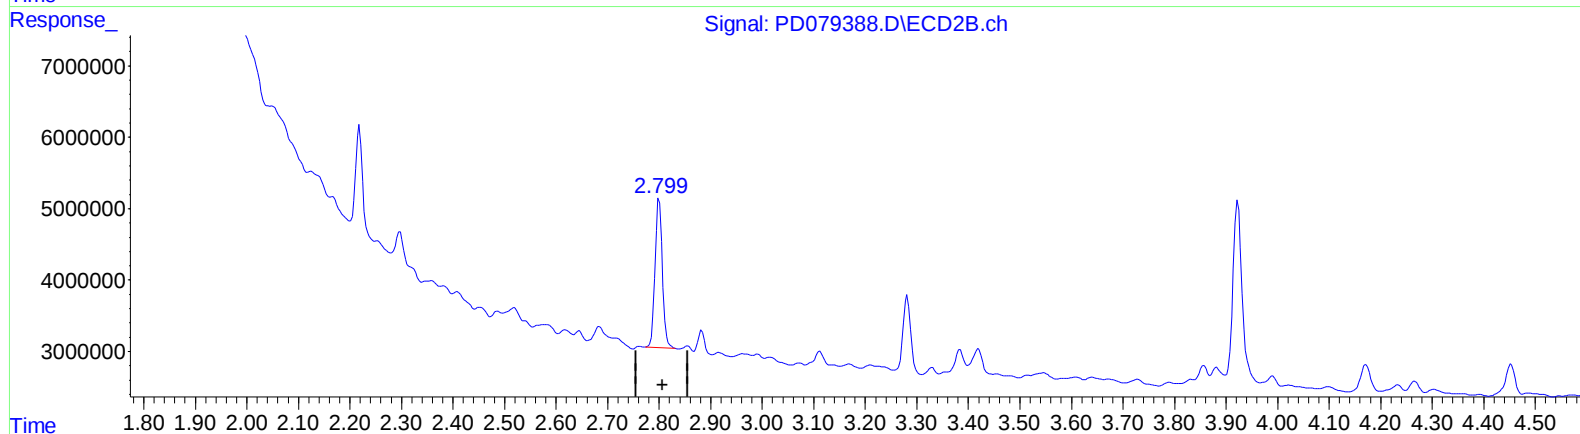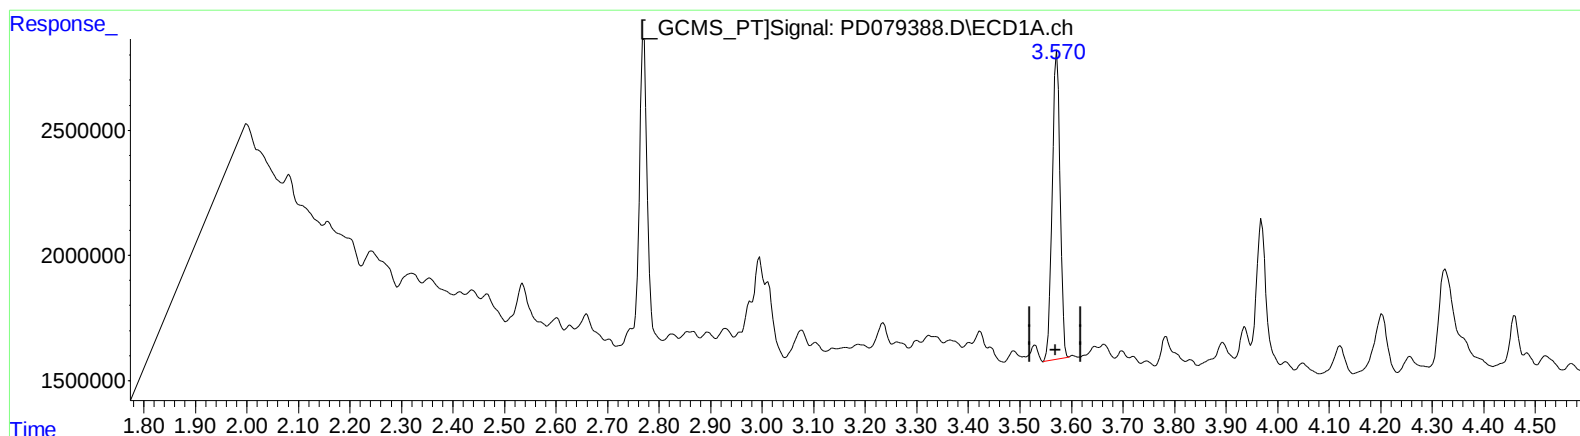

QEdit

(1) Tetrachloro-m-xylene (SA)

3.570min 8.595 ng/ml m

response 13181406

(1) Tetrachloro-m-xylene #2 (SA)

2.799min 9.604 ng/ml m

response 20827598

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110423\  
Data File : PD079388.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Nov 2023 11:18  
Operator : AR\AJ  
Sample : 04922-01  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

## Instrument :

ECD\_D

ClientSampleId :

EOAQ3



## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/06/2023

Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 02 21:30:04 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101723CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 17 09:38:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

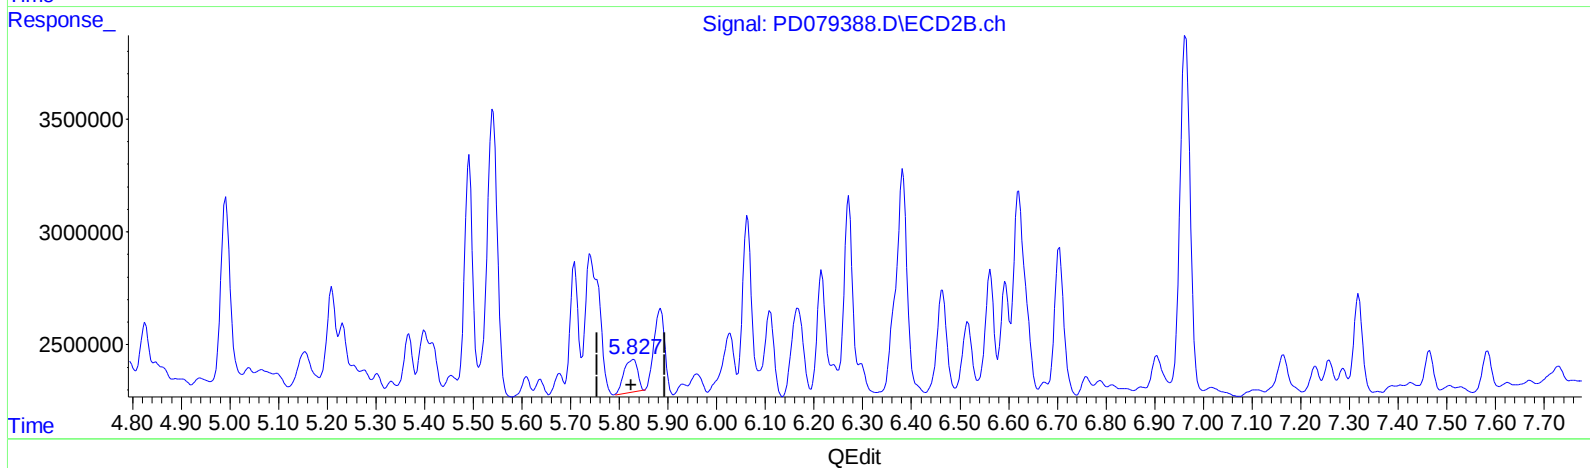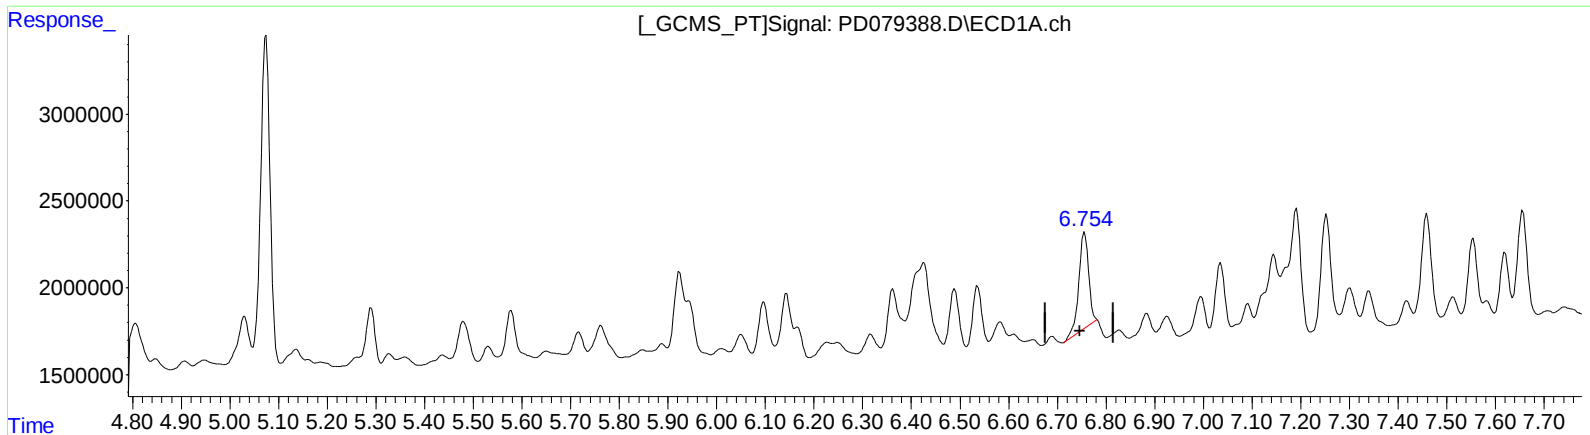

(16) 4,4'-DDD (A)

6.756min 4.724 ng/ml

response 7940398

(16) 4,4'-DDD #2 (A)

5.829min 1.281 ng/ml

response 2830035

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110423\  
Data File : PD079388.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Nov 2023 11:18  
Operator : AR\AJ  
Sample : 04922-01  
Misc :  
ALS Vial : 6 Sample Multiplier: 1


Instrument :  
ECD\_D  
ClientSampleId :  
EOAQ3

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/06/2023  
Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 02 21:30:04 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101723CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 17 09:38:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

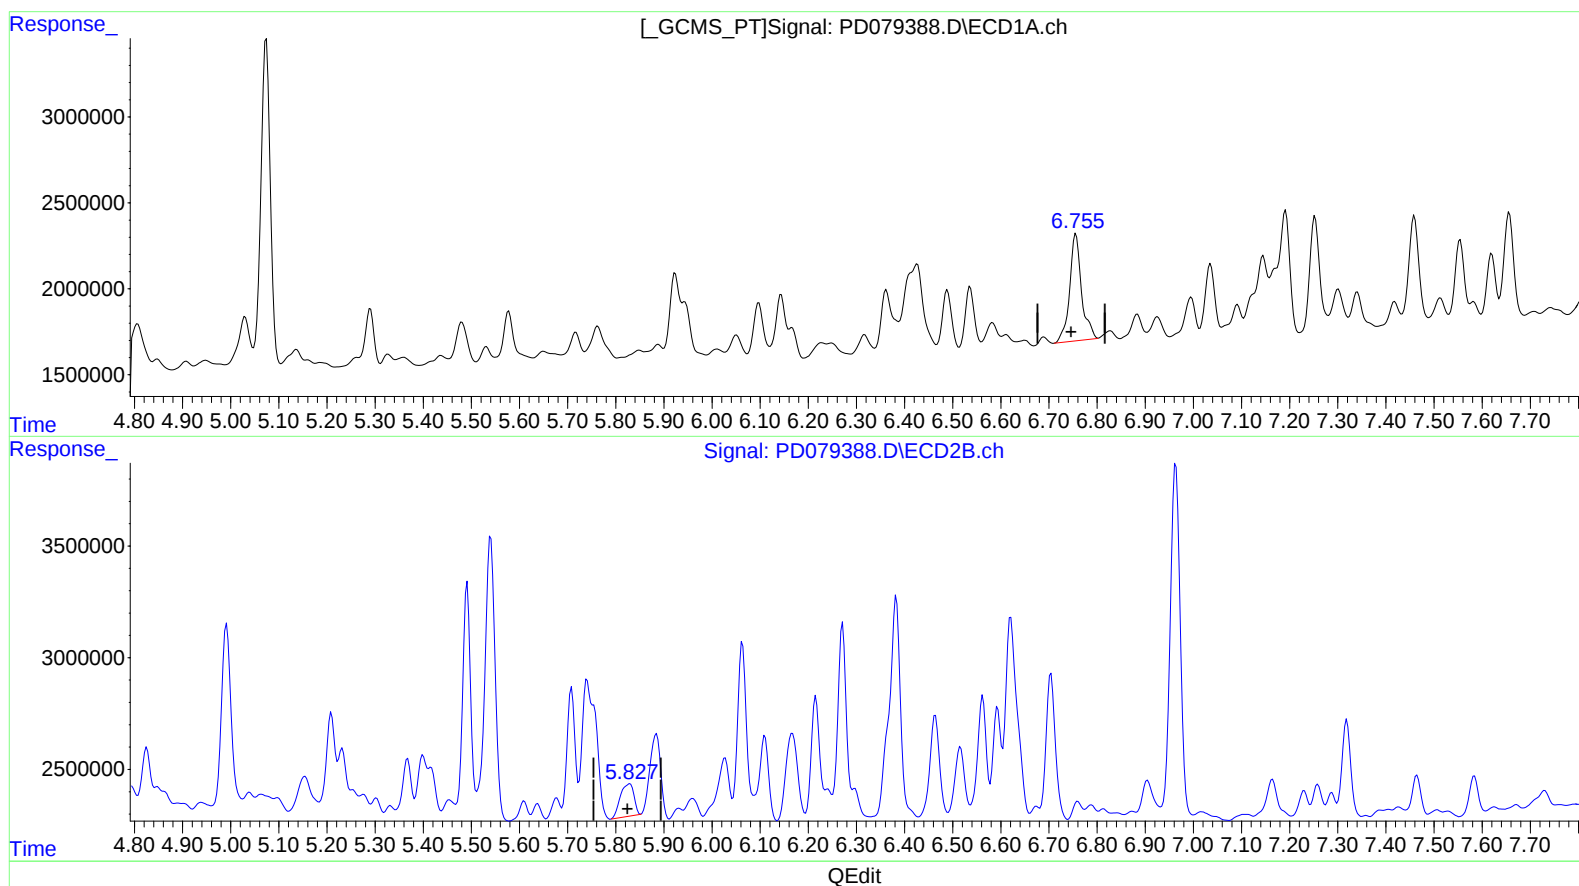

(16) 4,4'-DDD (A)  
6.755min 6.382 ng/ml m  
response 10727576

(16) 4,4'-DDD #2 (A)  
5.829min 1.281 ng/ml  
response 2830035

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110423\  
Data File : PD079388.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Nov 2023 11:18  
Operator : AR\AJ  
Sample : 04922-01  
Misc :  
ALS Vial : 6 Sample Multiplier: 1



Instrument :  
ECD\_D  
ClientSampleId :  
EOAQ3

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/06/2023  
Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 02 21:30:04 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101723CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 17 09:38:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

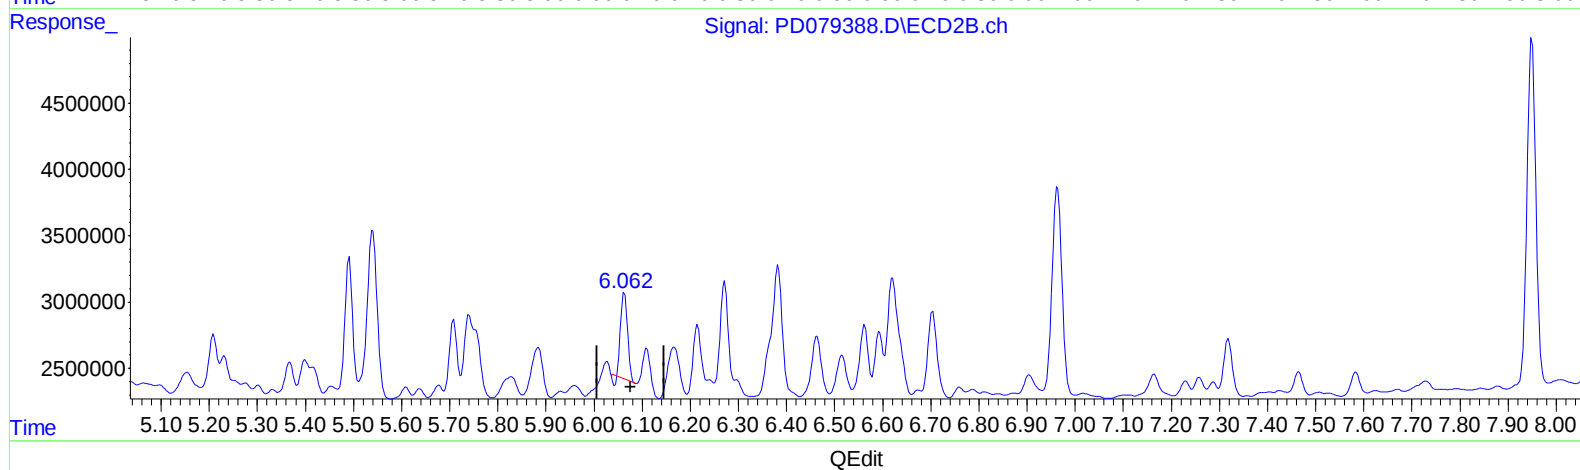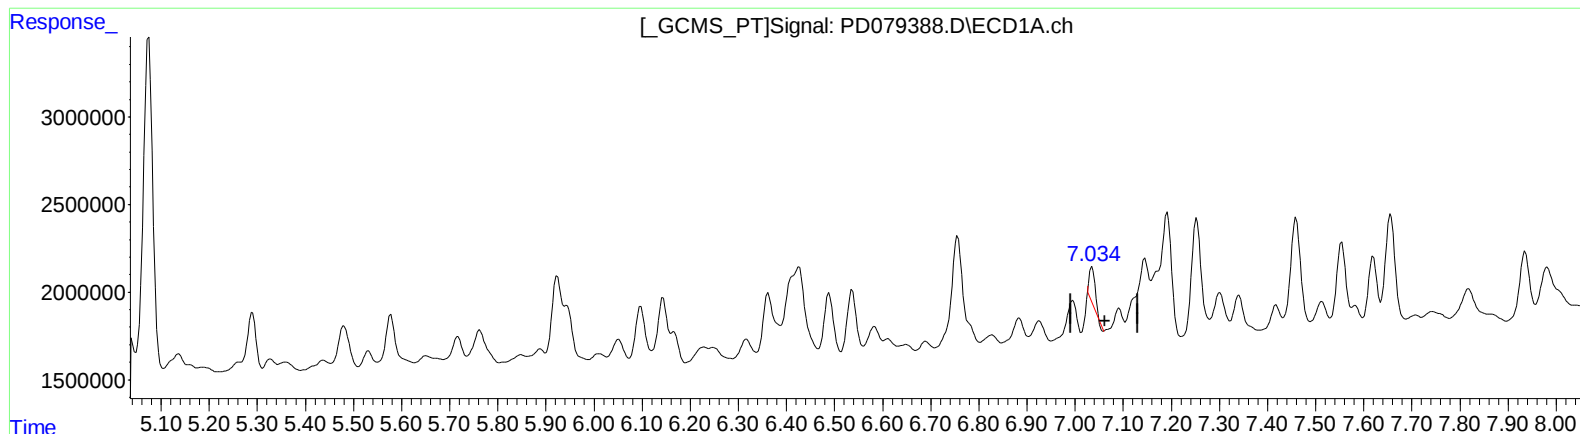

QEdit

(17) 4,4'-DDT (MA)

7.035min 0.953 ng/ml

response 1706285

(17) 4,4'-DDT #2 (MA)

6.063min 2.820 ng/ml

response 6353903

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110423\  
Data File : PD079388.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Nov 2023 11:18  
Operator : AR\AJ  
Sample : 04922-01  
Misc :  
ALS Vial : 6 Sample Multiplier: 1


Instrument :  
ECD\_D  
ClientSampleId :  
EOAQ3

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/06/2023  
Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 02 21:30:04 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101723CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 17 09:38:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

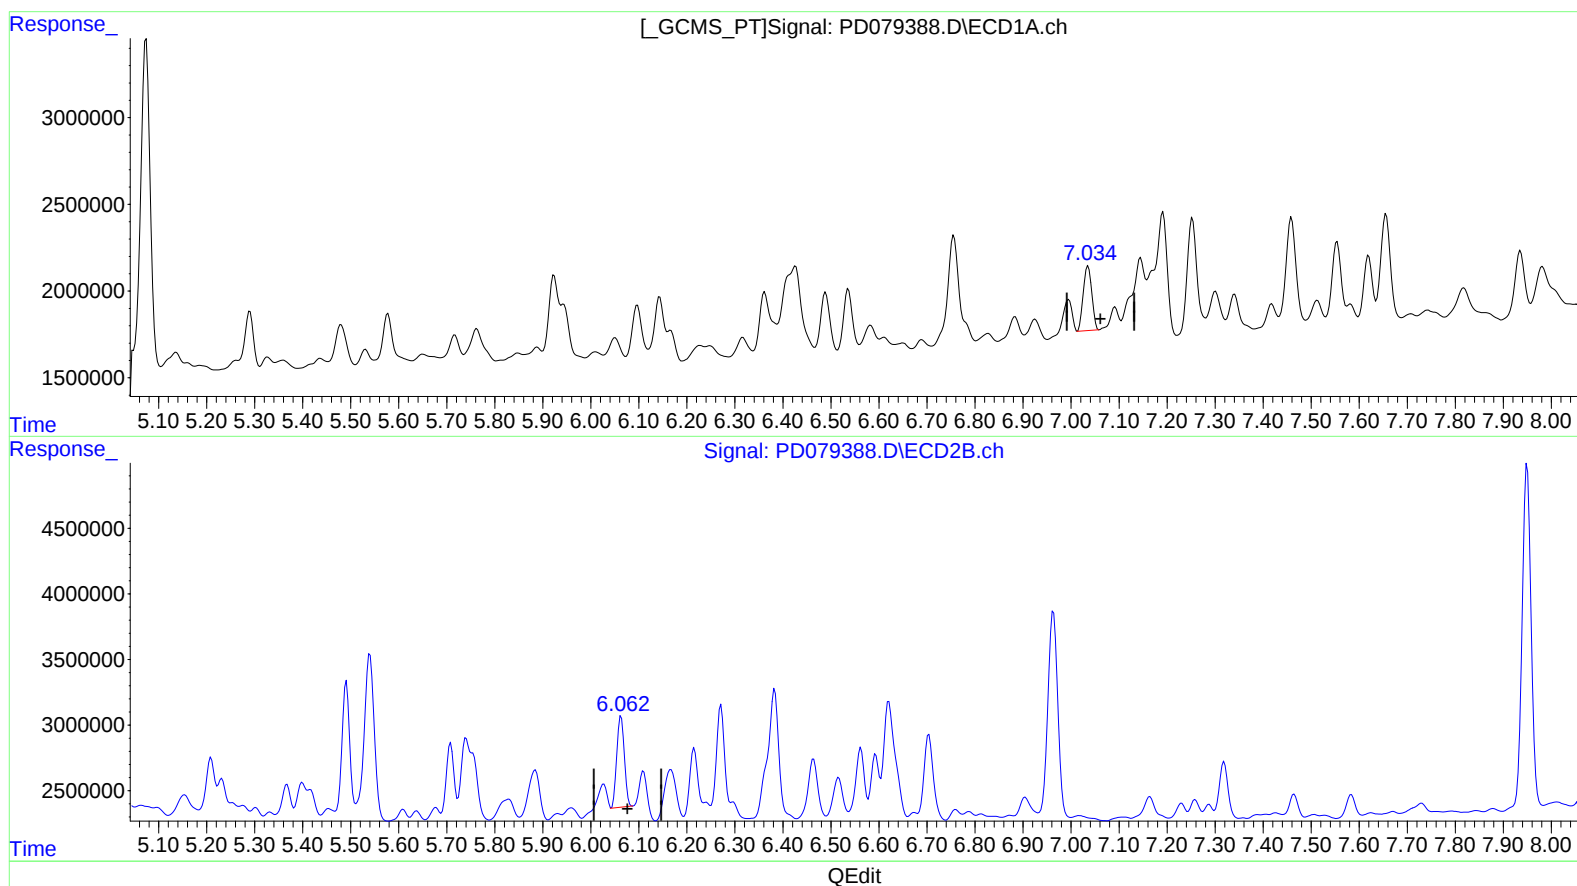

(17) 4,4'-DDT (MA)

7.034min 2.578 ng/ml m

response 4615751

(17) 4,4'-DDT #2 (MA)

6.062min 3.375 ng/ml m

response 7604194

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110423\  
Data File : PD079388.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Nov 2023 11:18  
Operator : AR\AJ  
Sample : 04922-01  
Misc :  
ALS Vial : 6 Sample Multiplier: 1


Instrument :  
ECD\_D  
ClientSampleId :  
EOAQ3

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/06/2023  
Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 07 03:39:17 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101723CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 17 09:38:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

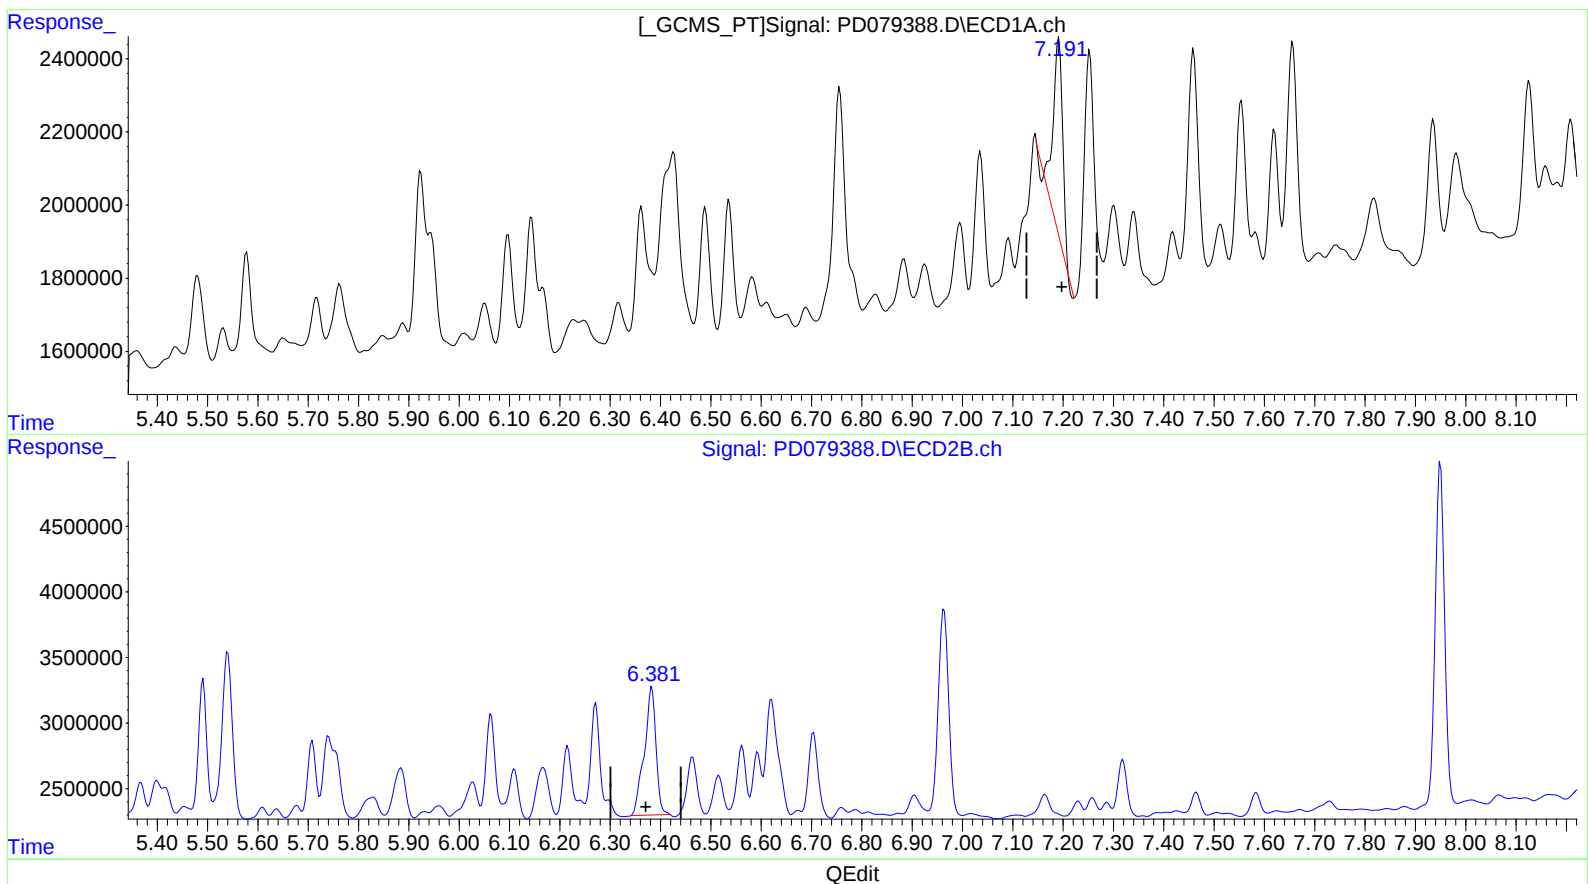

(19) Endosulfan Sulfate (B)

7.191min 3.630 ng/ml

response 6975148

(19) Endosulfan Sulfate #2 (B)

6.383min 6.812 ng/ml

response 15699752

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110423\  
Data File : PD079388.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Nov 2023 11:18  
Operator : AR\AJ  
Sample : 04922-01  
Misc :  
ALS Vial : 6 Sample Multiplier: 1


Instrument :  
ECD\_D  
ClientSampleId :  
EOAQ3

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/06/2023  
Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 02 21:30:04 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101723CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 17 09:38:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

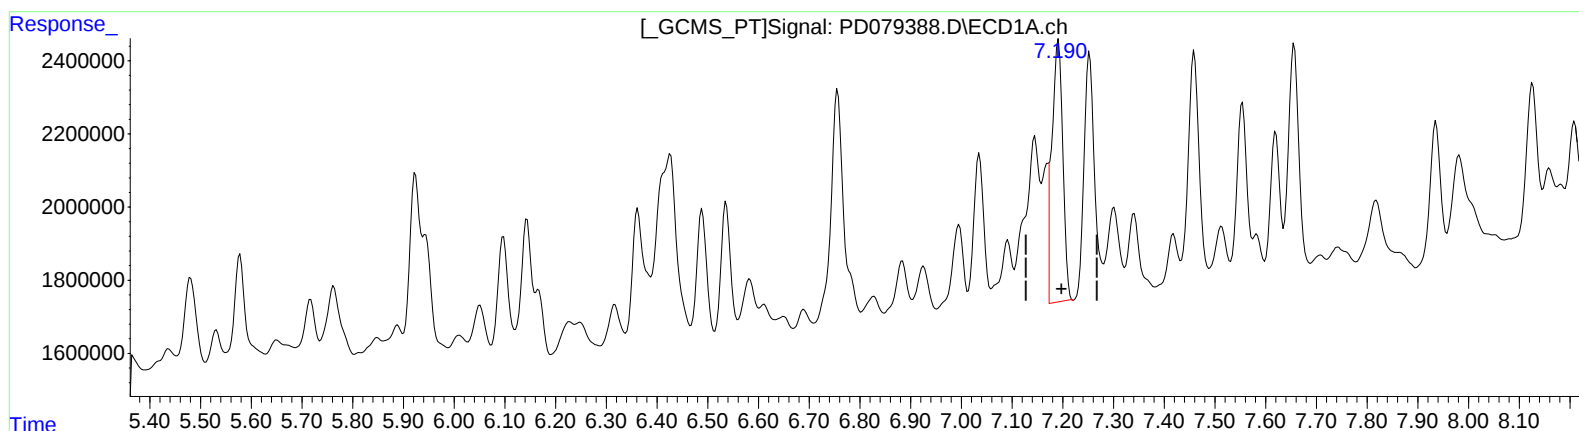

(19) Endosulfan Sulfate (B)

7.190min 5.443 ng/ml m

response 10460043

(19) Endosulfan Sulfate #2 (B)

6.381min 5.856 ng/ml m

response 13495922