

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 14:44
Operator : AR\AJ
Sample : 04922-15
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
EOAT4

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/03/2023
Supervised By :mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 03:43:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

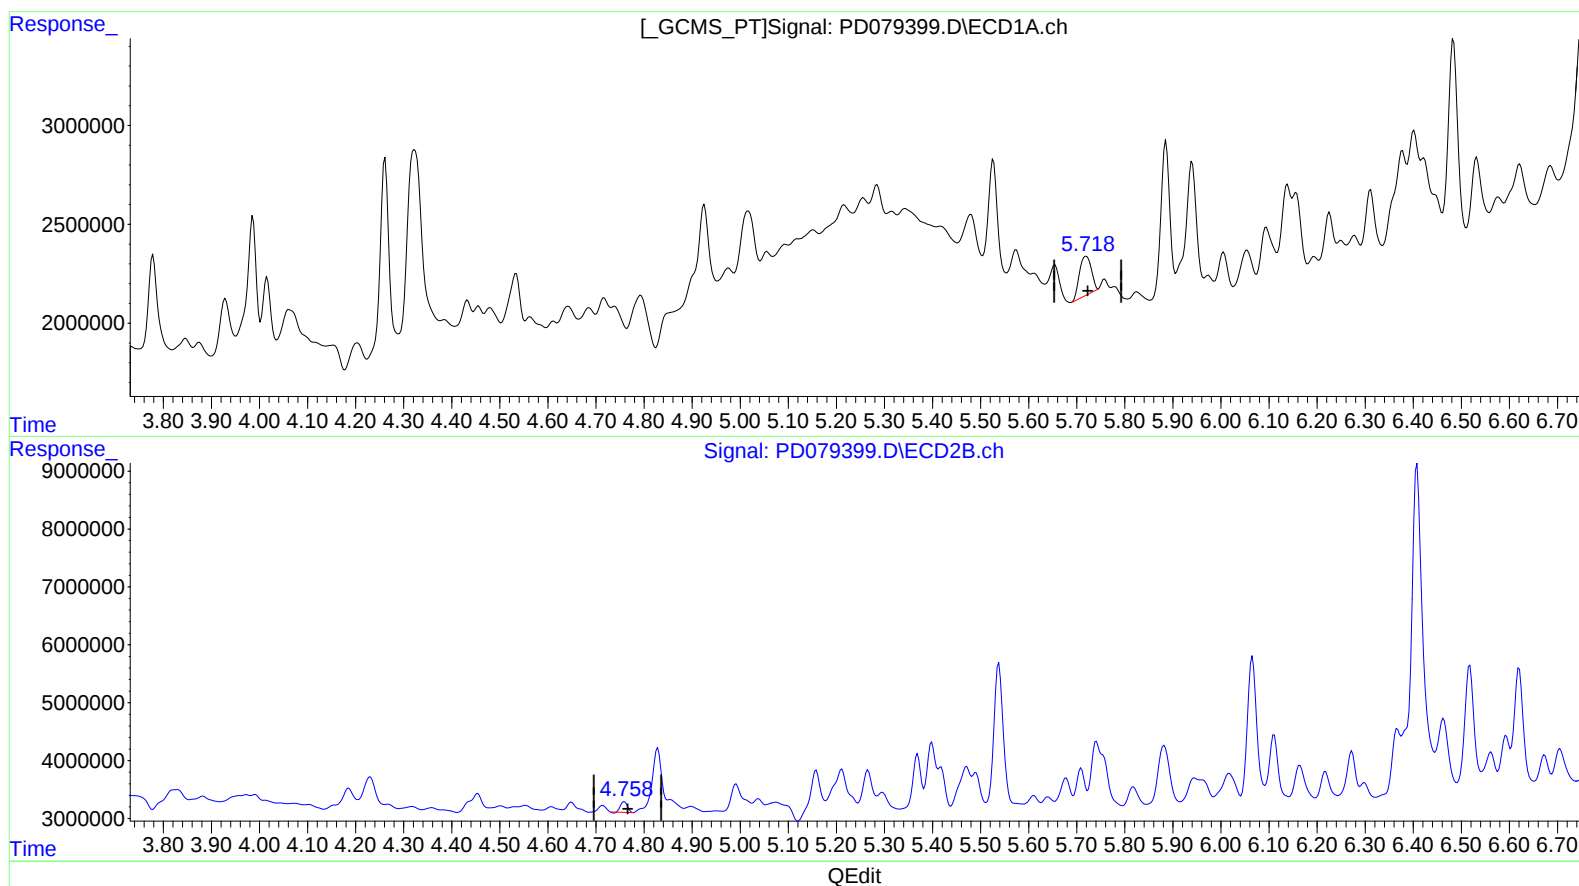

(8) Heptachlor epoxide (B)

5.720min 1.409 ng/ml

response 3383992

(8) Heptachlor epoxide #2 (B)

4.759min 0.629 ng/ml

response 1814561

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 14:44
Operator : AR\AJ
Sample : 04922-15
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
EOAT4

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/03/2023
Supervised By :mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:44:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

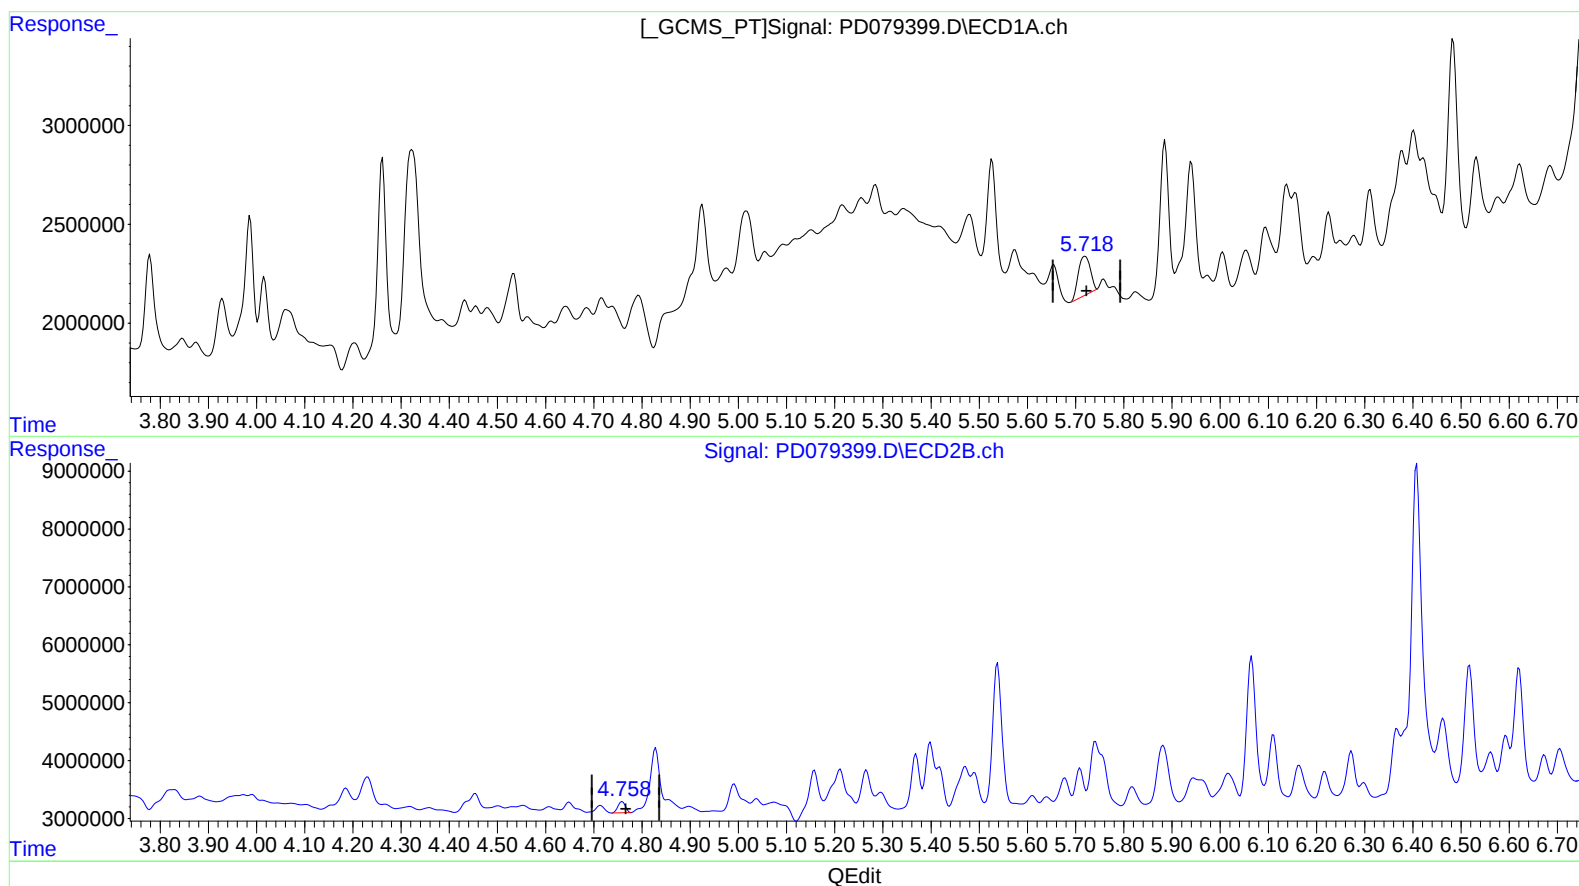

(8) Heptachlor epoxide (B)

5.720min 1.409 ng/ml

response 3383992

(8) Heptachlor epoxide #2 (B)

4.758min 0.711 ng/ml m

response 2050730

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 14:44
Operator : AR\AJ
Sample : 04922-15
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
EOAT4

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/03/2023
Supervised By :mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 03:43:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

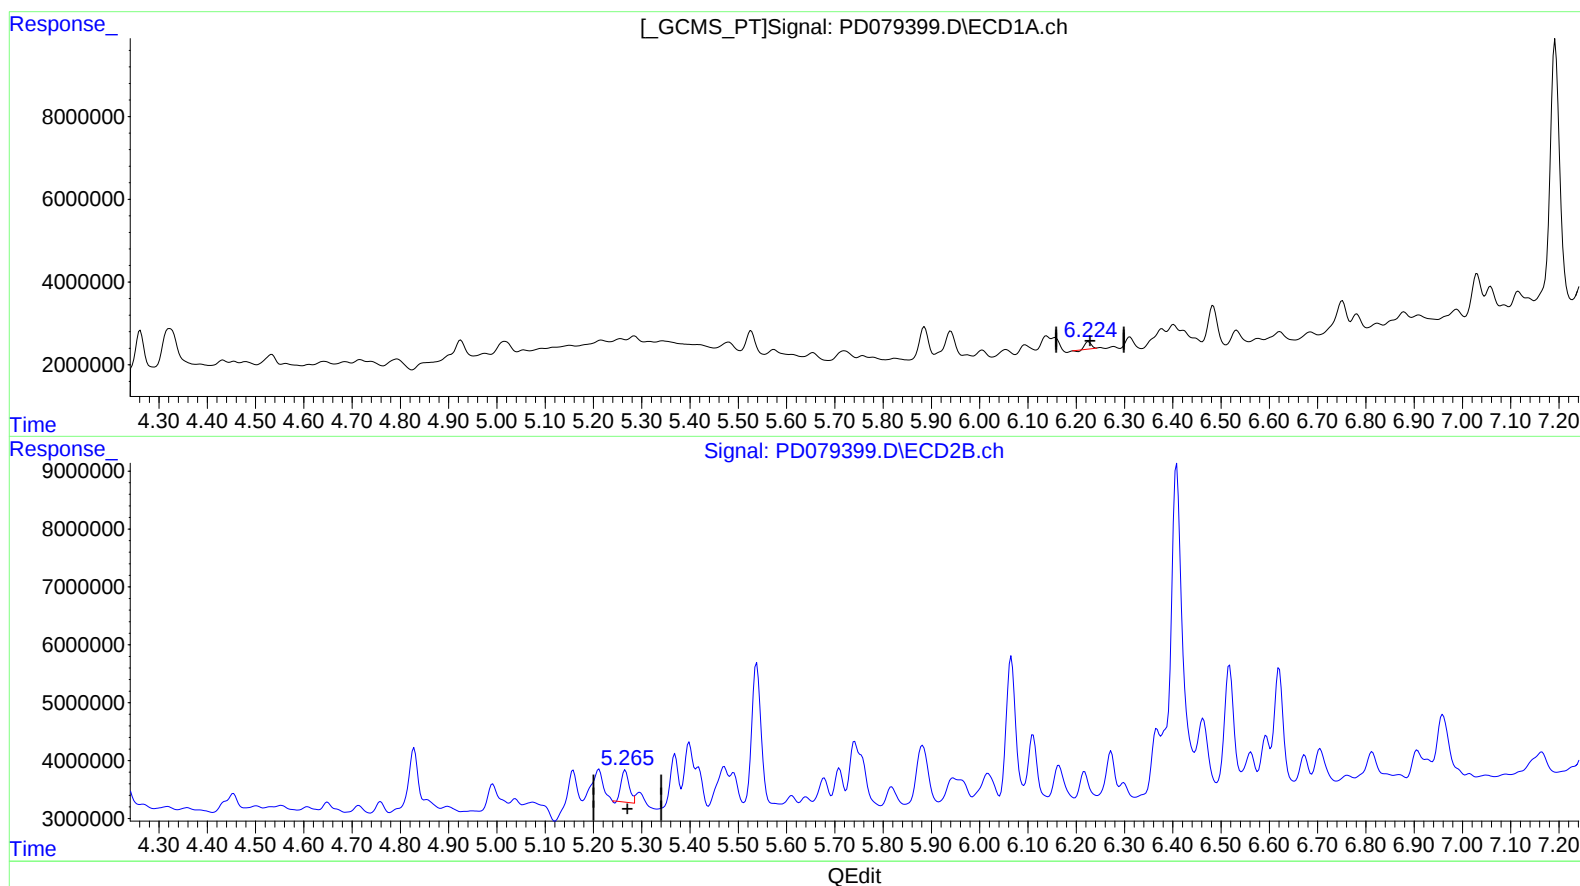

(12) 4,4'-DDE (B)

6.226min 0.692 ng/ml

response 1425897

(12) 4,4'-DDE #2 (B)

5.266min 2.428 ng/ml

response 6349442

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 14:44
Operator : AR\AJ
Sample : 04922-15
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
EOAT4

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/03/2023
Supervised By :mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:44:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

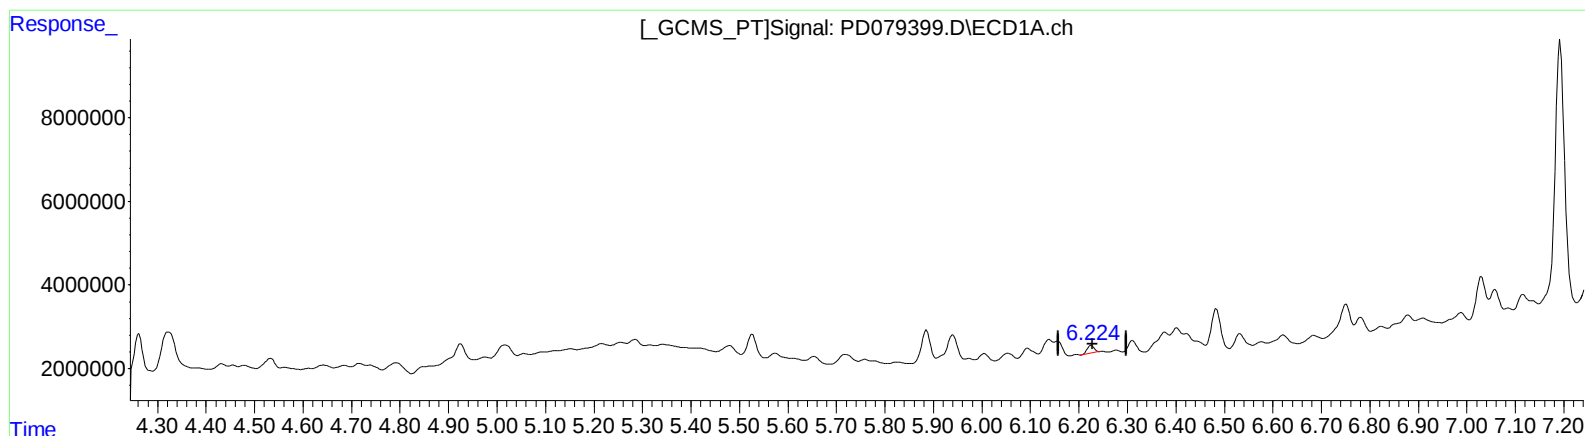

(12) 4,4'-DDE (B)

6.224min 0.900 ng/ml m

response 1854880

(12) 4,4'-DDE #2 (B)

5.265min 2.650 ng/ml m

response 6928498

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
 Data File : PD079399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 14:44
 Operator : AR\AJ
 Sample : 04922-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1



Instrument :
 ECD_D
 ClientSampleId :
 EOAT4

Manual IntegrationsAPPROVED

Reviewed By : Abdul Mirza 11/03/2023
 Supervised By : mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 21:44:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

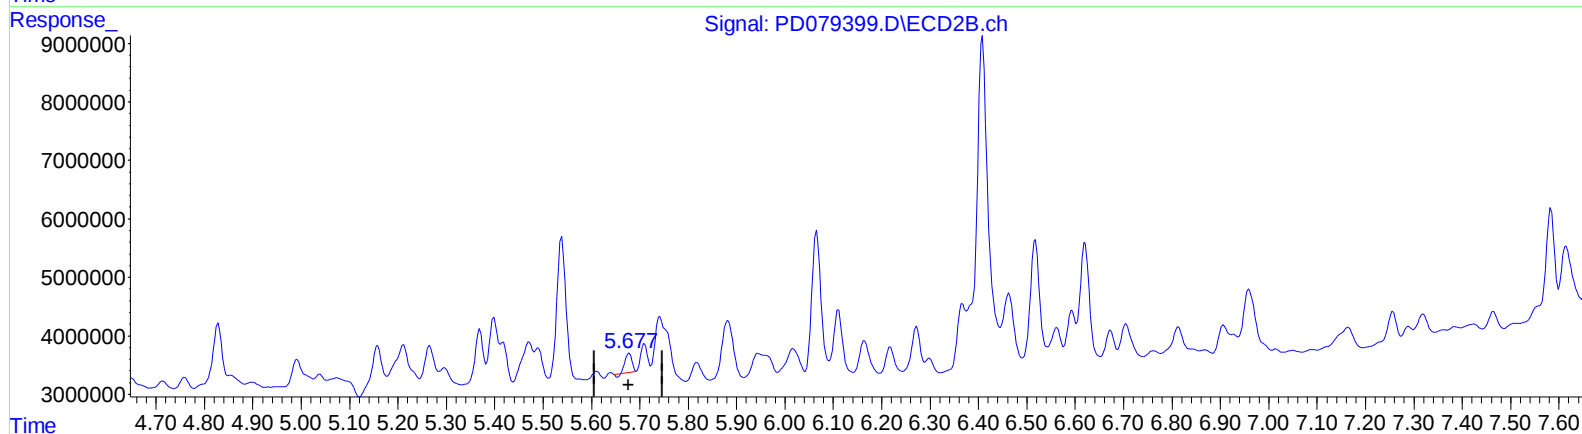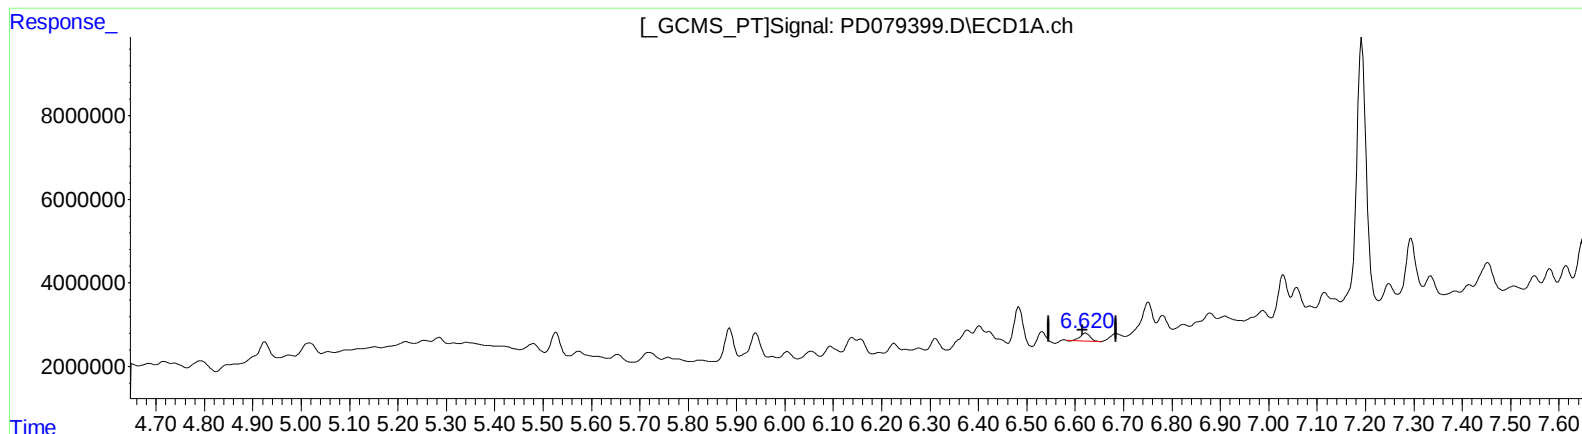

QEdit

(14) Endrin (MA)
 6.622min 1.359 ng/ml
 response 2573704

(14) Endrin #2 (MA)
 5.678min 1.160 ng/ml
 response 2928361

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 14:44
Operator : AR\AJ
Sample : 04922-15
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
EOAT4

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/03/2023
Supervised By :mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:44:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

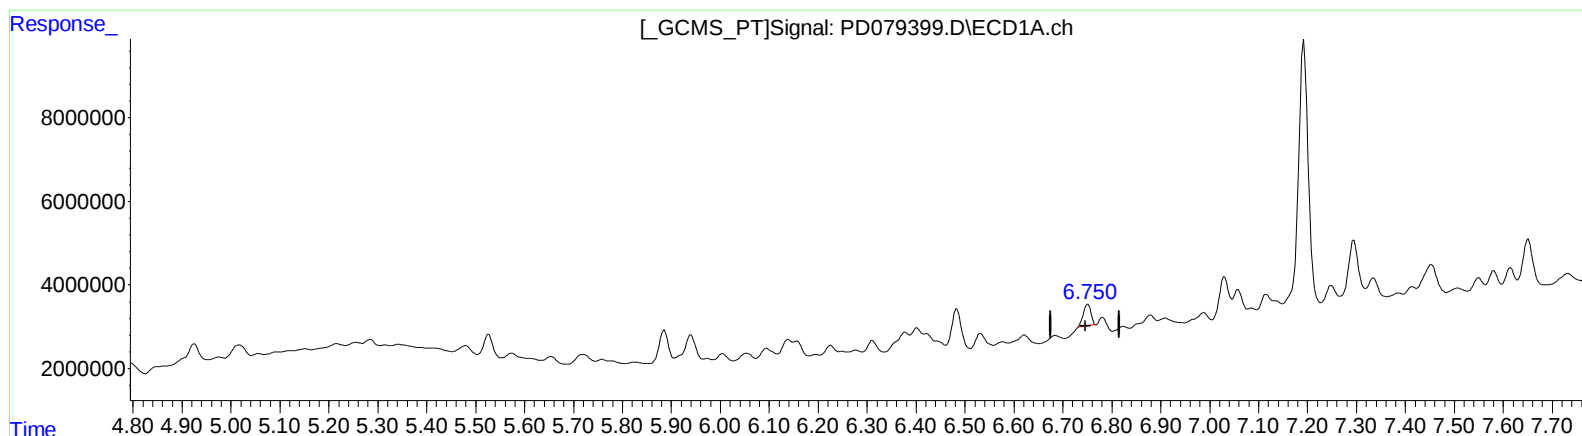

(16) 4,4'-DDD (A)

6.750min 3.375 ng/ml m

response 5673725

(16) 4,4'-DDD #2 (A)

5.817min 1.876 ng/ml m

response 4144556

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 14:44
Operator : AR\AJ
Sample : 04922-15
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
EOAT4

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/03/2023
Supervised By :mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:44:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

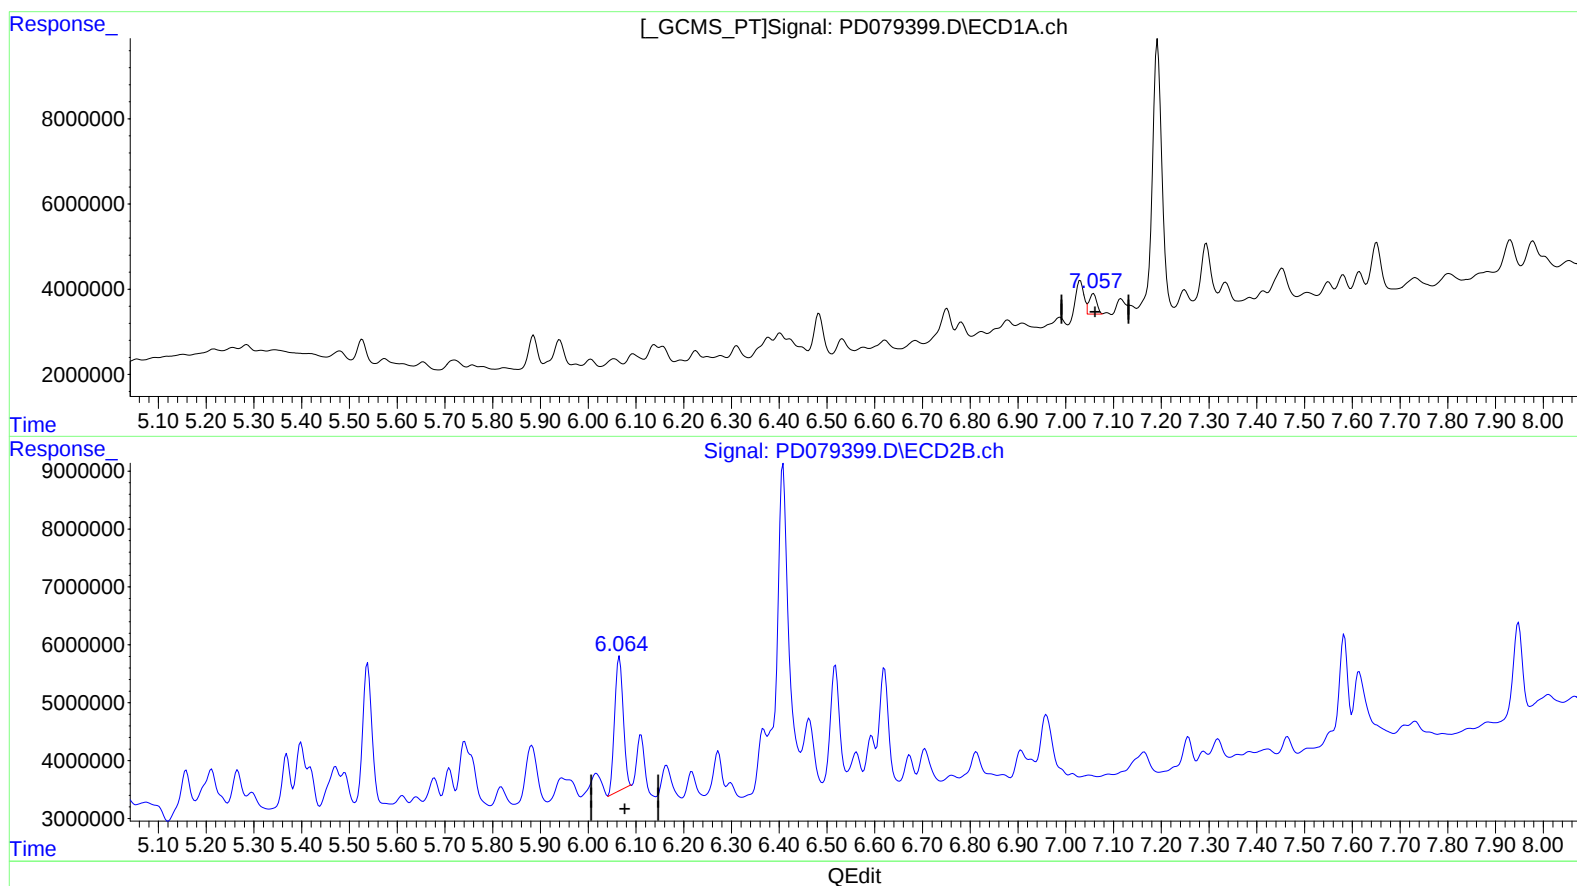

(17) 4,4'-DDT (MA)

7.057min 2.953 ng/ml m

response 5288238

(17) 4,4'-DDT #2 (MA)

6.064min 12.768 ng/ml m

response 28765466