

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
 Data File : PD079389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 11:37
 Operator : AR\AJ
 Sample : 04922-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAQ9

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/03/2023
 Supervised By :mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 21:31:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.580	2.815	12912291	20099948	8.419m	9.269m
2) SA Decachlor...	9.123	7.960	23145807	89109345	12.203m	38.207m#
Target Compounds						
8) B Heptachlo...	5.731	4.767	79811422	299.6E6	33.234m	103.824m#
13) MA Dieldrin	6.370	5.406	256.0E6	174.4E6	112.696	59.201m#
15) B Endosulfa...	6.820	5.977	589.4E6	252.6E6	297.224	106.141 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 11:37
Operator : AR\AJ
Sample : 04922-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:31:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

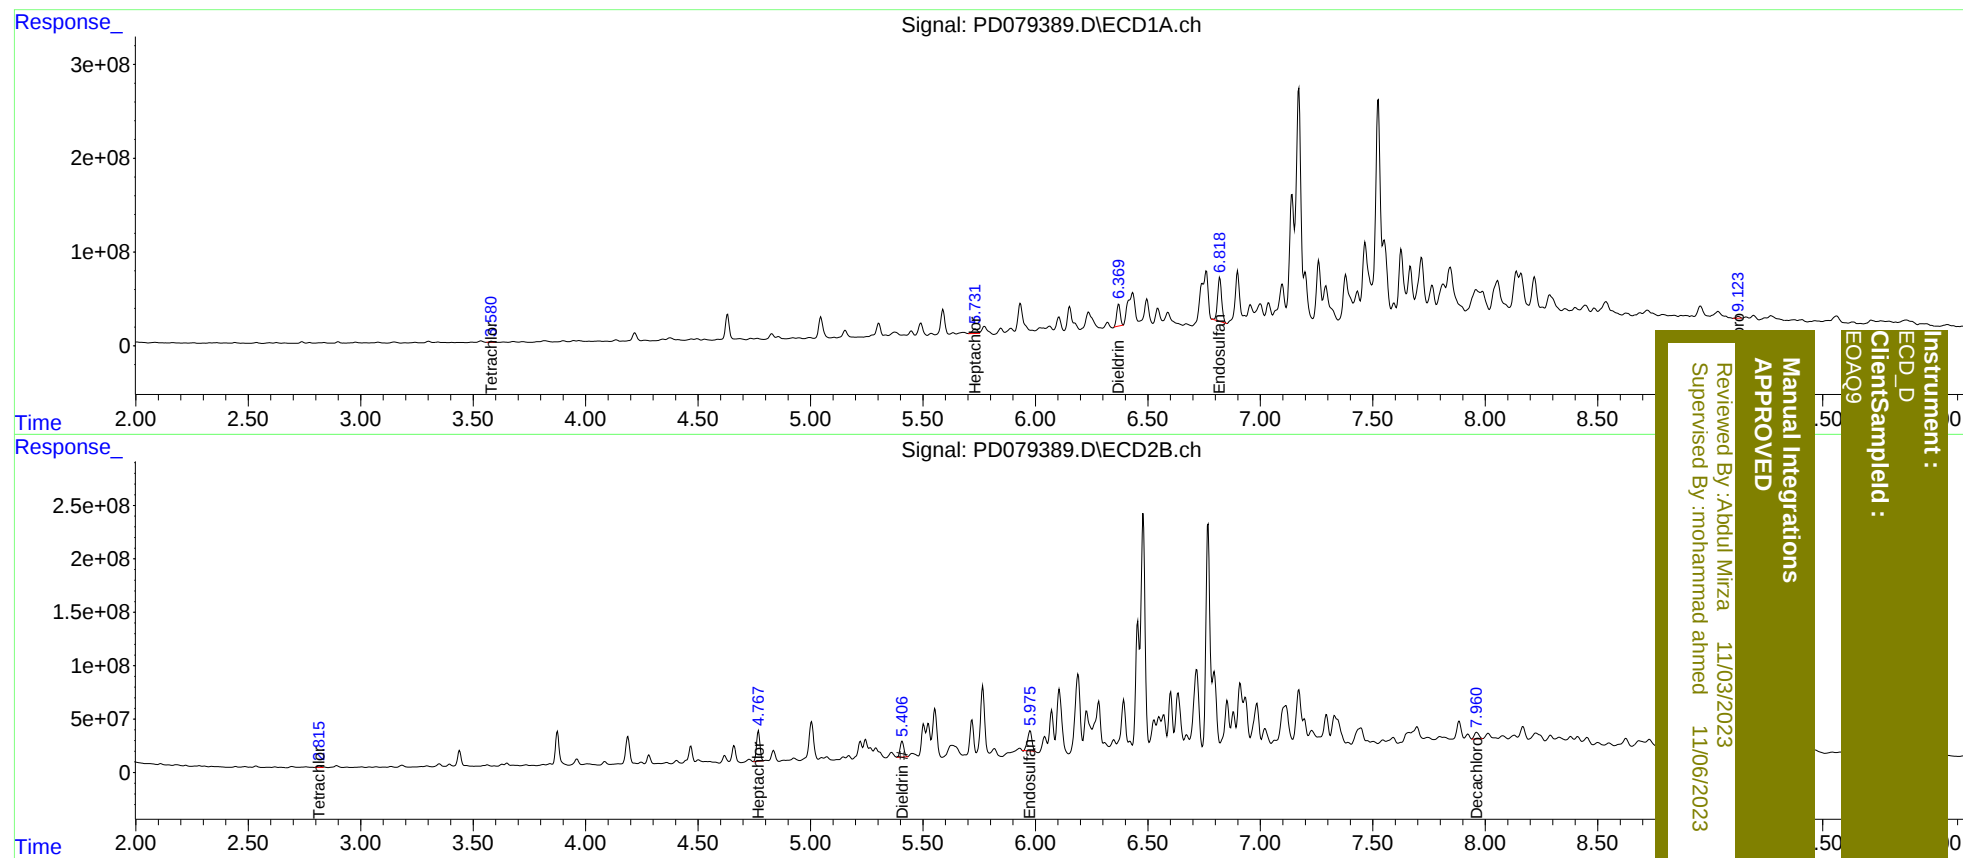

Instrument :
ECD_D
ClientSampled :
EOA09

Manual Integrations
APPROVED

Reviewed By : Abdul Miza 11/03/2023
Supervised By : mohammad ahmed 11/06/2023