

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
 Data File : PD079390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 12:01
 Operator : AR\AJ
 Sample : 04922-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAR2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/03/2023
 Supervised By : mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 21:32:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.803	10636572	19771826	6.935m	9.118 #
27)	SA Decachlor...	9.121	7.948	20349644	35773047	10.729	15.338 #
Target Compounds							
12)	B 4,4'-DDE	6.232	5.267	70009764	44027955	33.986m	16.837 #
13)	MA Dieldrin	6.385	5.399	75895084	87893302	33.408m	29.842m
14)	MA Endrin	6.612	5.678	19239885	42910668	10.162m	17.005m#
15)	B Endosulfa...	6.828	5.963	27864009	32243645	14.052m	13.551m
16)	A 4,4'-DDD	6.758	5.820	272.4E6	109.7E6	162.031m	49.688 #
17)	MA 4,4'-DDT	7.037	6.065	278.2E6	328.3E6	155.397m	145.735m
19)	B Endosulfa...	7.181	6.368	110.9E6	167.6E6	57.698	72.702 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:32:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

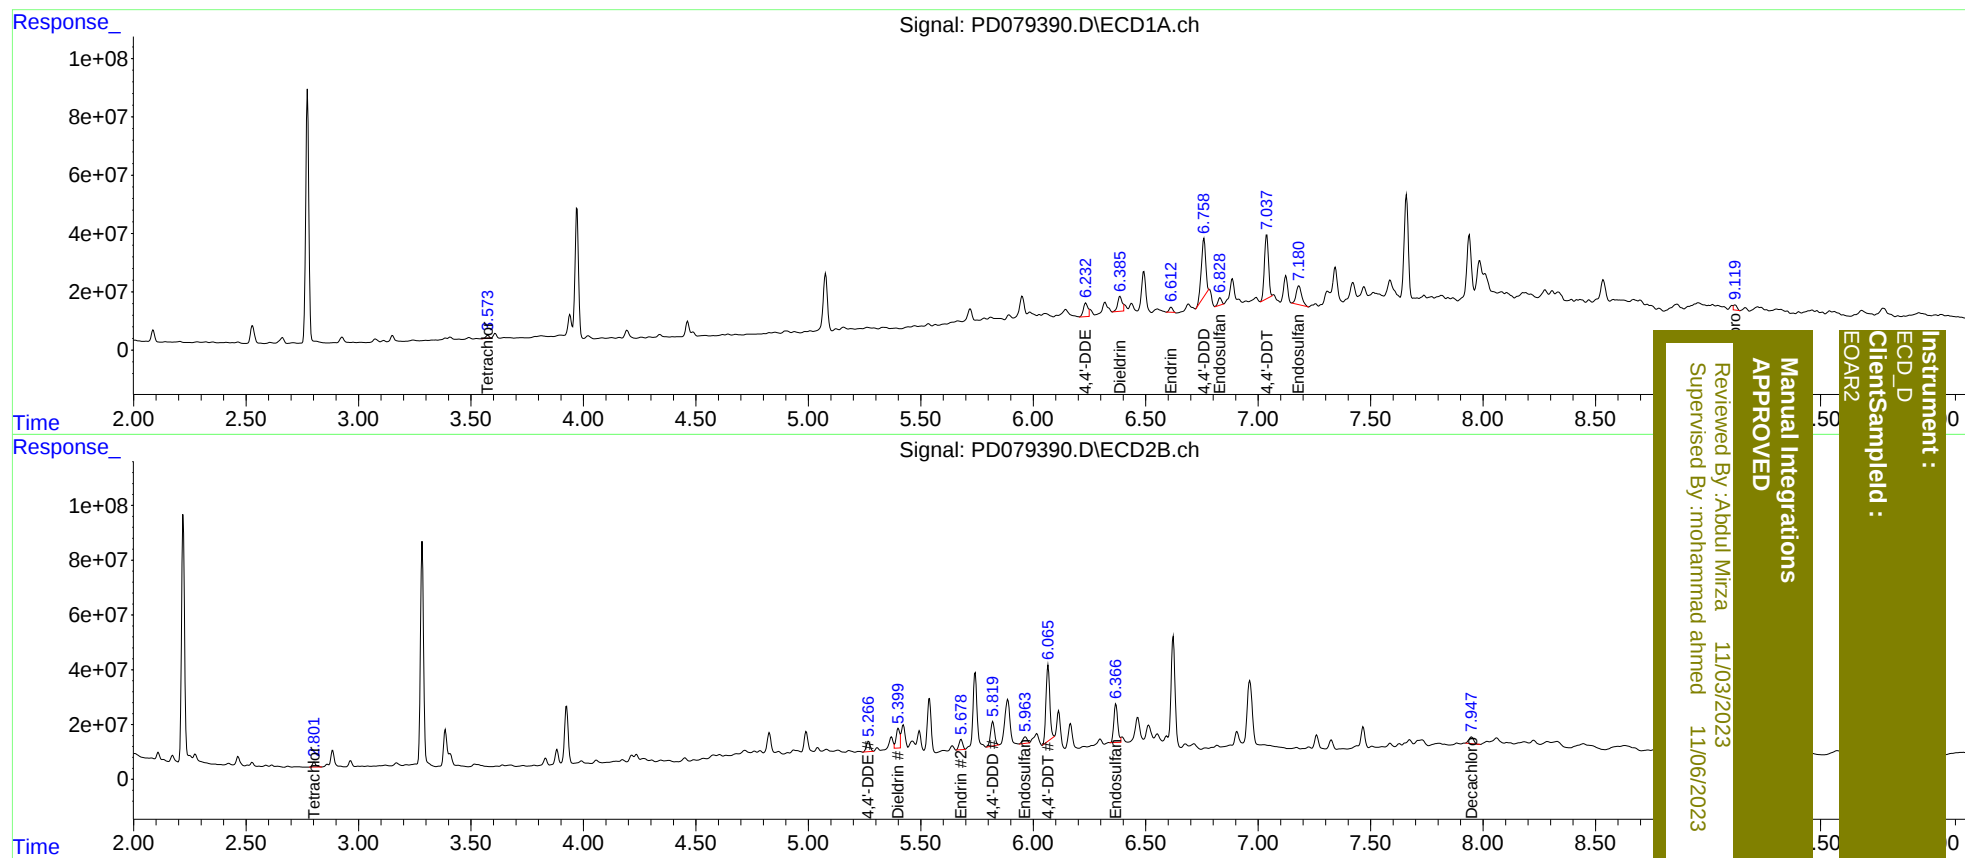

Reviewed By :Abdul Mirza 11/03/2023
Supervised By :mohammad ahmed 11/06/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampleId :
EOAR2