

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
 Data File : PD079395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 13:51
 Operator : AR\AJ
 Sample : 04922-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAT0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/03/2023
 Supervised By : mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 21:39:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.568	2.803	15940404	24398259	10.393	11.251
2) SA Decachlor...	9.110	7.949	11415132	12899155	6.019	5.531
Target Compounds						
12) B 4,4'-DDE	6.226	5.264	91183990	160.2E6	44.265	61.275m#
14) MA Endrin	6.645	5.681	9676877	17269513	5.111m	6.844m#
16) A 4,4'-DDD	6.744	5.819	26206102	37578499	15.591	17.013
17) MA 4,4'-DDT	7.058	6.070	76948120	129.6E6	42.975	57.513 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 13:51
Operator : AR\AJ
Sample : 04922-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:39:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

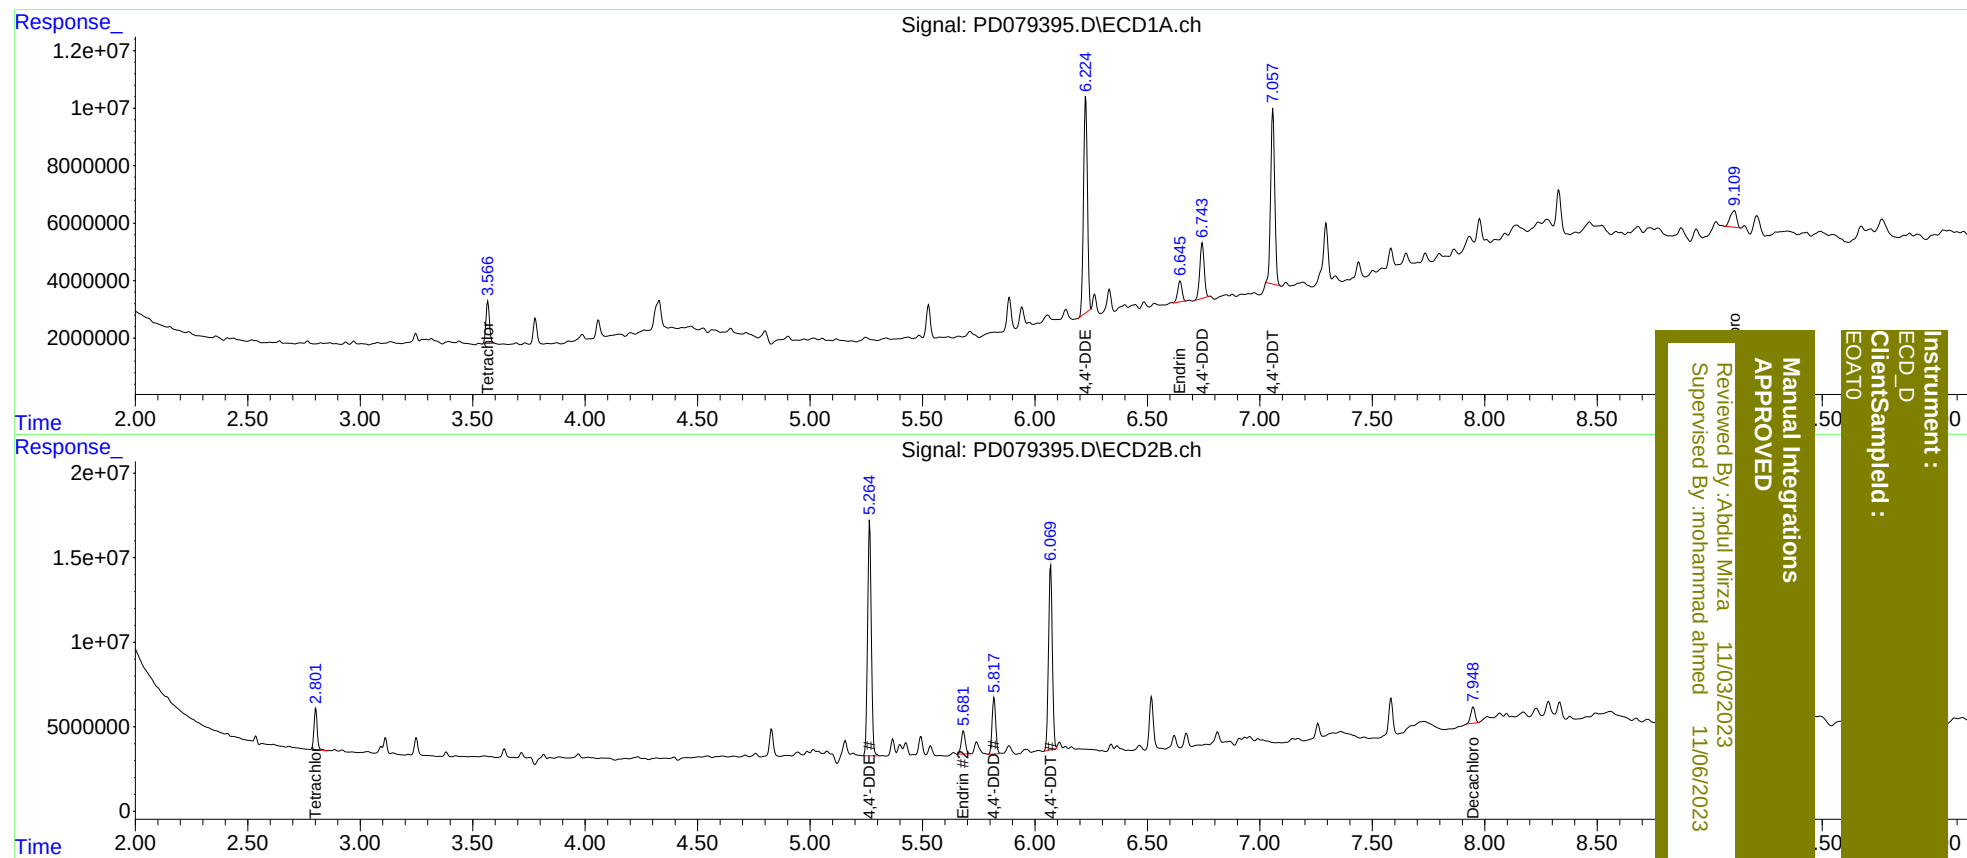

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/03/2023
Supervised By: mohammad ahmed 11/06/2023

Instrument :
ECD_D
ClientSampled :
EOATO