

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
 Data File : PD079396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 14:04
 Operator : AR\AJ
 Sample : 04922-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAT1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/03/2023
 Supervised By :mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 21:41:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.567	2.803	13203053	20233187	8.609	9.330
2) SA Decachlor...	9.107	7.947	11937336	15100320	6.294	6.475m
Target Compounds						
12) B 4,4'-DDE	6.226	5.266	83490872	141.1E6	40.531	53.973 #
14) MA Endrin	6.644	5.681	14414261	20524571	7.614m	8.134m
16) A 4,4'-DDD	6.742	5.819	33191809	52392943	19.747	23.720
17) MA 4,4'-DDT	7.058	6.071	266.8E6	412.0E6	148.983	182.856

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110423\
Data File : PD079396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 14:04
Operator : AR\AJ
Sample : 04922-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:41:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

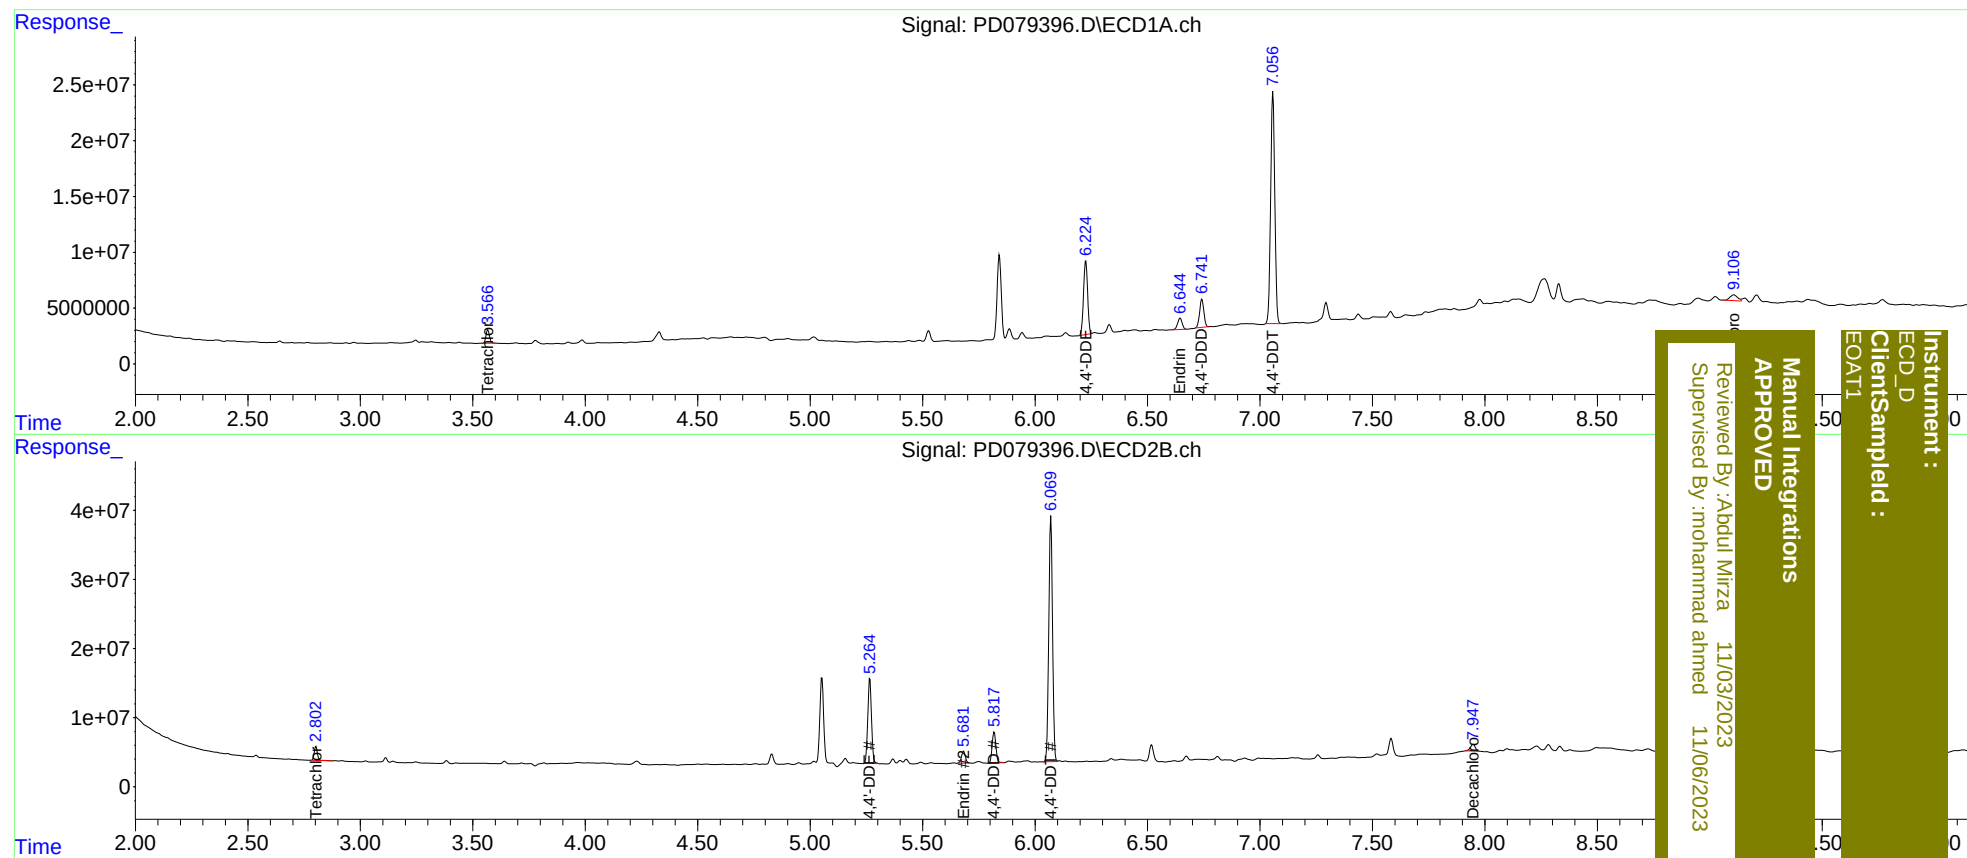

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/03/2023
Supervised By: mohammad ahmed 11/06/2023

Instrument :
ECD_D
ClientSampled :
EOAT1