

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
 Data File : PD050180.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 13:50
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 04:58:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.059	13472883	615.5E6	20.789	22.146
28)	SA Decachlor...	9.017	9.167	13105329	397.4E6	21.669	22.962
Target Compounds							
22)	Mirex	0.000	8.222f	0	37166681	N.D.	2.532 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
Data File : PD050180.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 13:50
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 04:58:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

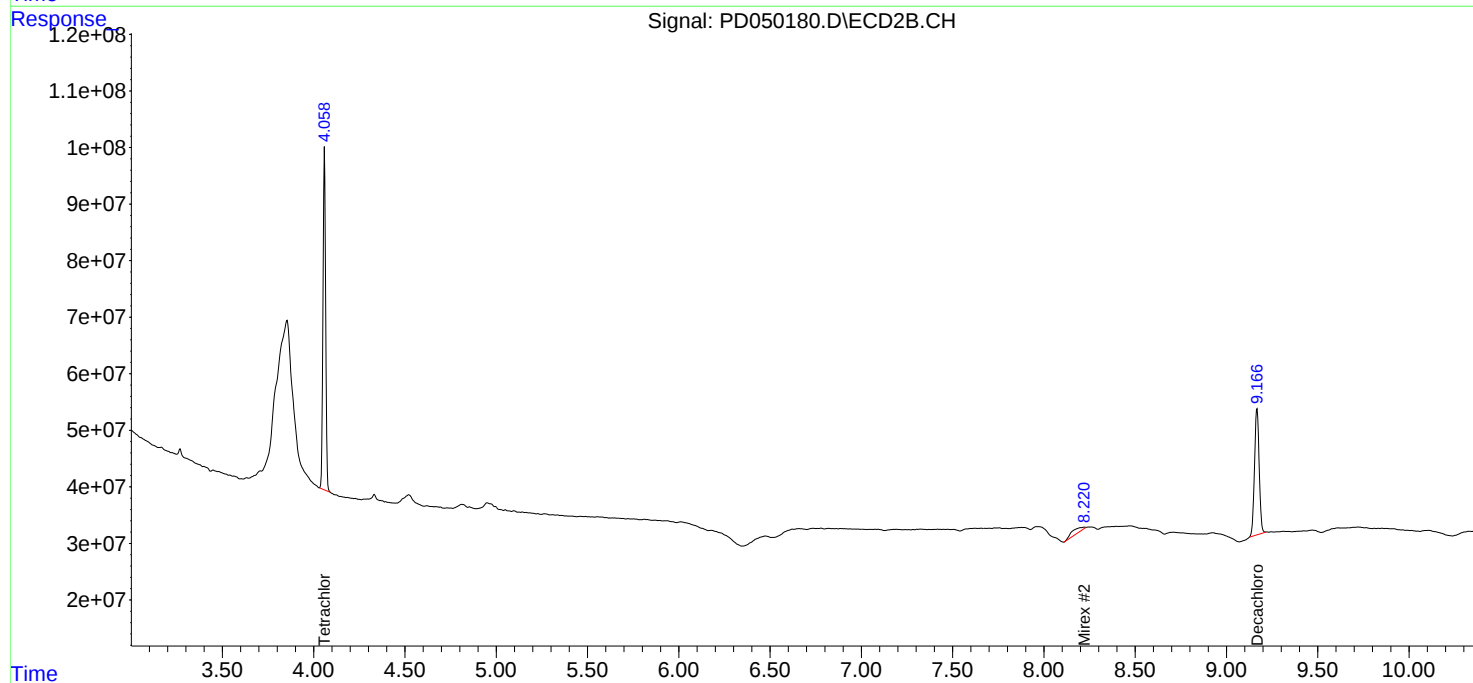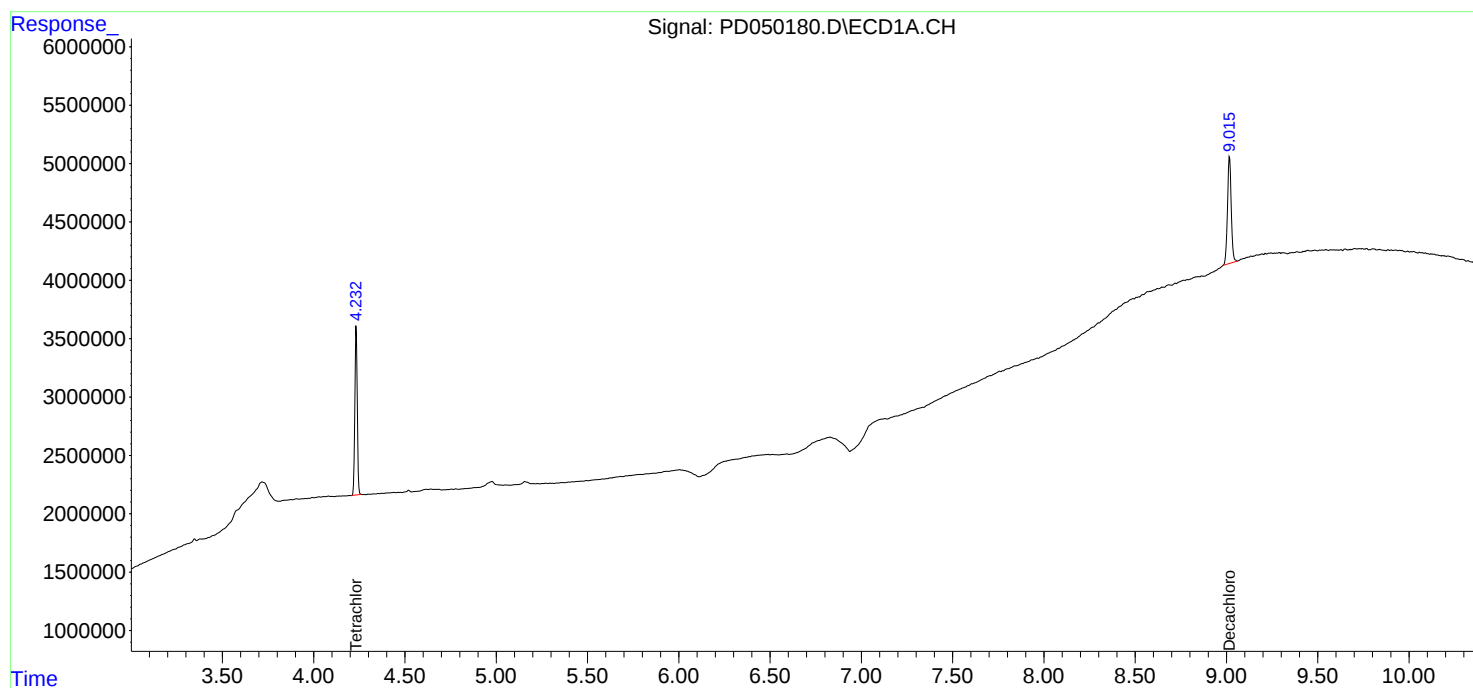


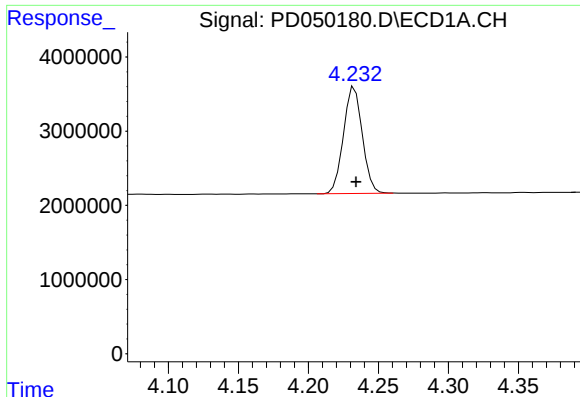

#1 Tetrachloro-m-xylene


R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 13472883
Conc: 20.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

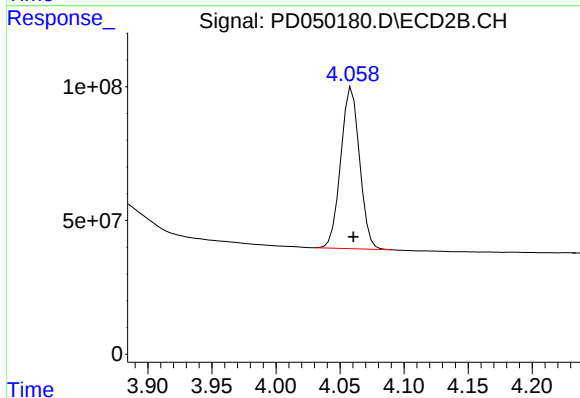


#1 Tetrachloro-m-xylene

R.T.: 4.059 min
Delta R.T.: -0.001 min
Response: 615472415
Conc: 22.15 ng/ml

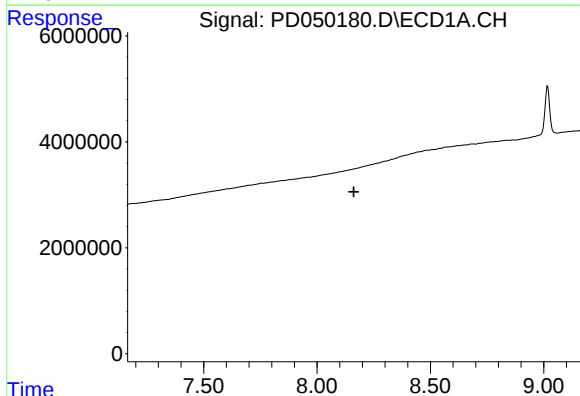


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.162 min
Response: 0
Conc: N.D.

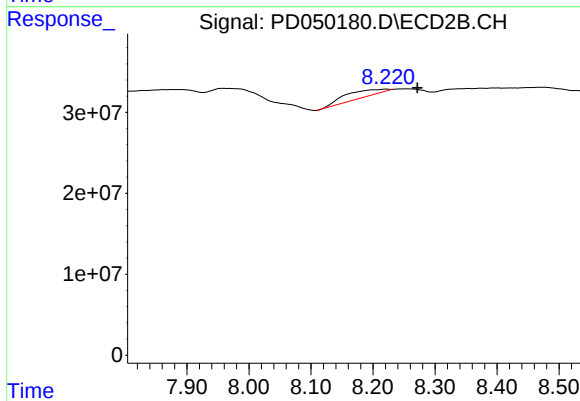

#22 Mirex


R.T.: 8.222 min
Delta R.T.: -0.050 min
Response: 37166681
Conc: 2.53 ng/ml

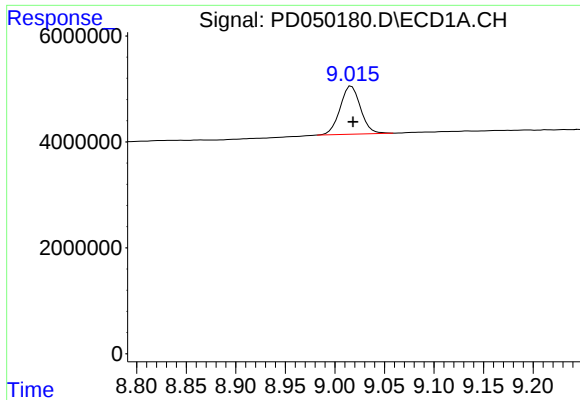

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.002 min
Response: 13105329
Conc: 21.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

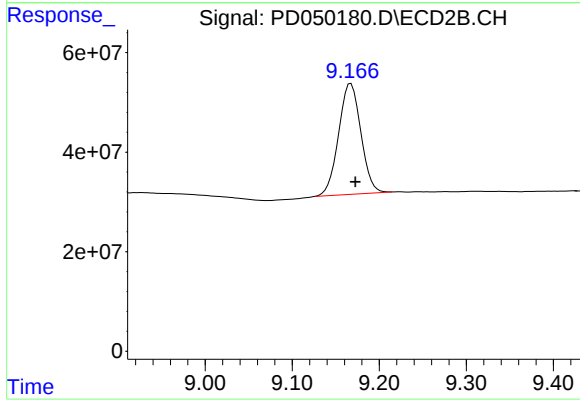

#28 Decachlorobiphenyl

R.T.: 9.167 min
Delta R.T.: -0.005 min
Response: 397357554
Conc: 22.96 ng/ml