

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
 Data File : PD050182.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 14:18
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc : FOR MIREX
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 04:59:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.060	32126869	1347.8E6	49.571	48.495
28)	SA Decachlor...	9.017	9.168	29735286	828.1E6	49.166	47.851
Target Compounds							
22)	Mirex	8.160	8.269	27817265	730.8E6	50.054	49.782



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
Data File : PD050182.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 14:18
Operator : AJ\SJ
Sample : PSTDCCC050
Misc : FOR MIREX
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 04:59:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

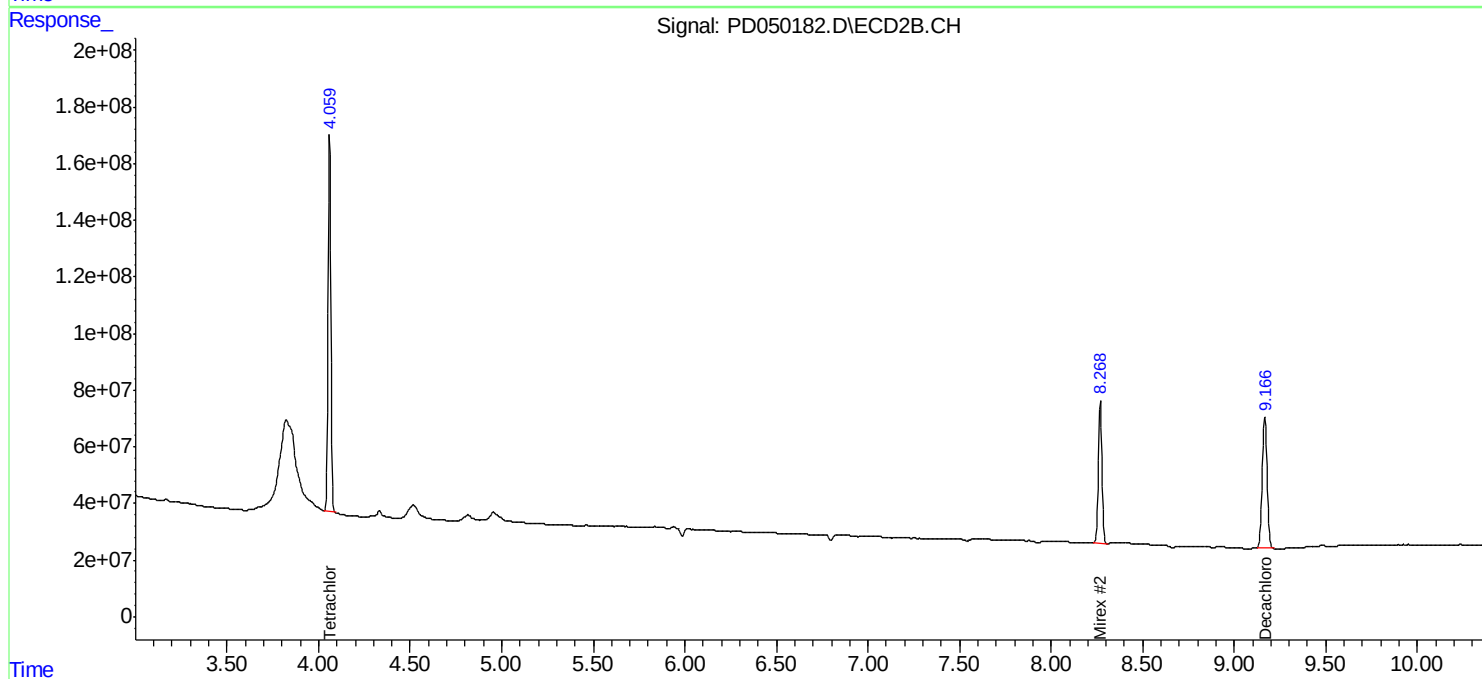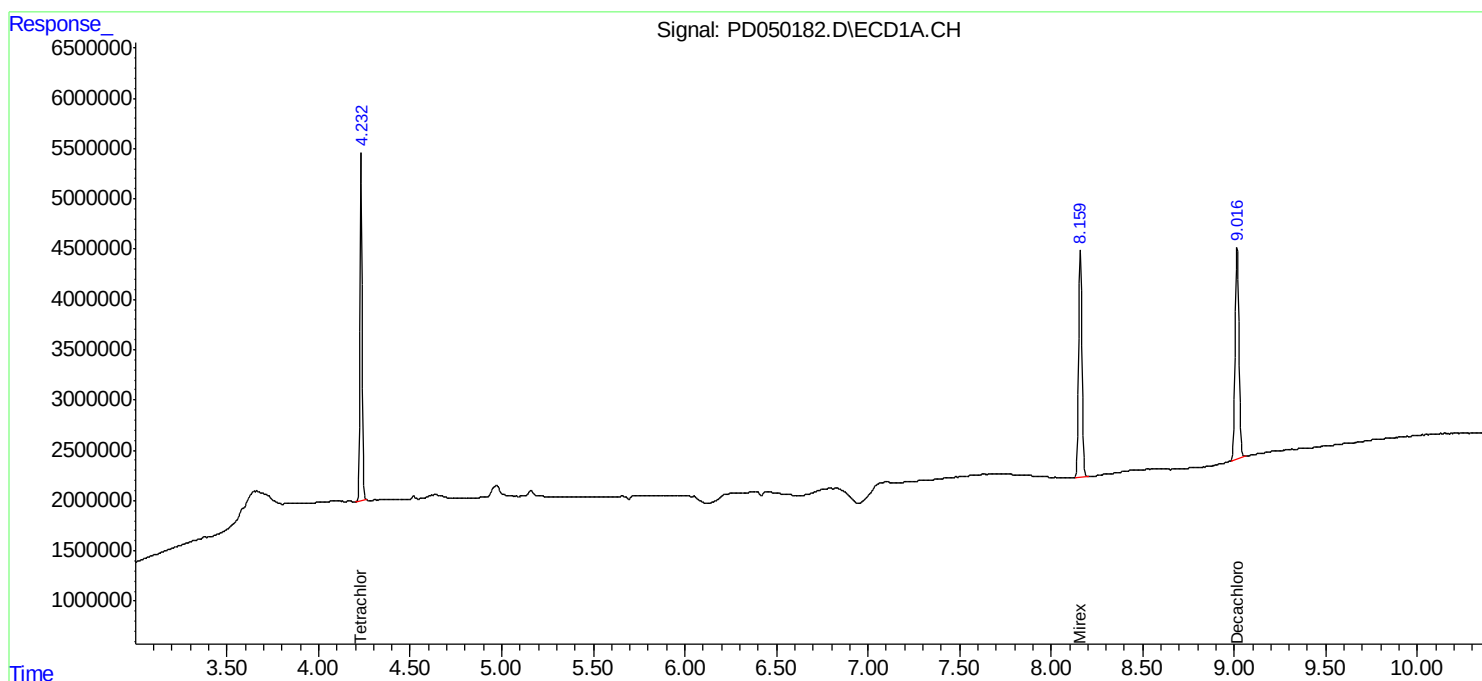


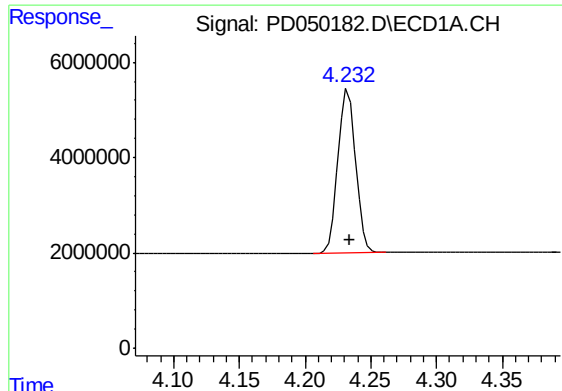

#1 Tetrachloro-m-xylene


R.T.: 4.233 min
Delta R.T.: -0.001 min
Response: 32126869
Conc: 49.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

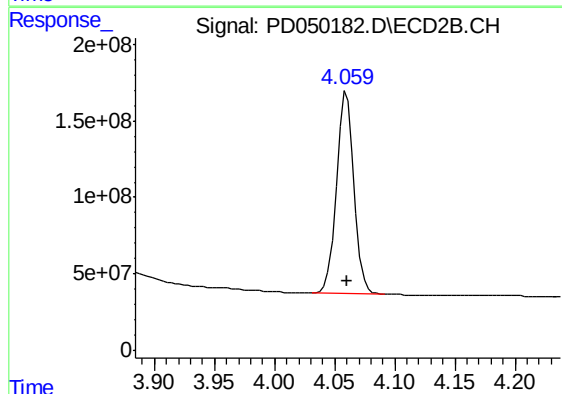


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: 0.000 min
Response: 1347777592
Conc: 48.50 ng/ml

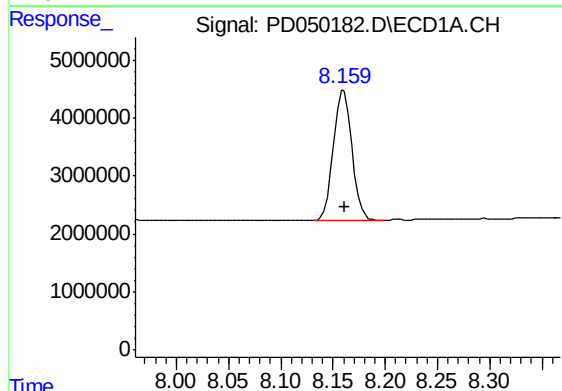


#22 Mirex

R.T.: 8.160 min
Delta R.T.: -0.001 min
Response: 27817265
Conc: 50.05 ng/ml

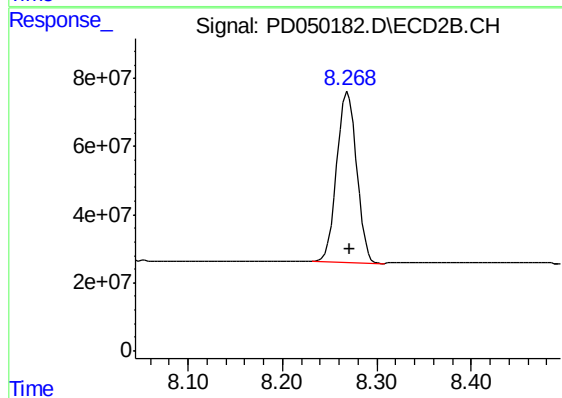

#22 Mirex


R.T.: 8.269 min
Delta R.T.: -0.002 min
Response: 730772232
Conc: 49.78 ng/ml

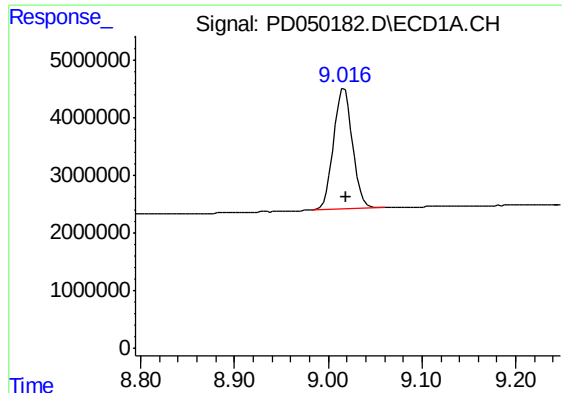

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.002 min
Response: 29735286
Conc: 49.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

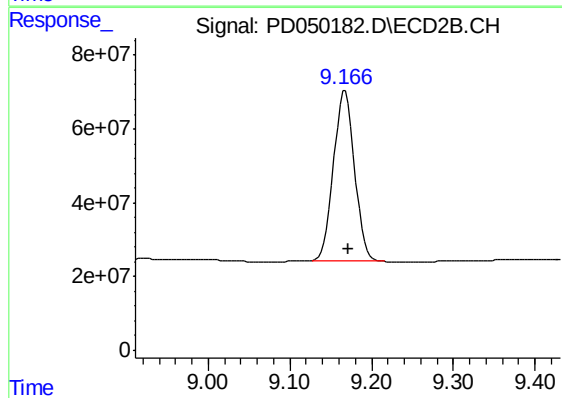

#28 Decachlorobiphenyl

R.T.: 9.168 min
Delta R.T.: -0.005 min
Response: 828073519
Conc: 47.85 ng/ml