

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
 Data File : PD050183.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 14:32
 Operator : AJ\SJ
 Sample : MIREX-MDL-BL-S-03
 Misc : FOR MIREX
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-BL-S-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 04:59:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.060	13320994	591.7E6	20.554	21.289
28)	SA Decachlor...	9.017	9.168	12780732	398.5E6	21.133	23.027

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
Data File : PD050183.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 14:32
Operator : AJ\SJ
Sample : MIREX-MDL-BL-S-03
Misc : FOR MIREX
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-BL-S-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 04:59:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

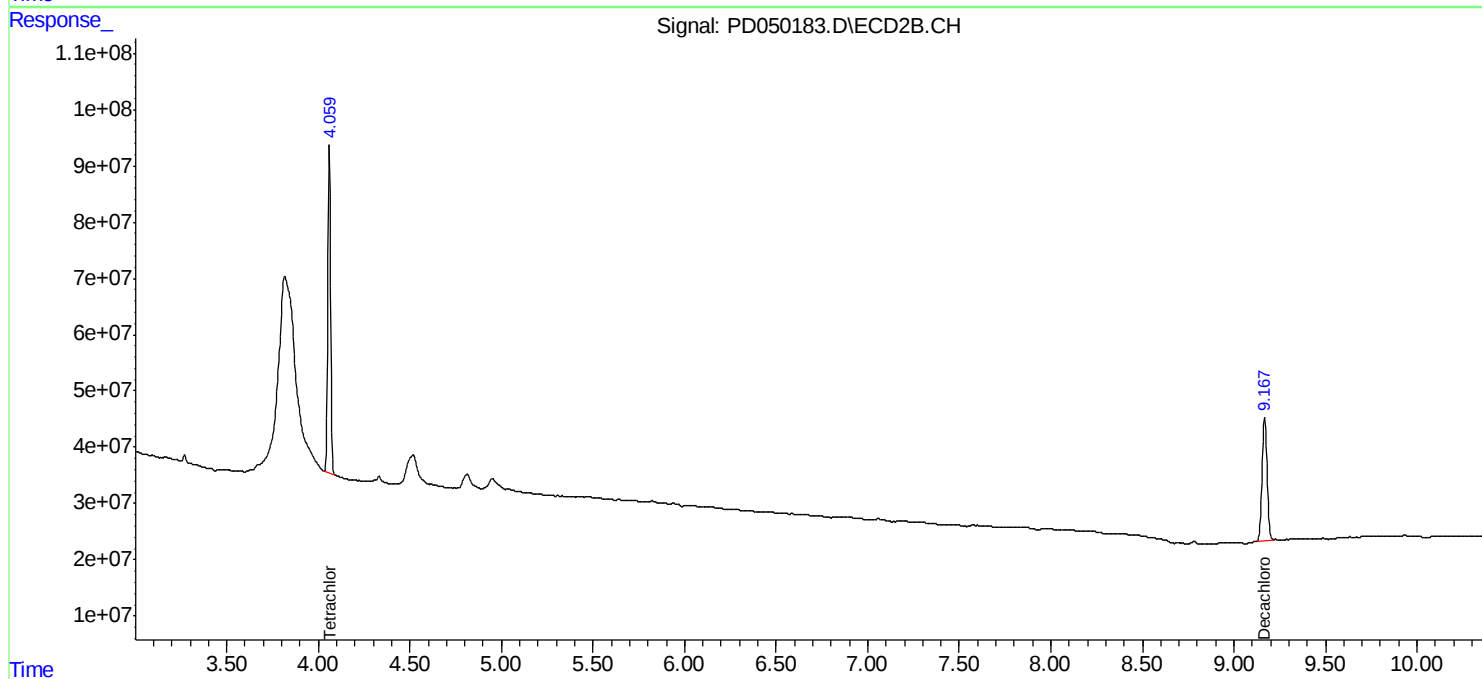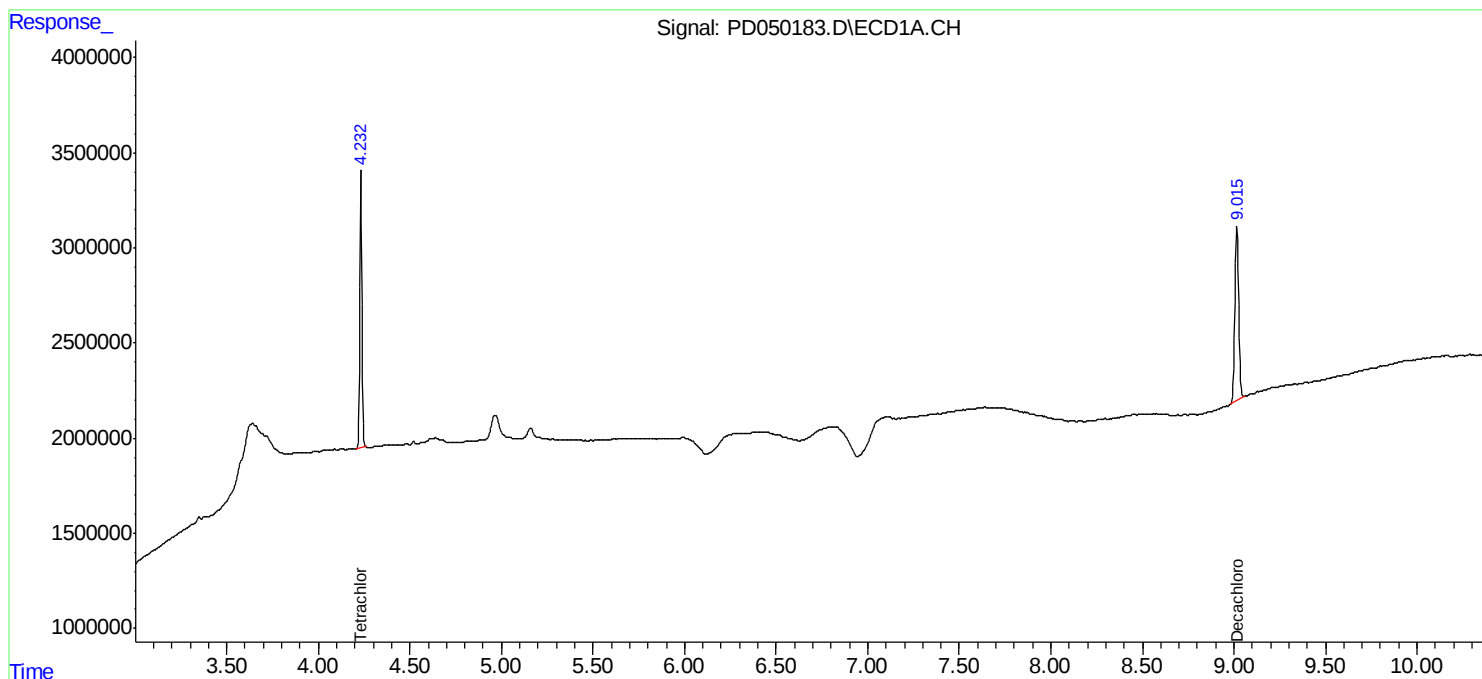


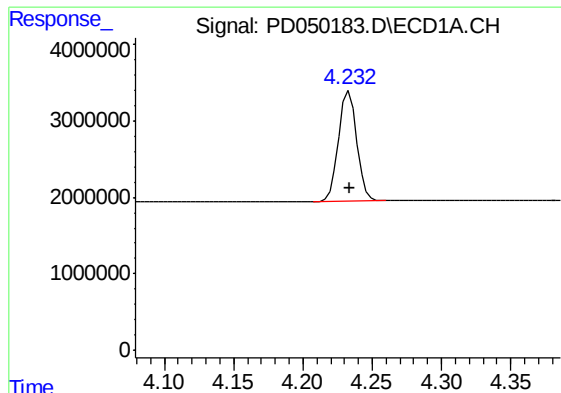

#1 Tetrachloro-m-xylene


R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 13320994
Conc: 20.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-BL-S-03

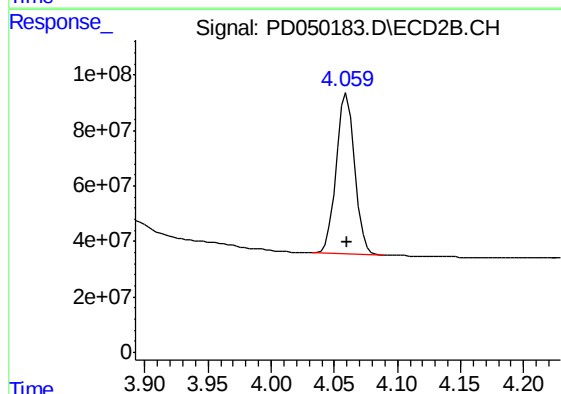


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: 0.000 min
Response: 591668208
Conc: 21.29 ng/ml

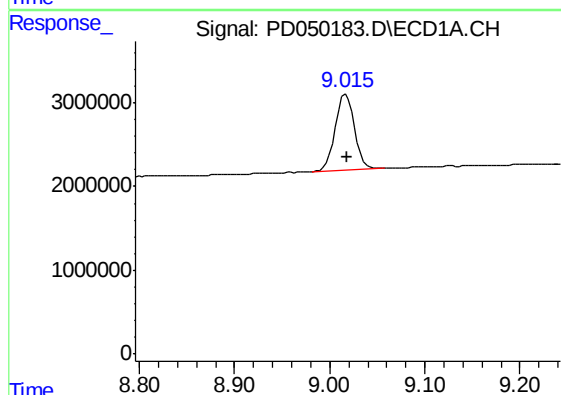

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.002 min
Response: 12780732
Conc: 21.13 ng/ml

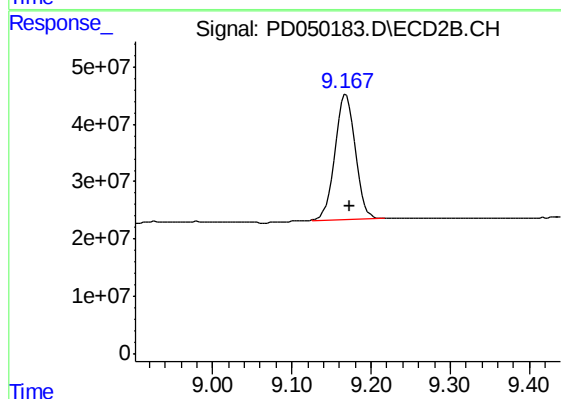

#28 Decachlorobiphenyl

R.T.: 9.168 min
Delta R.T.: -0.004 min
Response: 398481114
Conc: 23.03 ng/ml