

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
 Data File : PD050184.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 14:46
 Operator : AJ\SJ
 Sample : MIREX-MDL-S-06
 Misc : FOR MIREX
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-S-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 04:59:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	4.061	13288890	579.5E6	20.505	20.853
28)	SA Decachlor...	9.018	9.169	12919844	384.7E6	21.363	22.232
Target Compounds							
22)	Mirex	8.161	8.270	501103	16495418	0.902	1.124



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
Data File : PD050184.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 14:46
Operator : AJ\SJ
Sample : MIREX-MDL-S-06
Misc : FOR MIREX
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 04:59:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

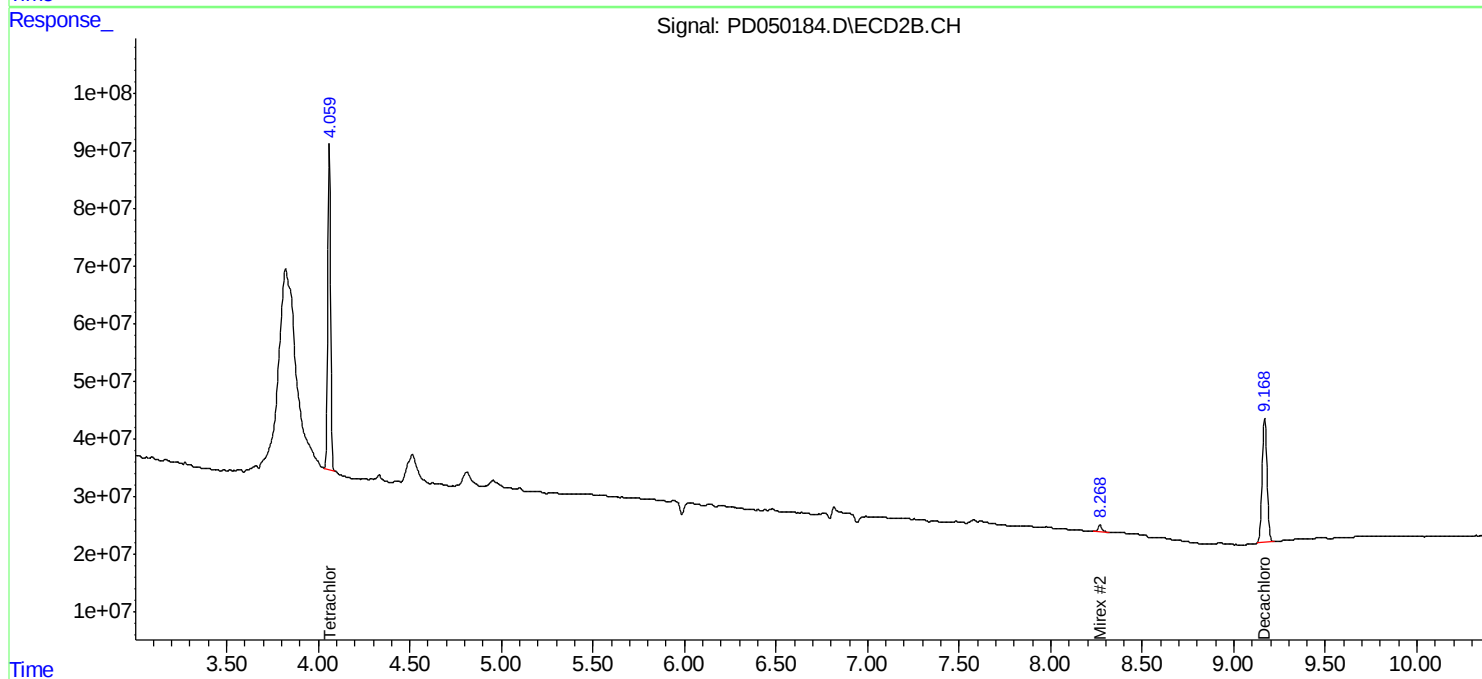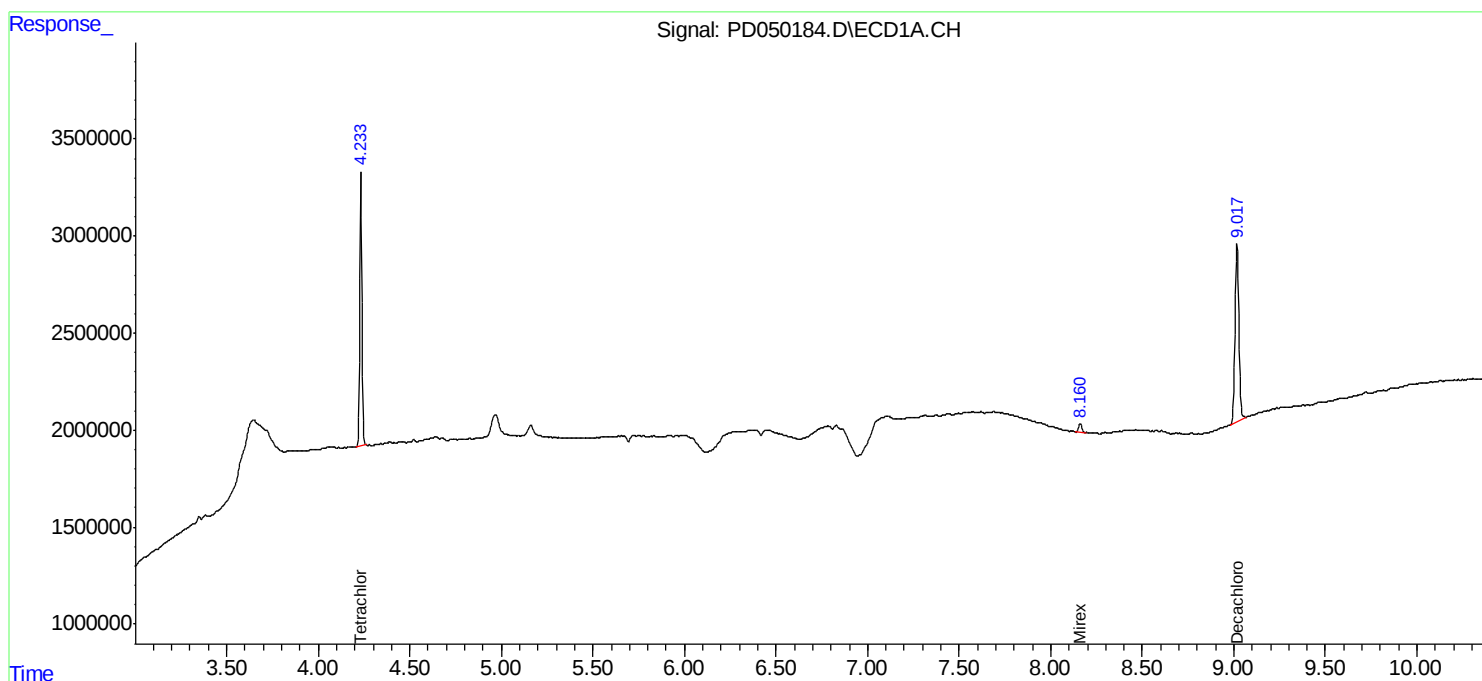


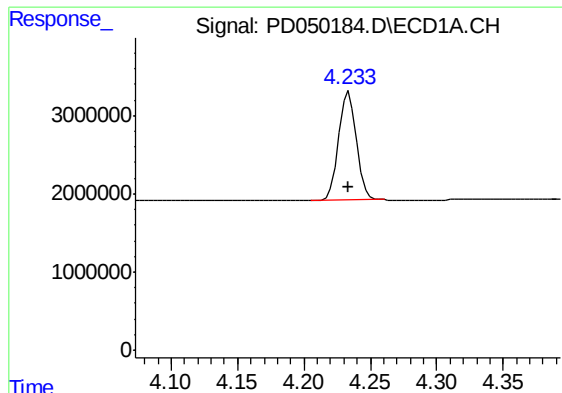

#1 Tetrachloro-m-xylene


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 13288890
Conc: 20.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-06

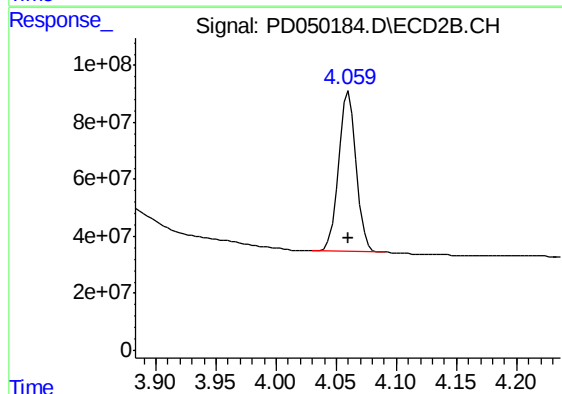


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 579532020
Conc: 20.85 ng/ml

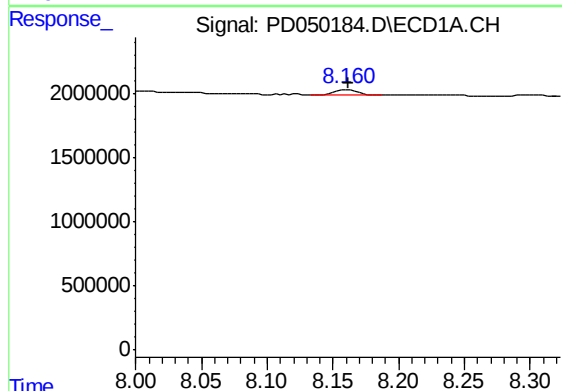


#22 Mirex

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 501103
Conc: 0.90 ng/ml

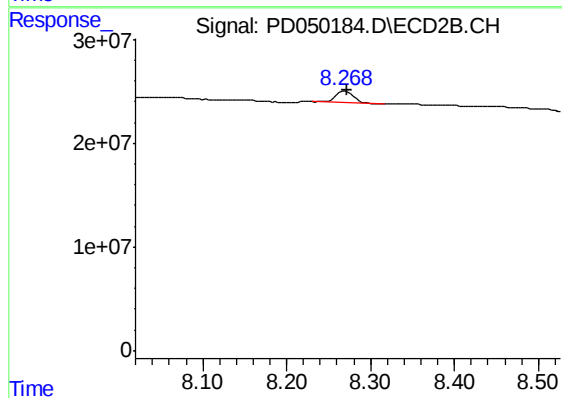

#22 Mirex


R.T.: 8.270 min
Delta R.T.: -0.002 min
Response: 16495418
Conc: 1.12 ng/ml

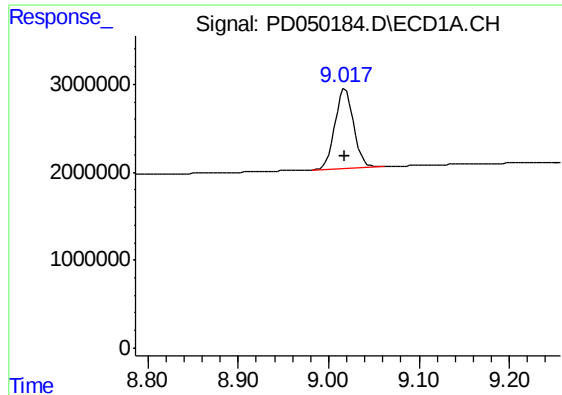

#28 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: 0.000 min
Response: 12919844
Conc: 21.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-06

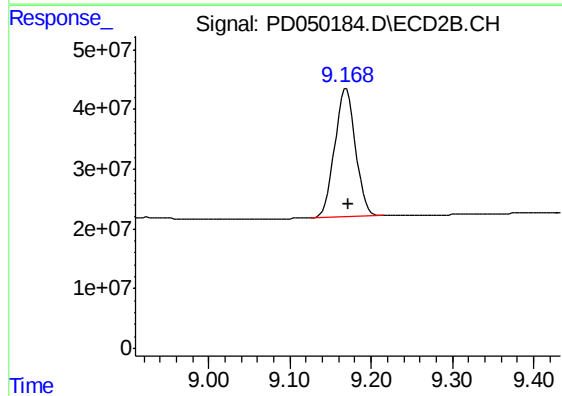

#28 Decachlorobiphenyl

R.T.: 9.169 min
Delta R.T.: -0.003 min
Response: 384723541
Conc: 22.23 ng/ml