

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
 Data File : PD050185.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 15:00
 Operator : AJ\SJ
 Sample : MIREX-MDL-S-07
 Misc : FOR MIREX
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-S-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 04:59:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	4.060	10433862	466.1E6	16.099	16.772
28)	SA Decachlor...	9.017	9.168	10456583	322.6E6	17.290	18.639
Target Compounds							
22)	Mirex	8.160	8.270	449385	13520868	0.809	0.921



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
Data File : PD050185.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 15:00
Operator : AJ\SJ
Sample : MIREX-MDL-S-07
Misc : FOR MIREX
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-07

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 04:59:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

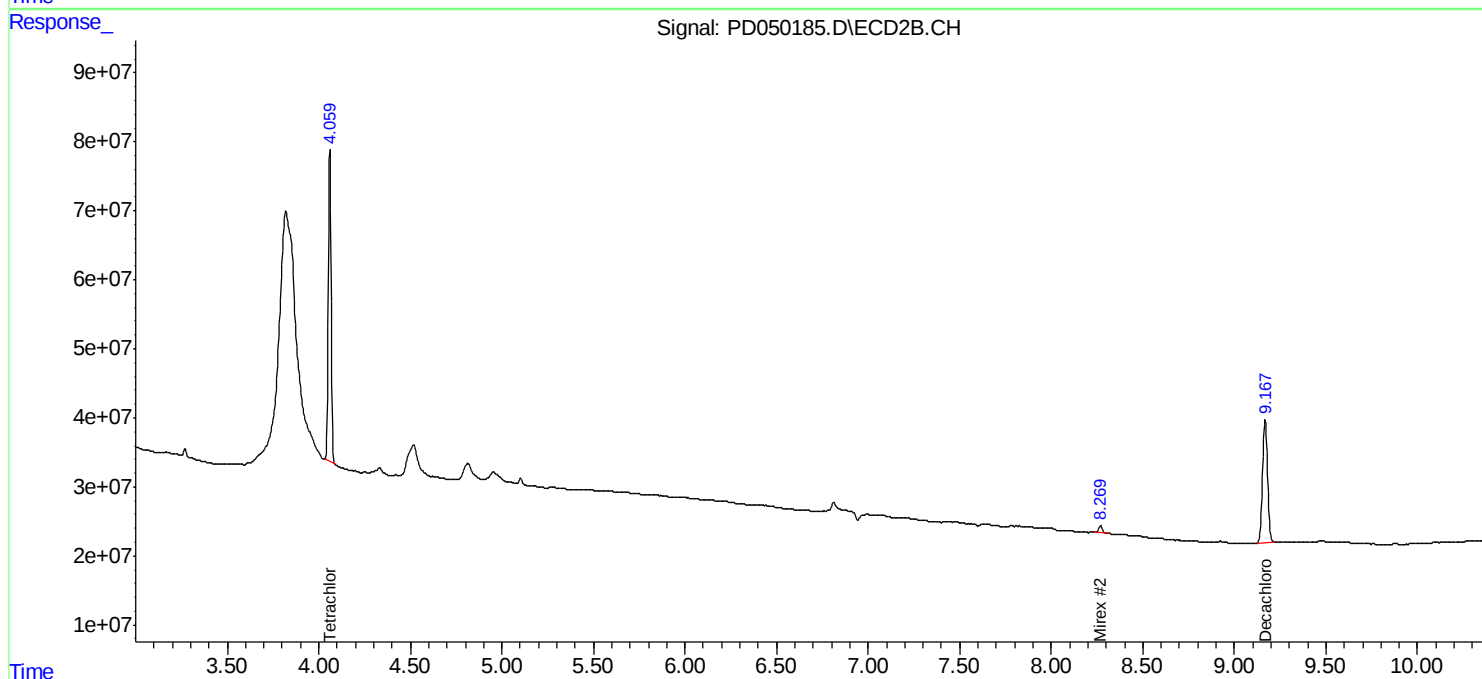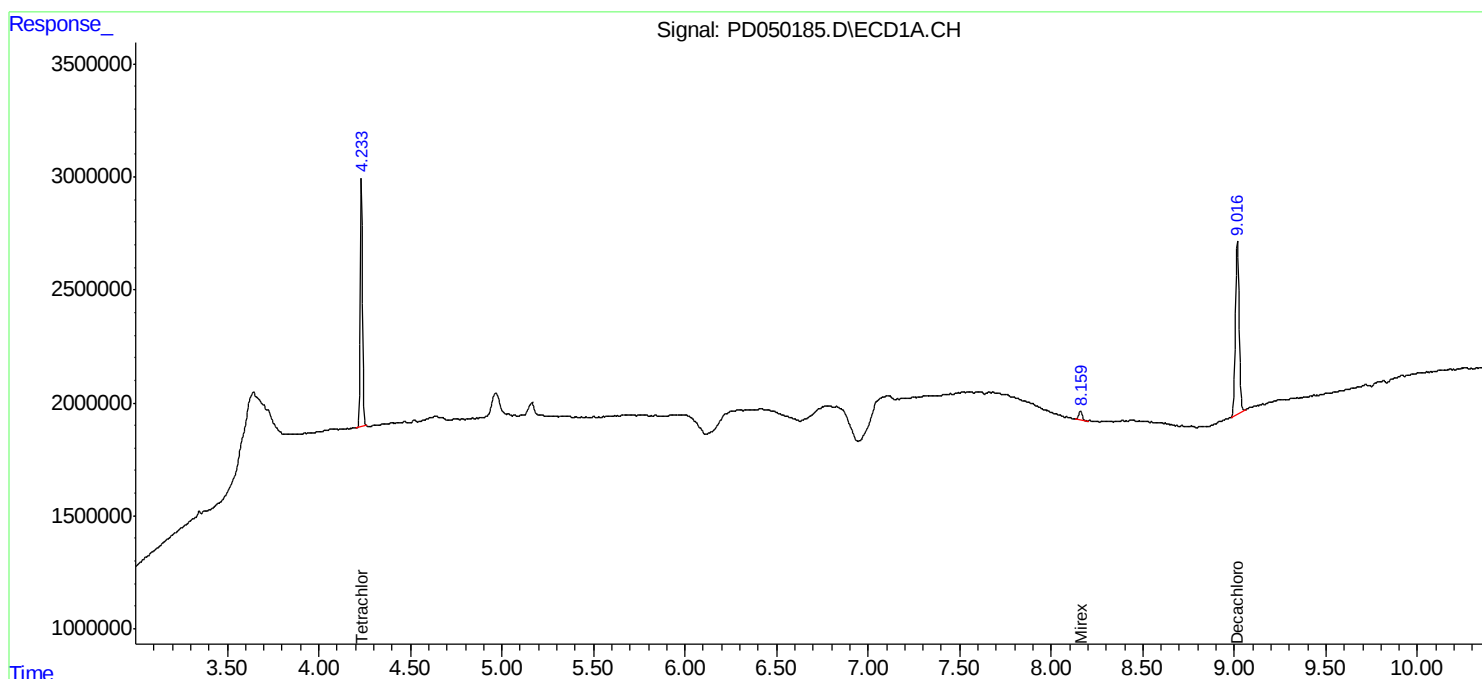


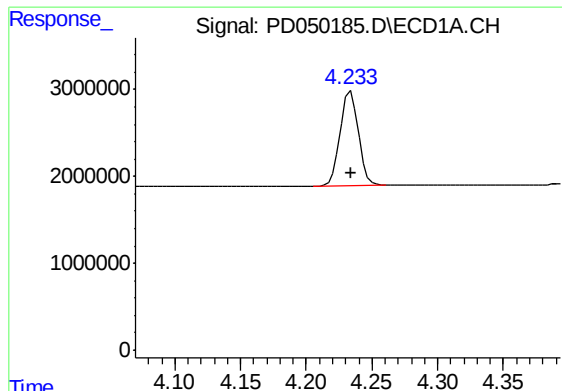

#1 Tetrachloro-m-xylene


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 10433862
Conc: 16.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-07

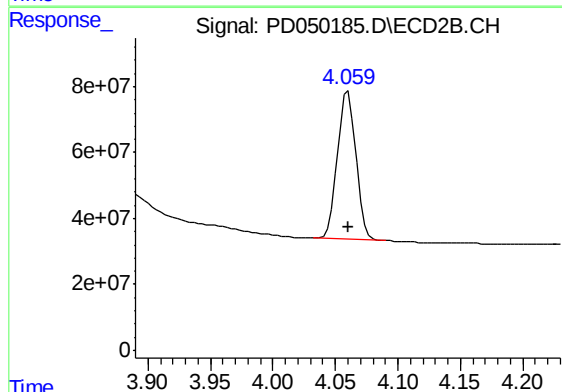


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: 0.000 min
Response: 466124229
Conc: 16.77 ng/ml

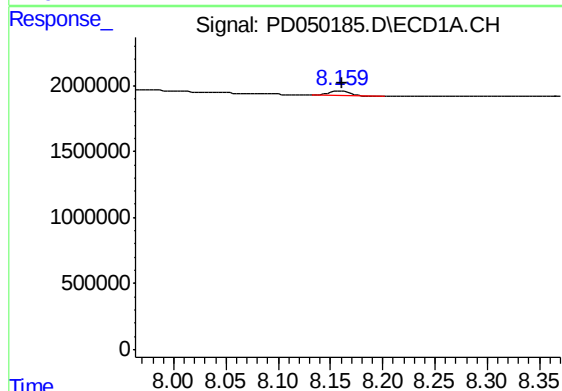


#22 Mirex

R.T.: 8.160 min
Delta R.T.: -0.001 min
Response: 449385
Conc: 0.81 ng/ml

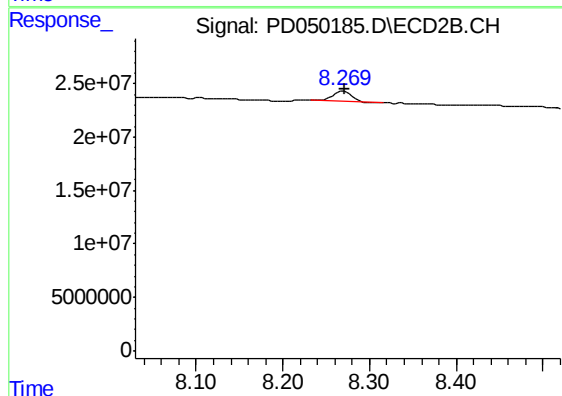

#22 Mirex


R.T.: 8.270 min
Delta R.T.: -0.002 min
Response: 13520868
Conc: 0.92 ng/ml

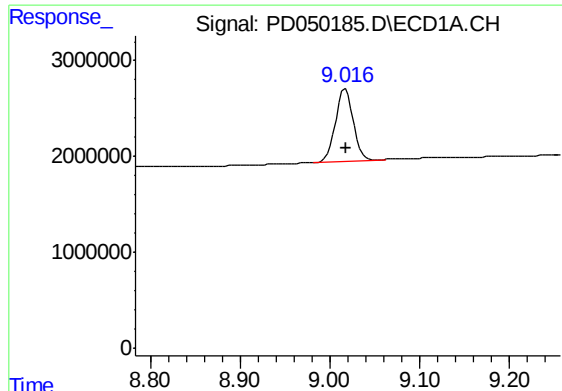

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.001 min
Response: 10456583
Conc: 17.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-07

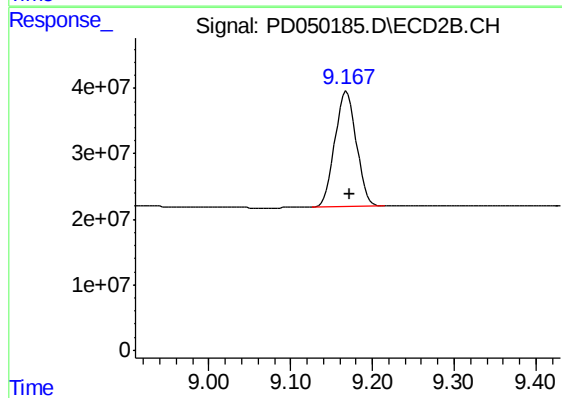

#28 Decachlorobiphenyl

R.T.: 9.168 min
Delta R.T.: -0.004 min
Response: 322554137
Conc: 18.64 ng/ml