

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
 Data File : PD050186.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 15:14
 Operator : AJ\SJ
 Sample : MIREX-MDL-BL-W-03
 Misc : FOR MIREX
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-BL-W-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 05:05:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	4.061	13244792	589.7E6	20.437	21.218
28)	SA Decachlor...	9.017	9.168	13051379	399.1E6	21.580	23.060

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
Data File : PD050186.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 15:14
Operator : AJ\SJ
Sample : MIREX-MDL-BL-W-03
Misc : FOR MIREX
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-BL-W-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 05:05:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

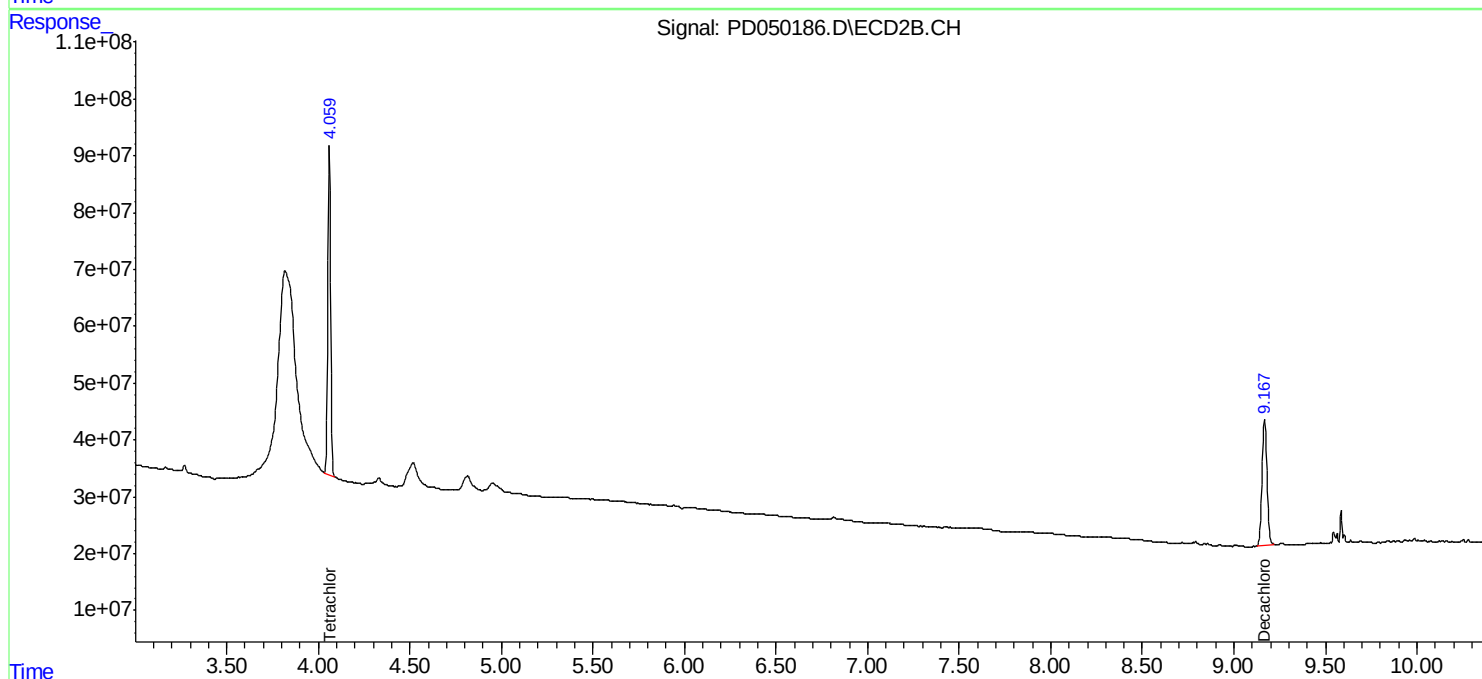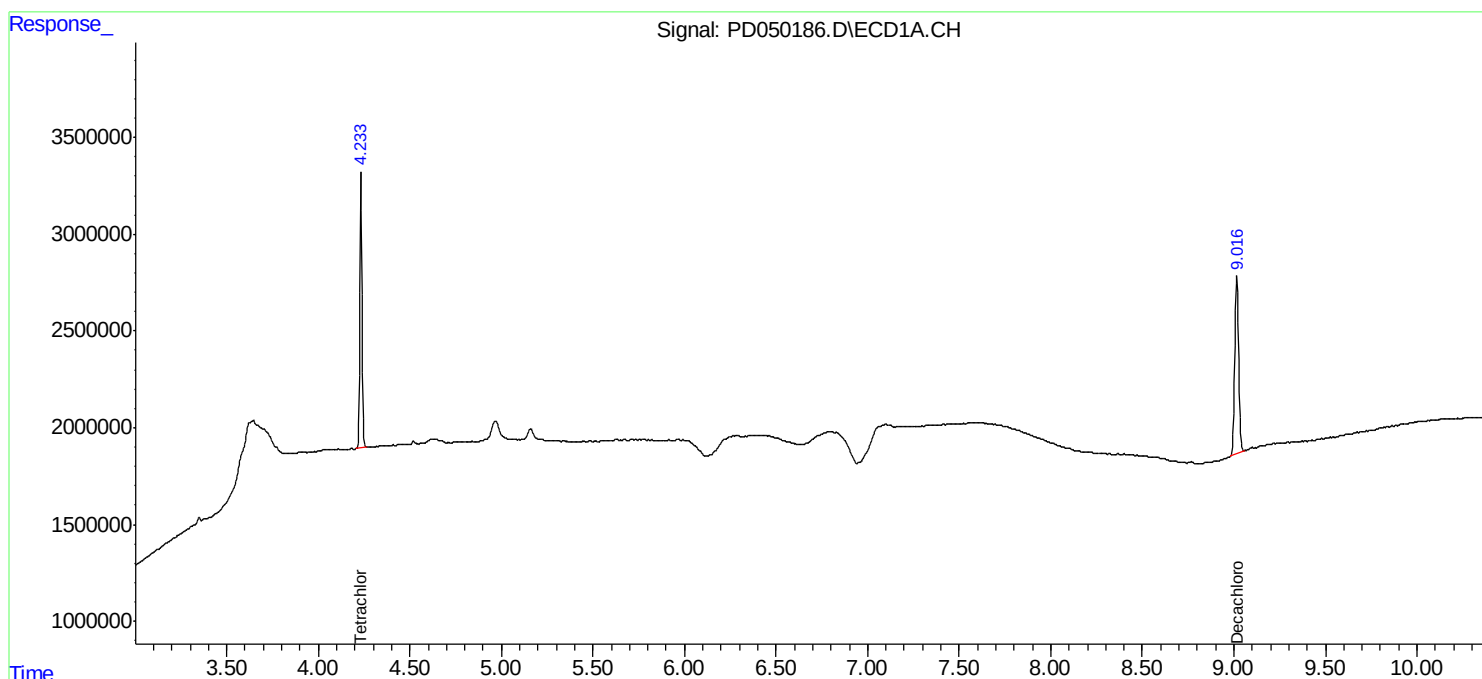


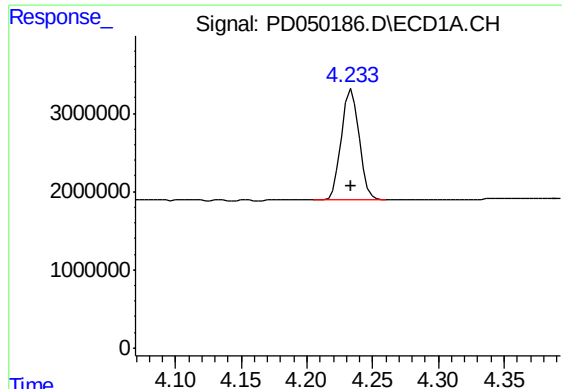

#1 Tetrachloro-m-xylene


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 13244792
Conc: 20.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-BL-W-03

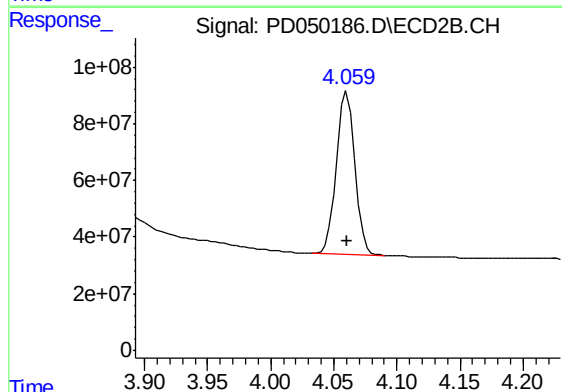


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 589679338
Conc: 21.22 ng/ml

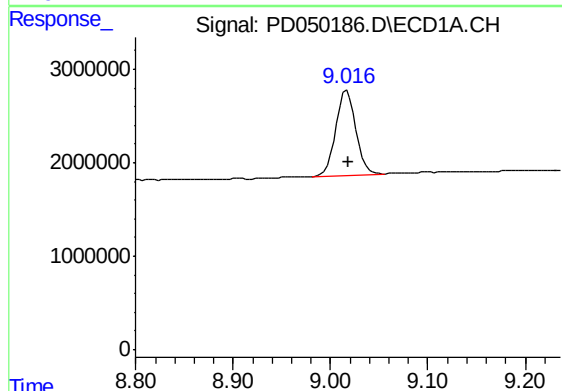

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.002 min
Response: 13051379
Conc: 21.58 ng/ml

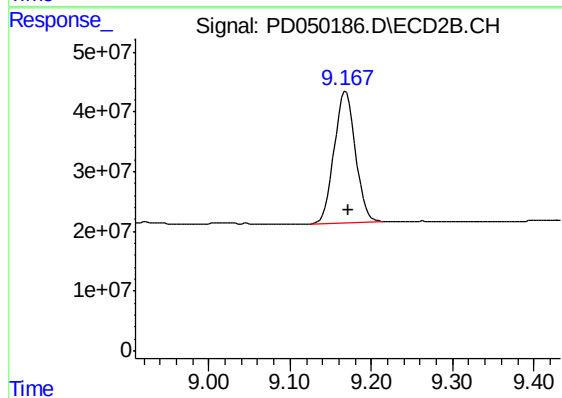

#28 Decachlorobiphenyl

R.T.: 9.168 min
Delta R.T.: -0.004 min
Response: 399058035
Conc: 23.06 ng/ml