

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
 Data File : PD050187.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 15:28
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-06
 Misc : FOR MIREX
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-W-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 05:02:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	4.060	13211212	578.4E6	20.385	20.813
28)	SA Decachlor...	9.017	9.168	12857628	390.2E6	21.260	22.547
Target Compounds							
22)	Mirex	8.161	8.269	540565	17948388	0.973	1.223 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
Data File : PD050187.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 15:28
Operator : AJ\SJ
Sample : MIREX-MDL-W-06
Misc : FOR MIREX
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 05:02:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

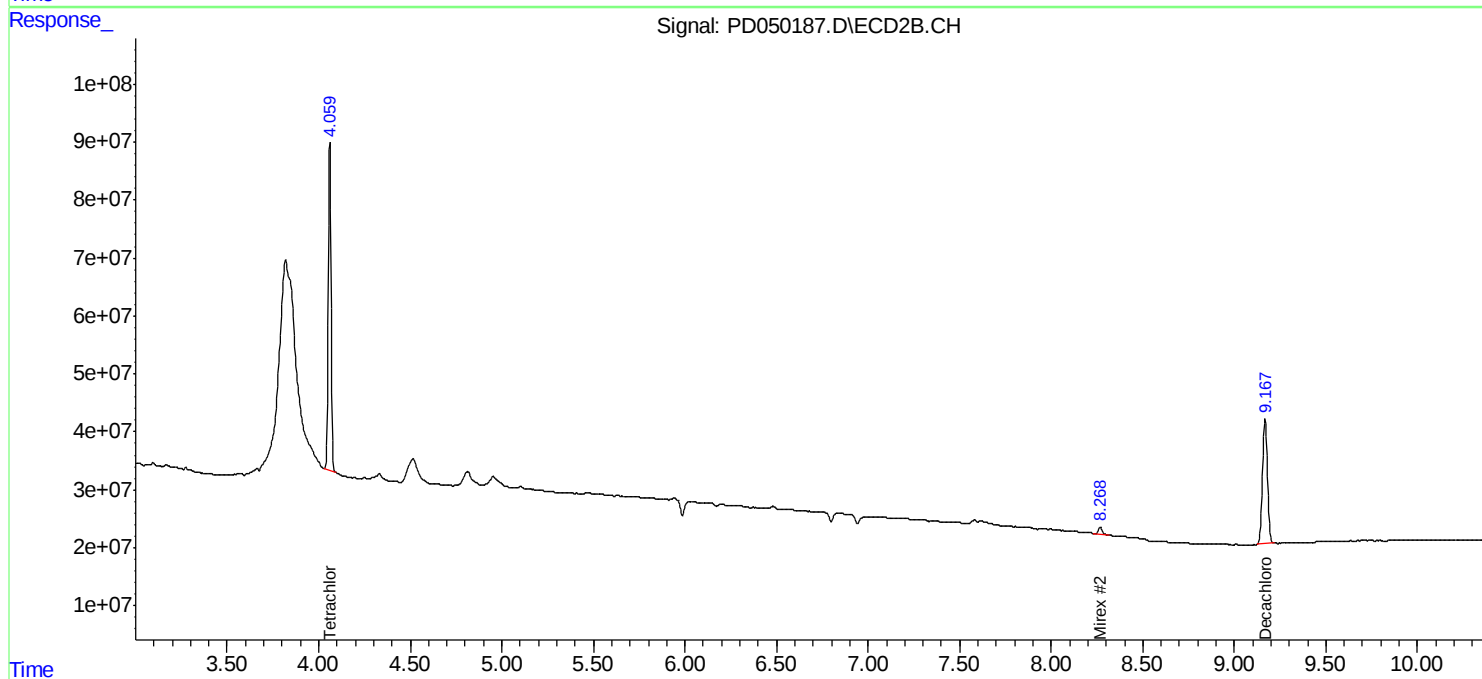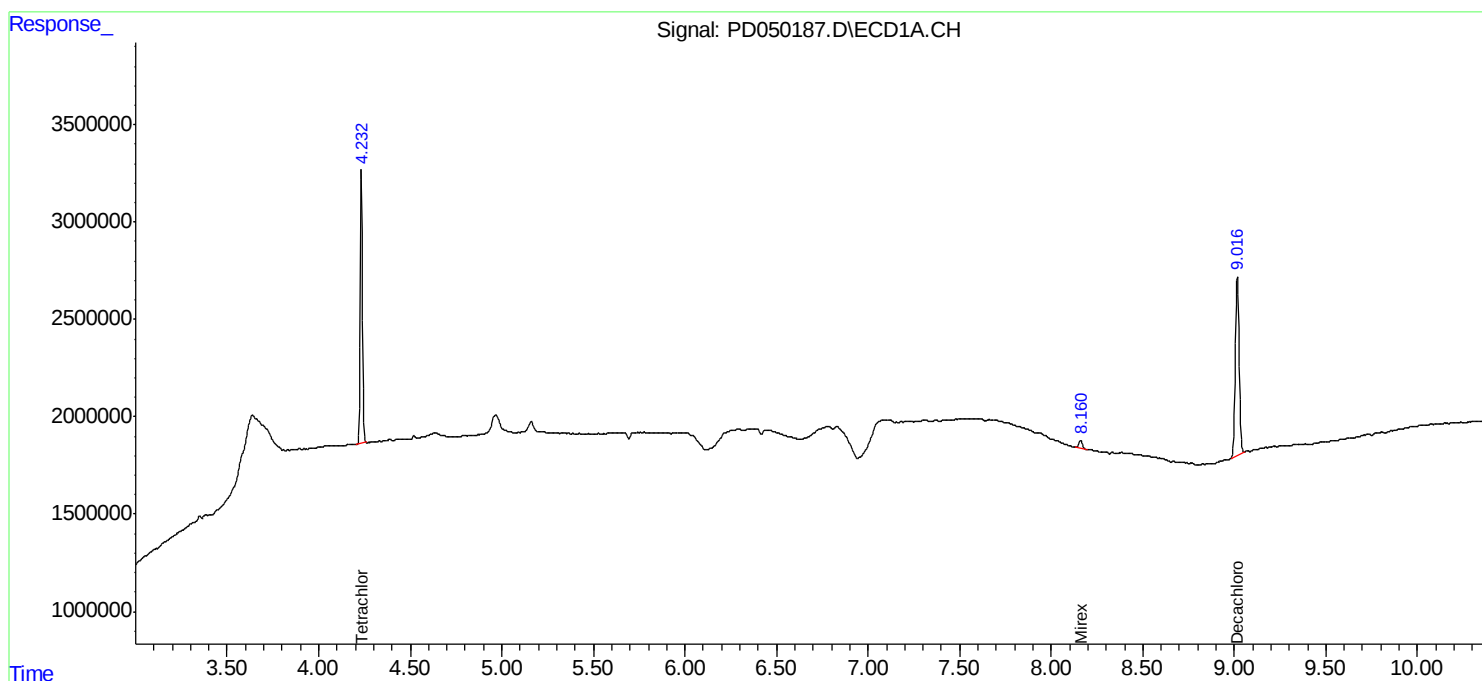


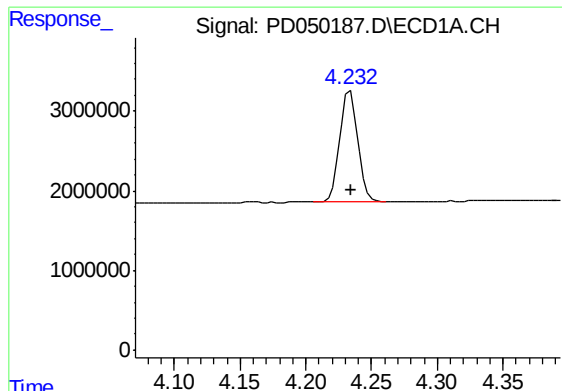

#1 Tetrachloro-m-xylene


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 13211212
Conc: 20.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-06

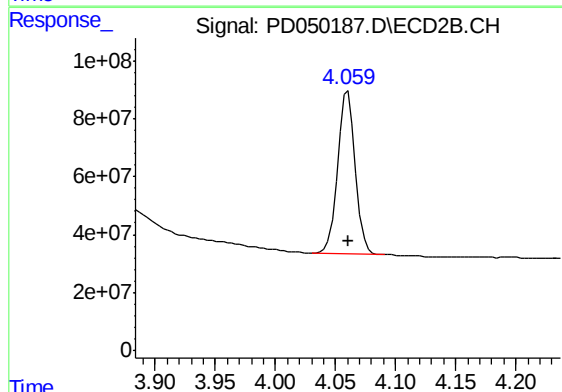


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: 0.000 min
Response: 578444030
Conc: 20.81 ng/ml

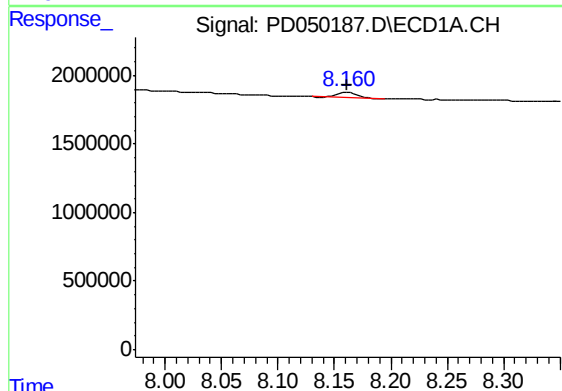


#22 Mirex

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 540565
Conc: 0.97 ng/ml

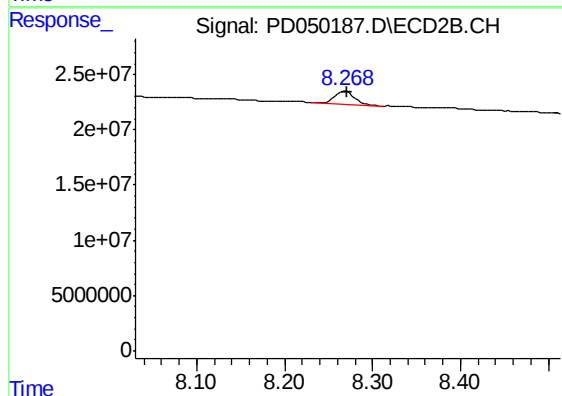

#22 Mirex


R.T.: 8.269 min
Delta R.T.: -0.003 min
Response: 17948388
Conc: 1.22 ng/ml

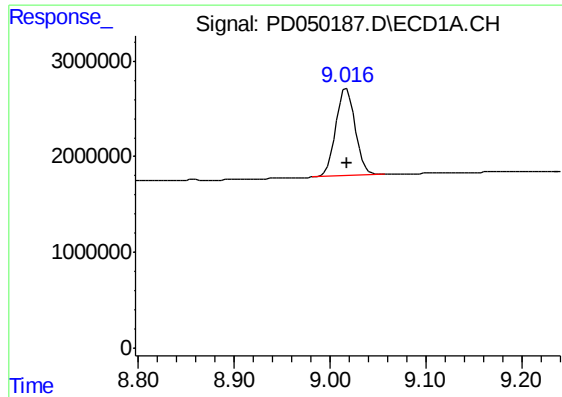

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.001 min
Response: 12857628
Conc: 21.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-06

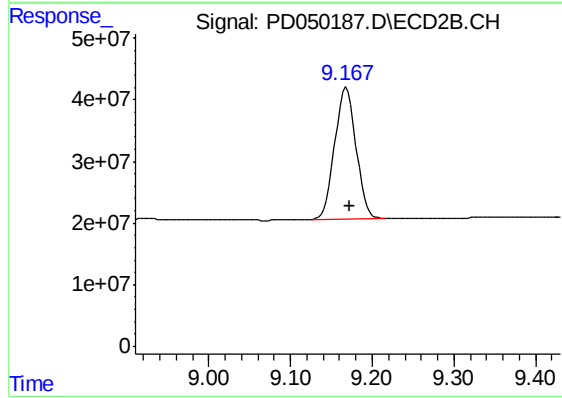

#28 Decachlorobiphenyl

R.T.: 9.168 min
Delta R.T.: -0.004 min
Response: 390173920
Conc: 22.55 ng/ml