

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
 Data File : PD050188.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 15:42
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-07
 Misc : FOR MIREX
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-W-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 05:03:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	4.061	10579068	479.9E6	16.323	17.267
28)	SA Decachlor...	9.017	9.169	10564370	326.0E6	17.468	18.839
Target Compounds							
22)	Mirex	8.160	8.269	483673	15329526	0.870	1.044



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110518\
Data File : PD050188.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 15:42
Operator : AJ\SJ
Sample : MIREX-MDL-W-07
Misc : FOR MIREX
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-07

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 05:03:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

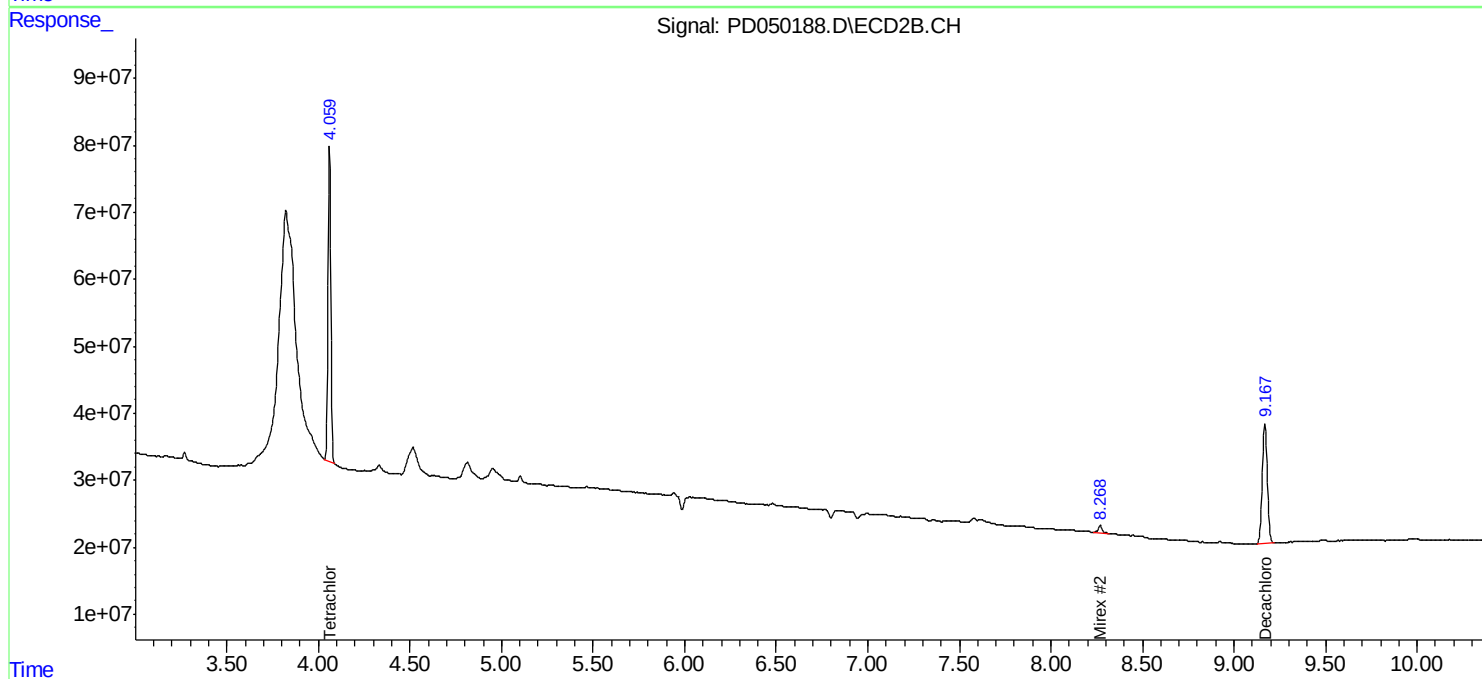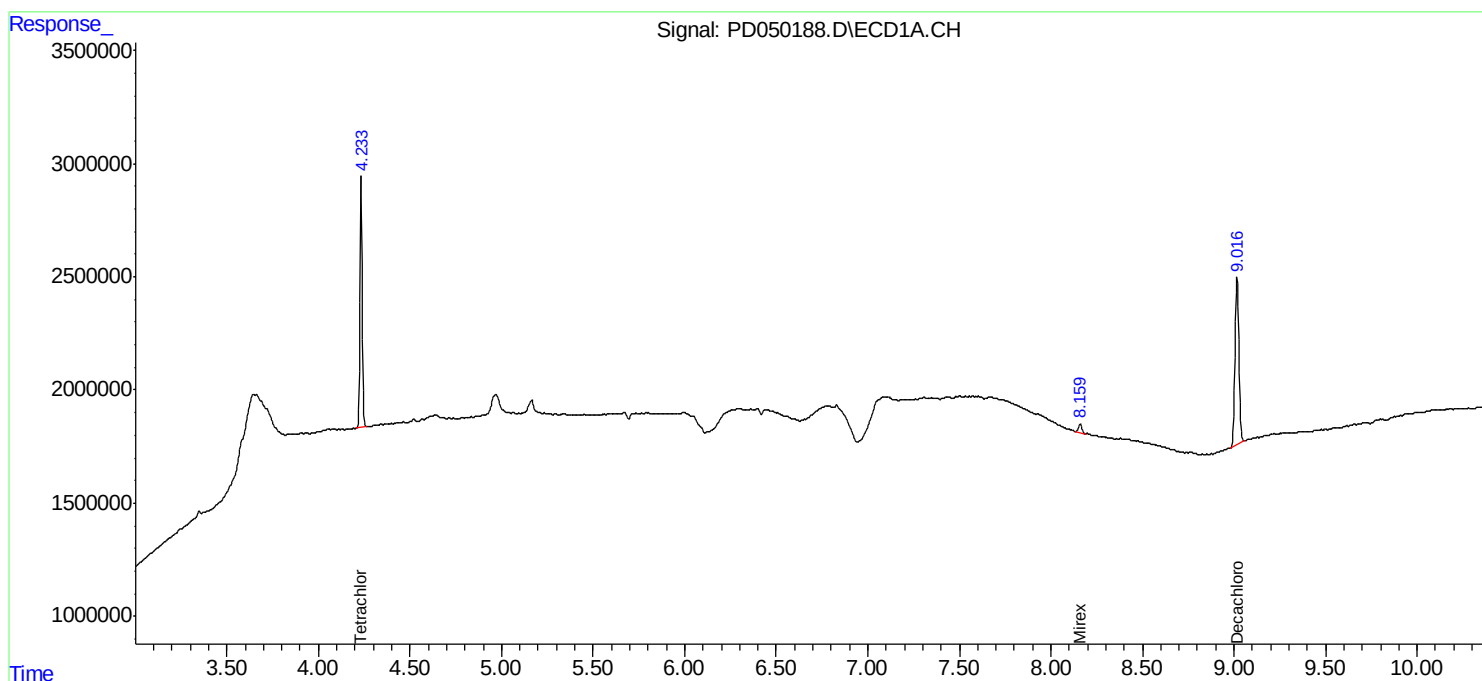


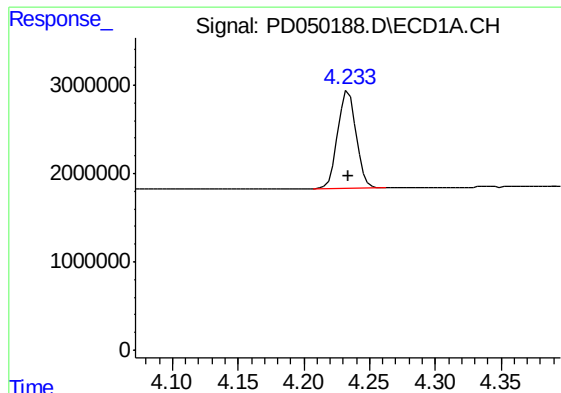

#1 Tetrachloro-m-xylene


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 10579068
Conc: 16.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-07

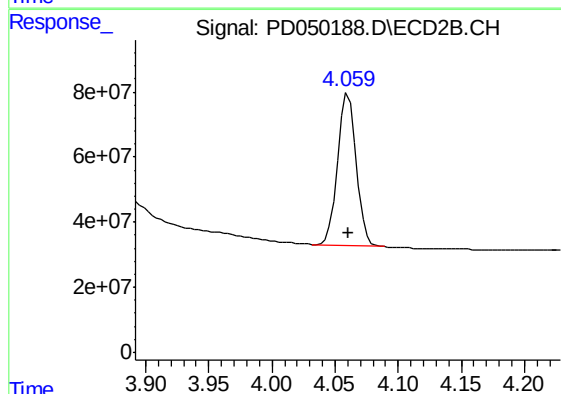


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 479893566
Conc: 17.27 ng/ml

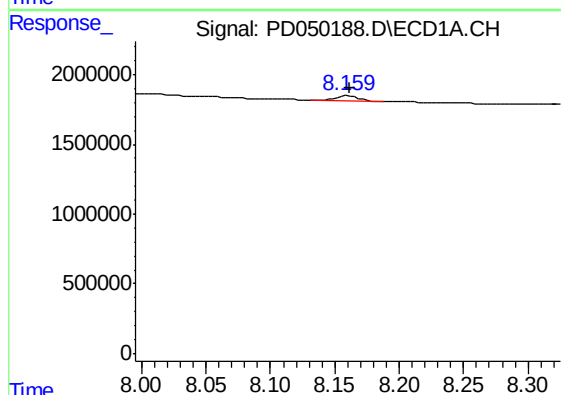


#22 Mirex

R.T.: 8.160 min
Delta R.T.: -0.002 min
Response: 483673
Conc: 0.87 ng/ml

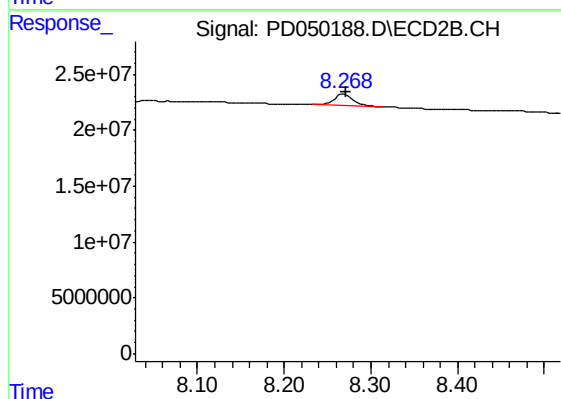

#22 Mirex


R.T.: 8.269 min
Delta R.T.: -0.003 min
Response: 15329526
Conc: 1.04 ng/ml

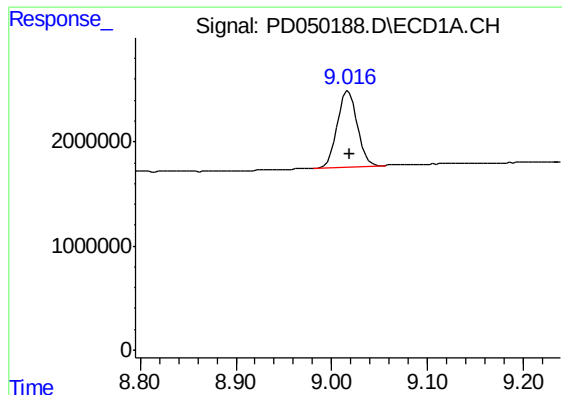

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.001 min
Response: 10564370
Conc: 17.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-07

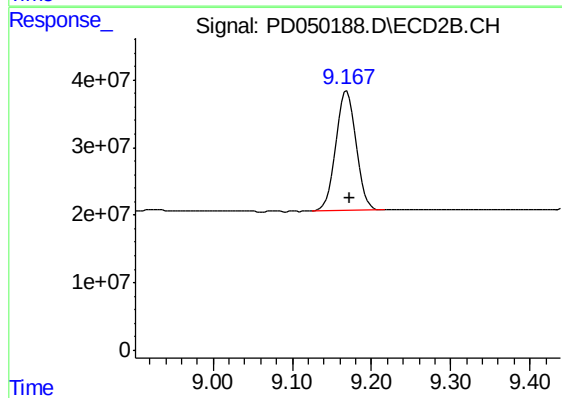

#28 Decachlorobiphenyl

R.T.: 9.169 min
Delta R.T.: -0.004 min
Response: 326009722
Conc: 18.84 ng/ml