

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110521\
 Data File : PD066746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2021 13:41
 Operator : AR\AJ
 Sample : M4412-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG372

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/08/2021
 Supervised By :mohammad ahmed 11/08/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 05:40:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.438	3.968	36044044	154.8E6	18.646	17.873
2) SA Decachlor...	8.163	9.023	41096107	213.5E6	35.075	40.937
Target Compounds						
19) B Endosulfa...	6.624	7.229	1761574	4603193	0.966	0.668 #
20) A Methoxychlor	6.861	7.547	7796676	27897357	8.319m	8.632

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110521\
Data File : PD066746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2021 13:41
Operator : AR\AJ
Sample : M4412-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 05:40:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

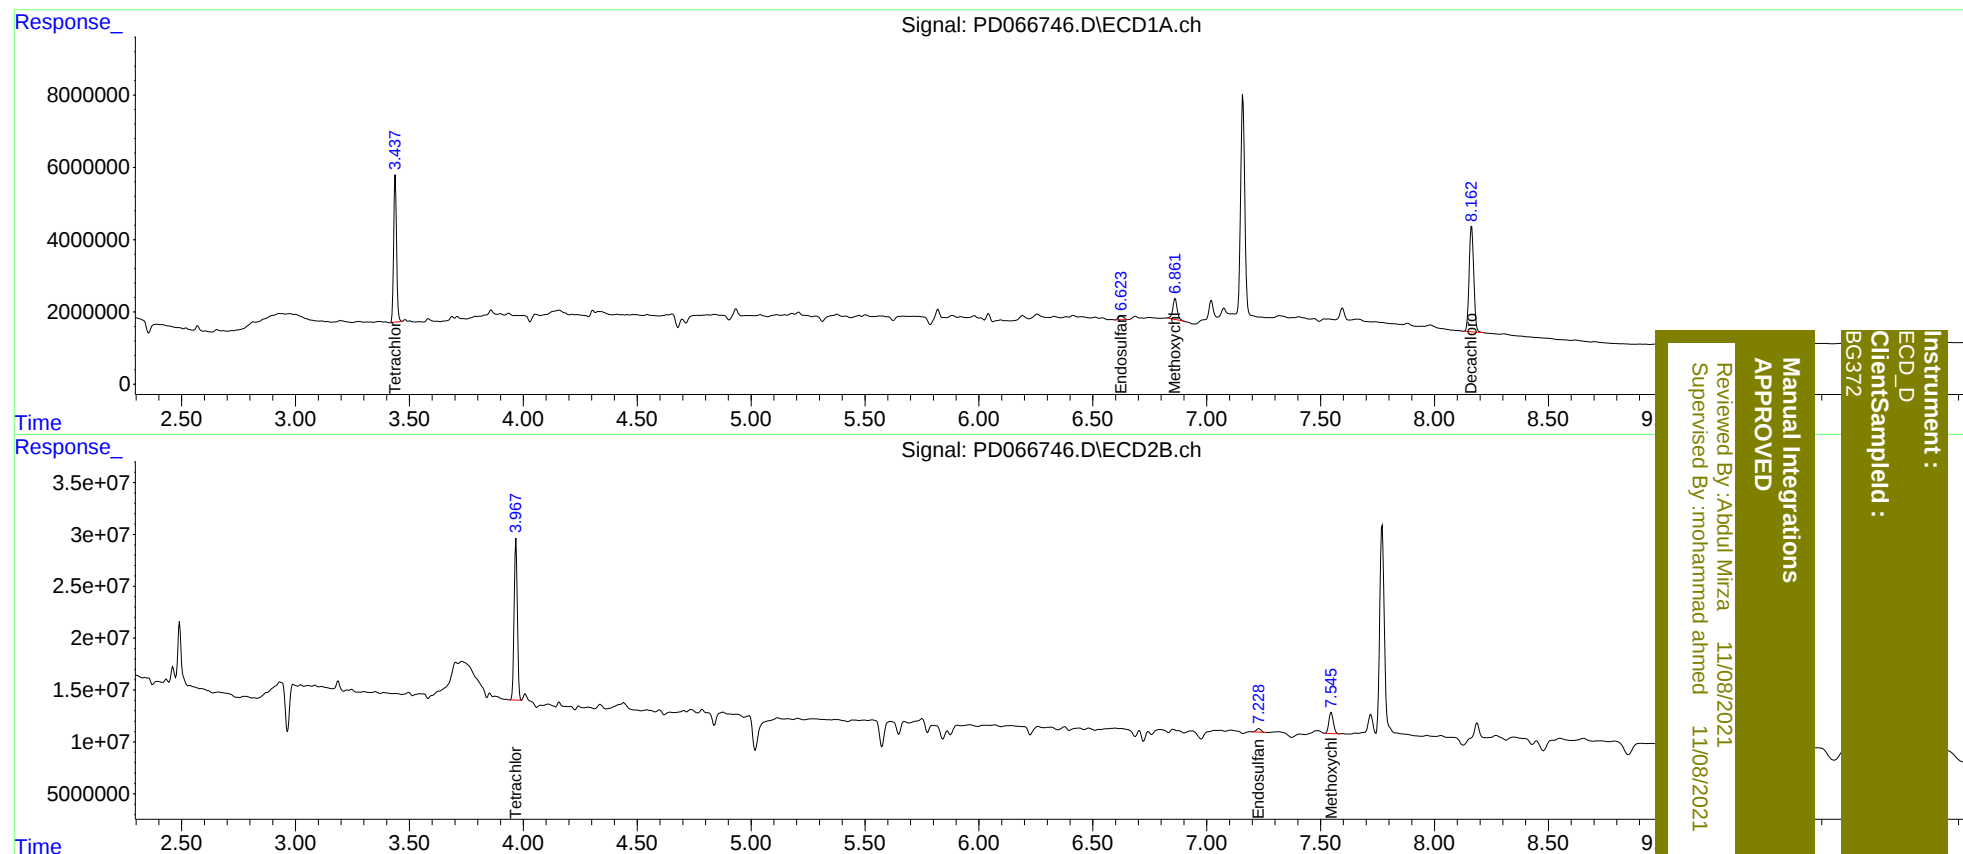

Reviewed By: Abdul Miza 11/08/2021
Supervised By: mohammad ahmed 11/08/2021

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BG372