

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110523\
 Data File : PD079413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 13:29
 Operator : AR\AJ
 Sample : PB156704BSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:16:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.803	24106906	36815406	14.931	15.901
28)	SA Decachlor...	9.111	7.949	33144572	45709565	16.523	18.753
Target Compounds							
2)	A alpha-BHC	4.024	3.306	21375820	30792223	8.030	8.880
3)	MA gamma-BHC...	4.357	3.636	20594741	30009384	7.925	8.837
4)	MA Heptachlor	4.950	3.978	23154801	30894616	8.656	10.116
5)	MB Aldrin	5.294	4.259	21352508	33936385	8.286	10.374 #
6)	B beta-BHC	4.550	3.931	10242508	14724707	9.558	10.450
7)	B delta-BHC	4.801	4.162	18796557	31505450	7.021	9.410 #
8)	B Heptachlo...	5.719	4.761	23901648	28251360	10.198	9.529
9)	A Endosulfan I	6.106	5.131	20109792	23987904	9.276	9.060
10)	B gamma-Chl...	5.976	5.011	23086306	26723745	10.069	9.313
11)	B alpha-Chl...	6.056	5.076	21087367	27367884	9.248	9.536
12)	B 4,4'-DDE	6.226	5.265	17440591	25249815	8.254	9.484
13)	MA Dieldrin	6.382	5.396	18854296	27613904	8.096	9.298
14)	MA Endrin	6.612	5.671	17083496	25274342	8.772	9.876
15)	B Endosulfa...	6.829	5.963	16785253	23367060	8.230	9.360
16)	A 4,4'-DDD	6.743	5.818	16554262	22283795	9.417	9.755
17)	MA 4,4'-DDT	7.058	6.070	13294352	20165813	7.020	8.808 #
18)	B Endrin al...	6.959	6.143	9501878	17370095	6.153	9.342 #
19)	B Endosulfa...	7.193	6.365	15960290	23466277	8.028	10.051 #
20)	A Methoxychlor	7.531	6.644	6989899	12196104	6.379	8.983 #
21)	B Endrin ke...	7.680	6.871	18387346	25096857	8.434	8.977
22)	Mirex	8.157	7.057	18171857	26303182	10.736	12.312
23)	Chlordane-1	0.000	3.837f	0	277026	N.D.	3.190 #
24)	Chlordane-2	5.294f	0.000	21352508	0	267.482	N.D. #
25)	Chlordane-3	5.976	5.011	23086306	26723745	74.471	100.190 #
26)	Chlordane-4	6.056	5.076	21087367	27367884	56.759	111.533 #
27)	Chlordane-5	0.000	5.963	0	23367060	N.D.	234.458 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110523\
Data File : PD079413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 13:29
Operator : AR\AJ
Sample : PB156704BSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:16:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

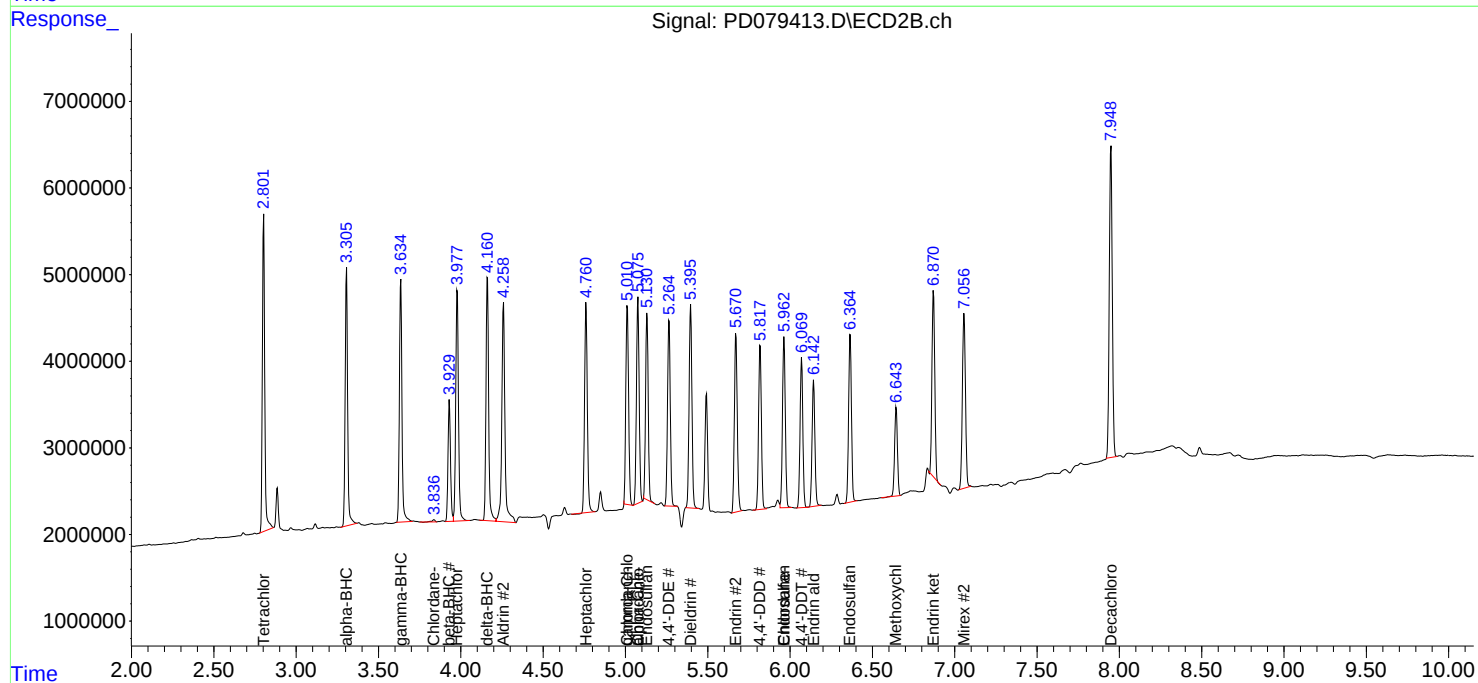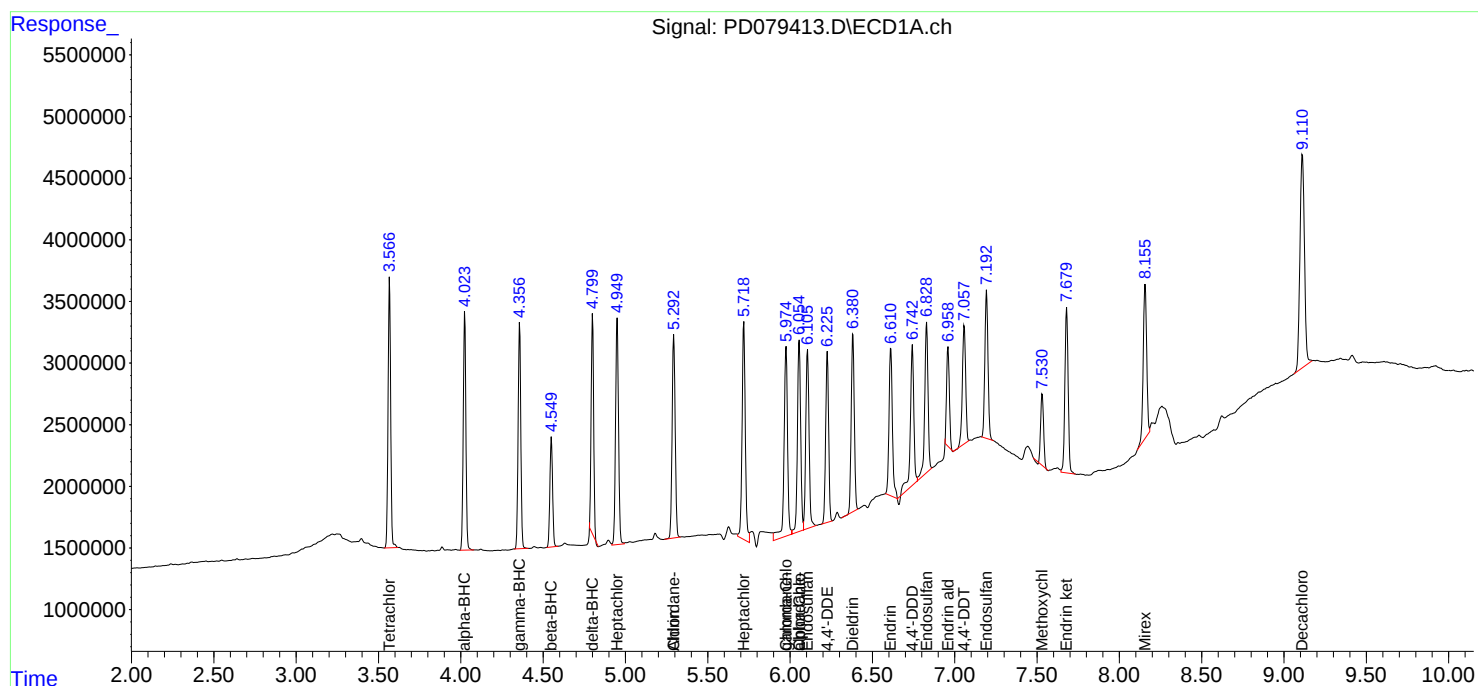


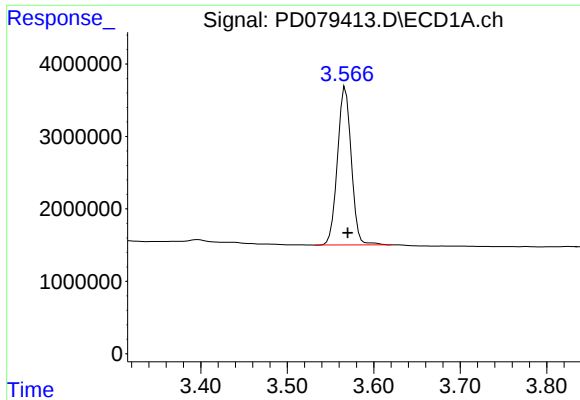

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: -0.003 min
Response: 24106906
Conc: 14.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

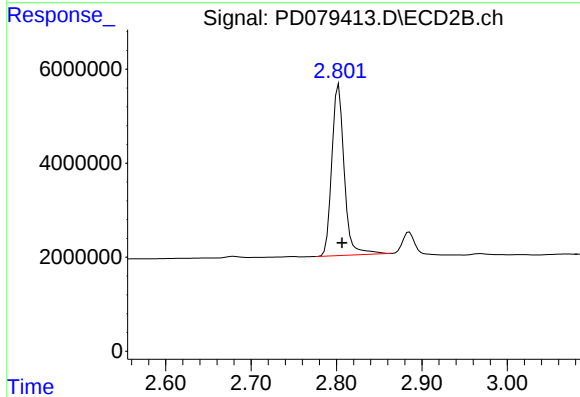


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: -0.004 min
Response: 36815406
Conc: 15.90 ng/ml

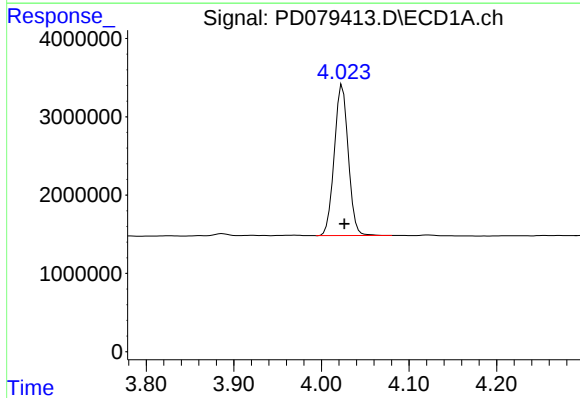


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: -0.002 min
Response: 21375820
Conc: 8.03 ng/ml

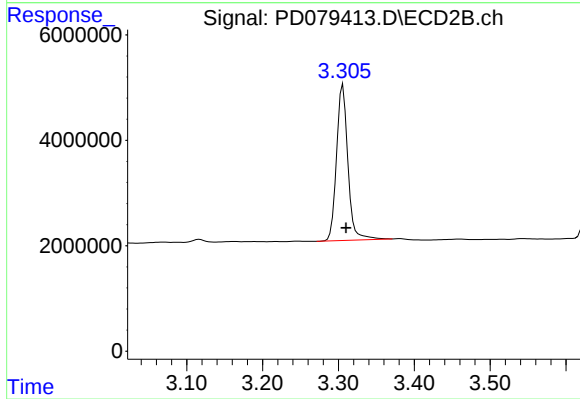

#2 alpha-BHC


R.T.: 3.306 min
Delta R.T.: -0.004 min
Response: 30792223
Conc: 8.88 ng/ml

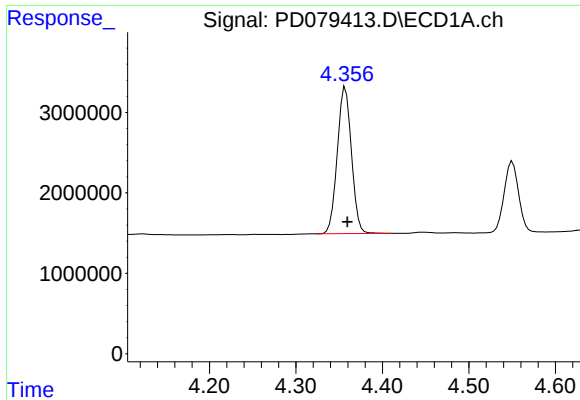

#3 gamma-BHC (Lindane)


R.T.: 4.357 min
Delta R.T.: -0.002 min
Response: 20594741
Conc: 7.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

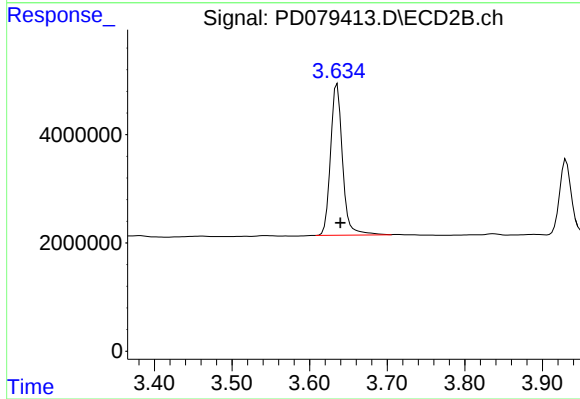


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: -0.004 min
Response: 30009384
Conc: 8.84 ng/ml

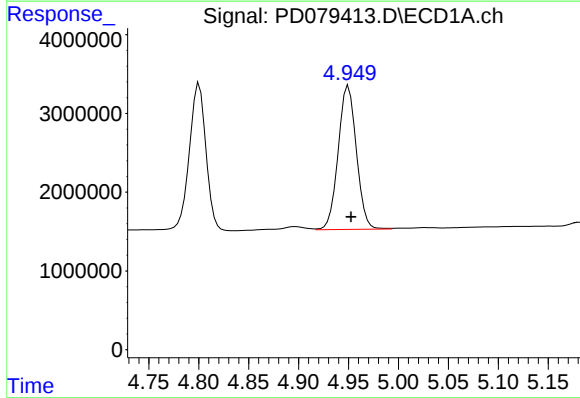


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: -0.003 min
Response: 23154801
Conc: 8.66 ng/ml

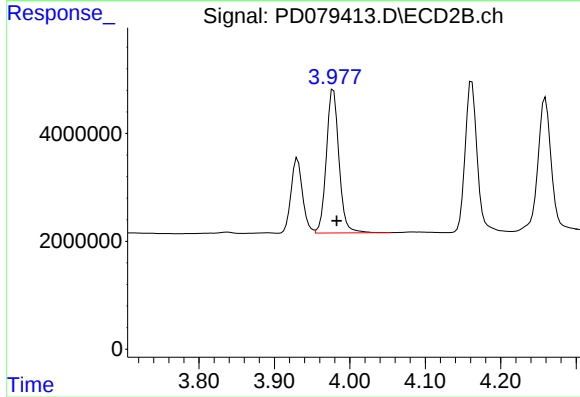

#4 Heptachlor


R.T.: 3.978 min
Delta R.T.: -0.004 min
Response: 30894616
Conc: 10.12 ng/ml

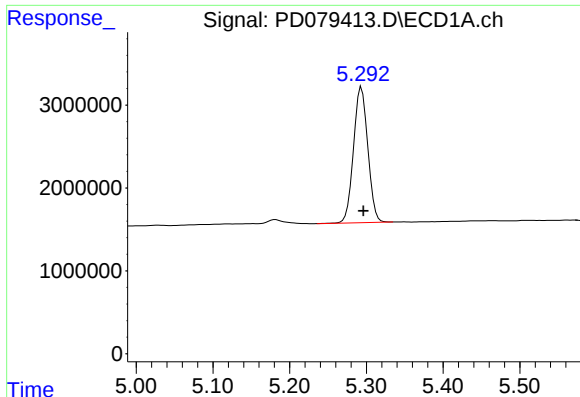

#5 Aldrin


R.T.: 5.294 min
Delta R.T.: -0.002 min
Response: 21352508
Conc: 8.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

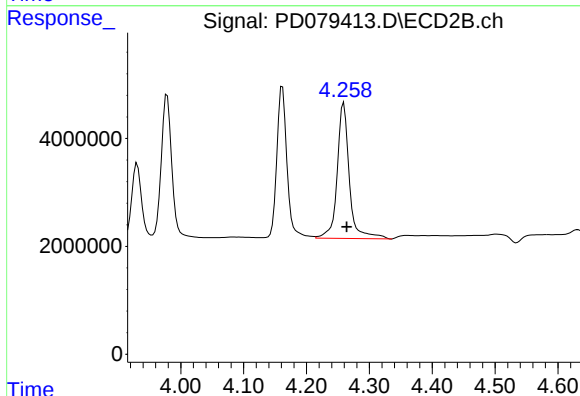


#5 Aldrin

R.T.: 4.259 min
Delta R.T.: -0.005 min
Response: 33936385
Conc: 10.37 ng/ml

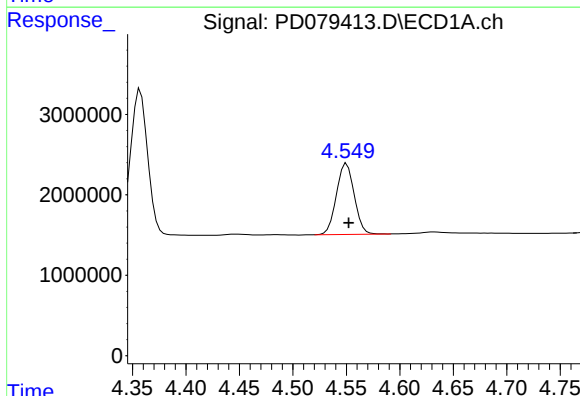


#6 beta-BHC

R.T.: 4.550 min
Delta R.T.: -0.002 min
Response: 10242508
Conc: 9.56 ng/ml

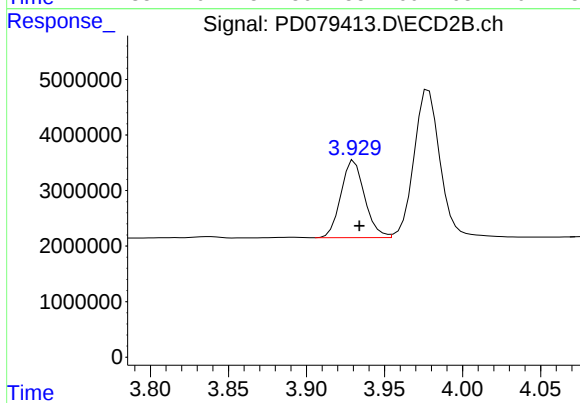

#6 beta-BHC


R.T.: 3.931 min
Delta R.T.: -0.003 min
Response: 14724707
Conc: 10.45 ng/ml

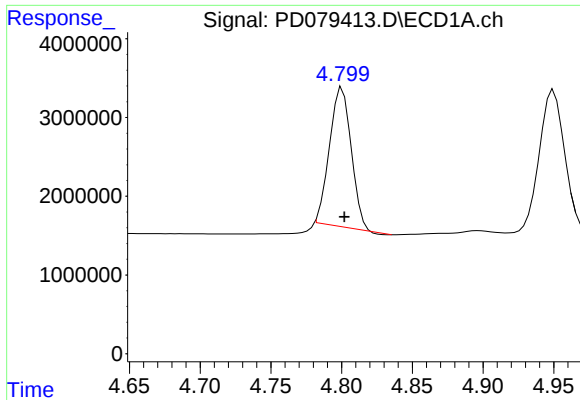

#7 delta-BHC


R.T.: 4.801 min
Delta R.T.: -0.001 min
Response: 18796557
Conc: 7.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

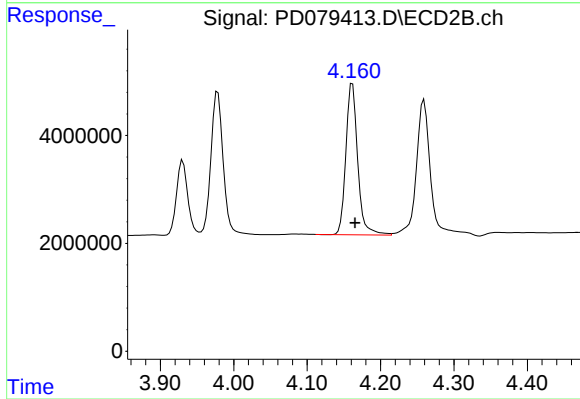


#7 delta-BHC

R.T.: 4.162 min
Delta R.T.: -0.004 min
Response: 31505450
Conc: 9.41 ng/ml

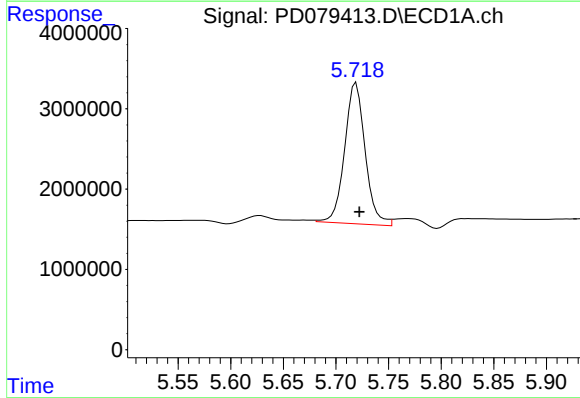


#8 Heptachlor epoxide

R.T.: 5.719 min
Delta R.T.: -0.003 min
Response: 23901648
Conc: 10.20 ng/ml

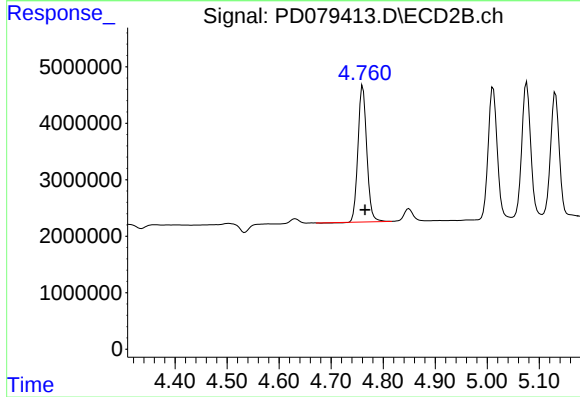

#8 Heptachlor epoxide


R.T.: 4.761 min
Delta R.T.: -0.005 min
Response: 28251360
Conc: 9.53 ng/ml

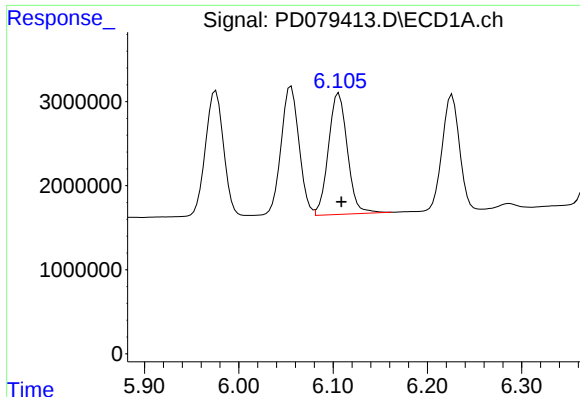

#9 Endosulfan I


R.T.: 6.106 min
Delta R.T.: -0.003 min
Response: 20109792
Conc: 9.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

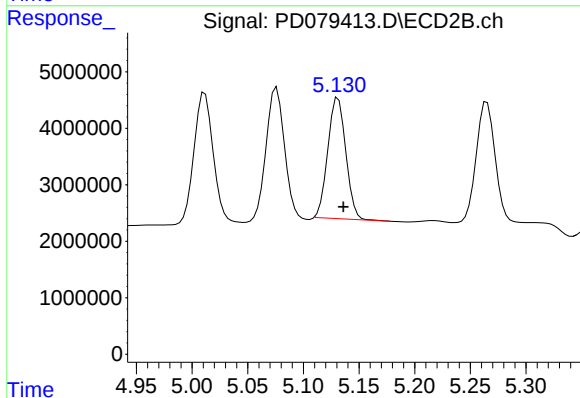


#9 Endosulfan I

R.T.: 5.131 min
Delta R.T.: -0.005 min
Response: 23987904
Conc: 9.06 ng/ml

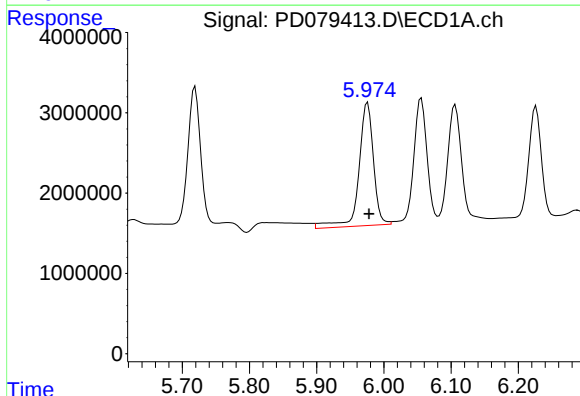


#10 gamma-Chlordane

R.T.: 5.976 min
Delta R.T.: -0.002 min
Response: 23086306
Conc: 10.07 ng/ml

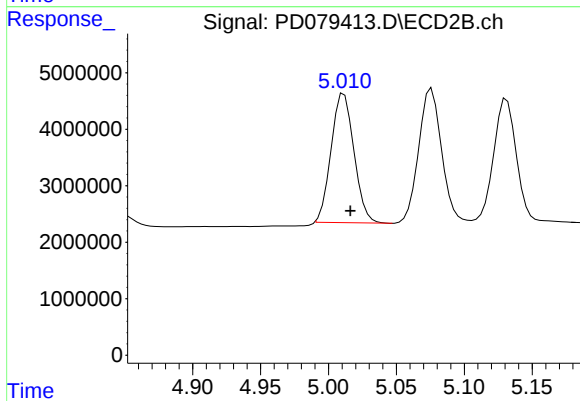

#10 gamma-Chlordane


R.T.: 5.011 min
Delta R.T.: -0.005 min
Response: 26723745
Conc: 9.31 ng/ml

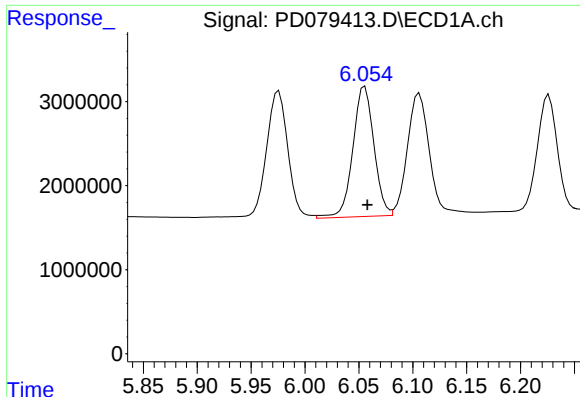

#11 alpha-Chlordane


R.T.: 6.056 min
Delta R.T.: -0.002 min
Response: 21087367
Conc: 9.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

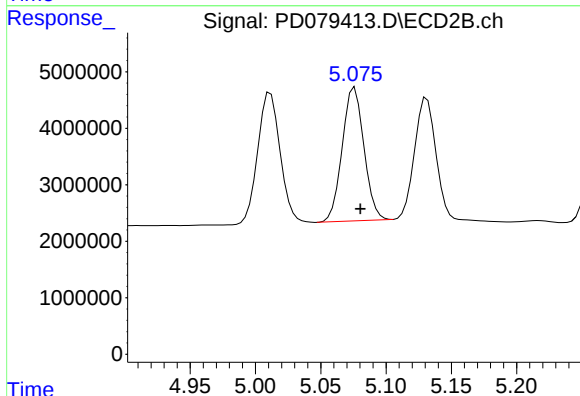


#11 alpha-Chlordane

R.T.: 5.076 min
Delta R.T.: -0.004 min
Response: 27367884
Conc: 9.54 ng/ml

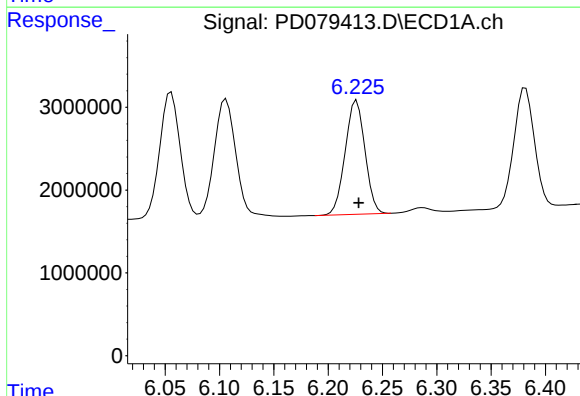


#12 4,4'-DDE

R.T.: 6.226 min
Delta R.T.: -0.002 min
Response: 17440591
Conc: 8.25 ng/ml

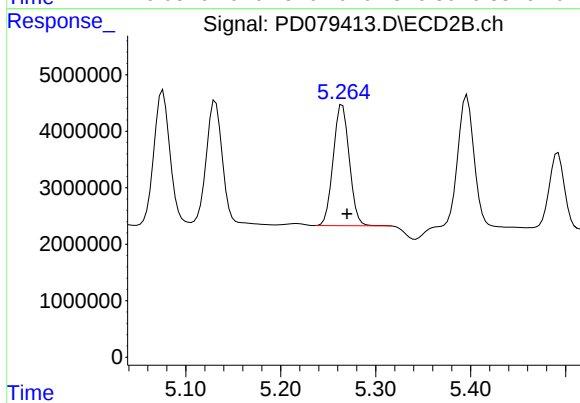

#12 4,4'-DDE


R.T.: 5.265 min
Delta R.T.: -0.005 min
Response: 25249815
Conc: 9.48 ng/ml

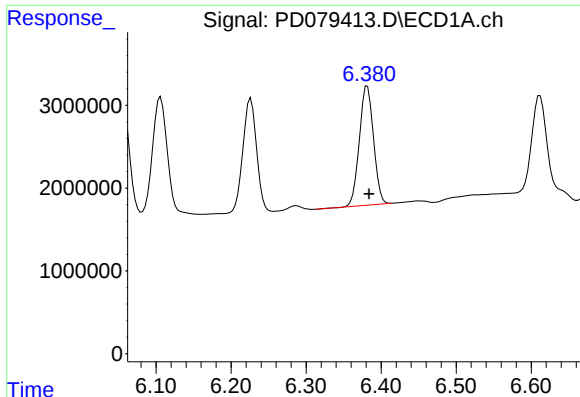

#13 Dieldrin


R.T.: 6.382 min
Delta R.T.: -0.002 min
Response: 18854296
Conc: 8.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

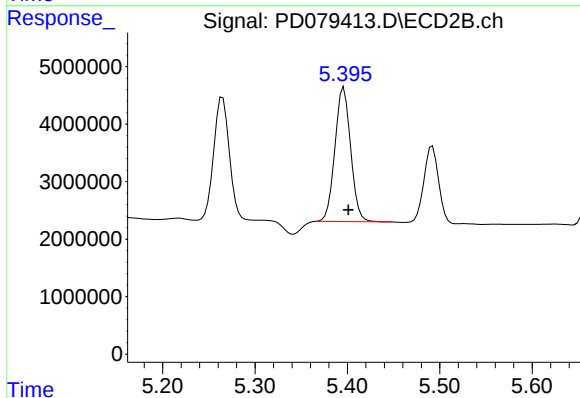


#13 Dieldrin

R.T.: 5.396 min
Delta R.T.: -0.005 min
Response: 27613904
Conc: 9.30 ng/ml

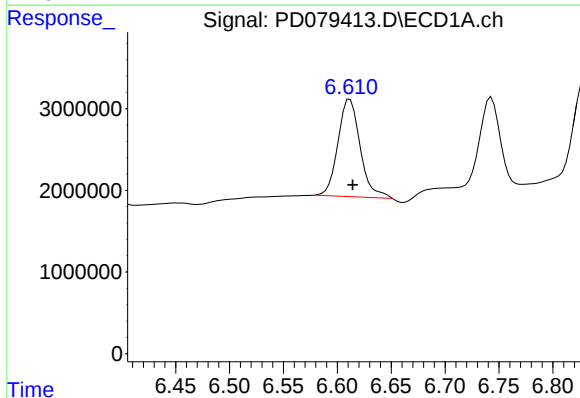


#14 Endrin

R.T.: 6.612 min
Delta R.T.: -0.002 min
Response: 17083496
Conc: 8.77 ng/ml

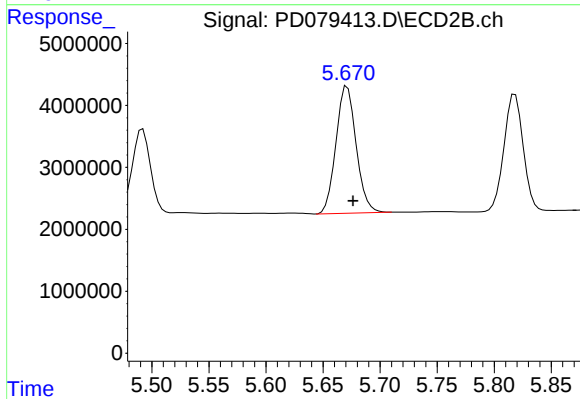

#14 Endrin


R.T.: 5.671 min
Delta R.T.: -0.005 min
Response: 25274342
Conc: 9.88 ng/ml

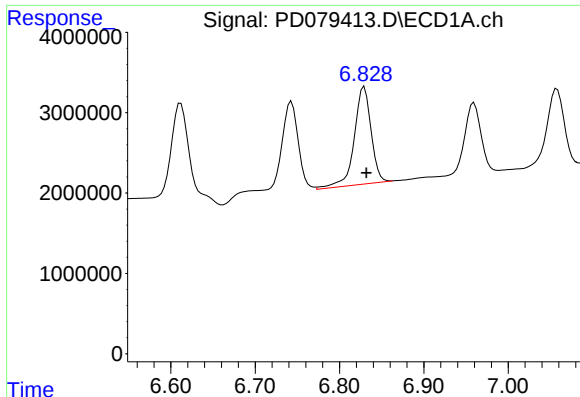

#15 Endosulfan II


R.T.: 6.829 min
Delta R.T.: -0.002 min
Response: 16785253
Conc: 8.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

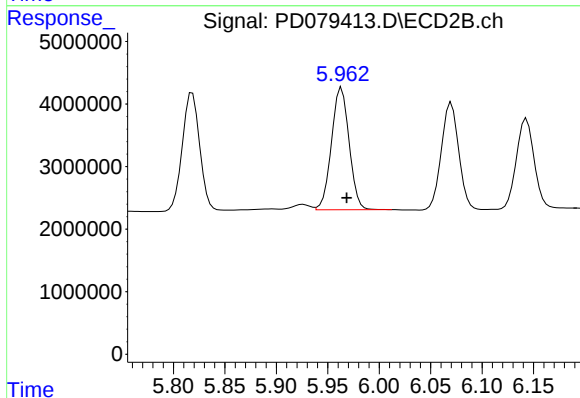


#15 Endosulfan II

R.T.: 5.963 min
Delta R.T.: -0.005 min
Response: 23367060
Conc: 9.36 ng/ml

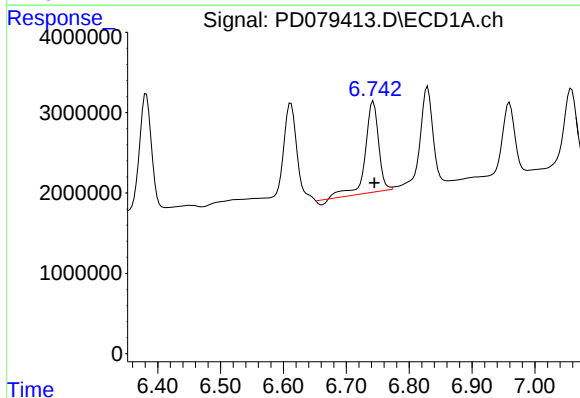


#16 4,4'-DDD

R.T.: 6.743 min
Delta R.T.: -0.002 min
Response: 16554262
Conc: 9.42 ng/ml

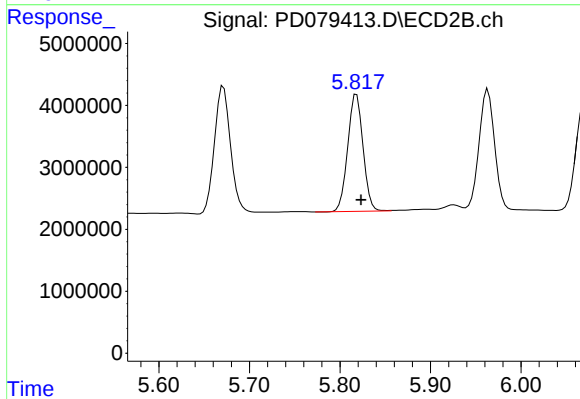

#16 4,4'-DDD


R.T.: 5.818 min
Delta R.T.: -0.005 min
Response: 22283795
Conc: 9.76 ng/ml

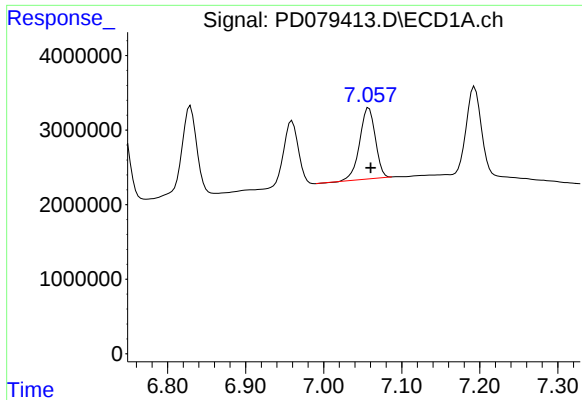

#17 4,4'-DDT


R.T.: 7.058 min
Delta R.T.: -0.002 min
Response: 13294352
Conc: 7.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

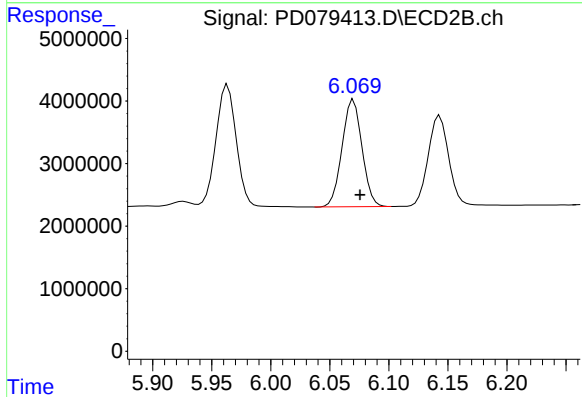


#17 4,4'-DDT

R.T.: 6.070 min
Delta R.T.: -0.005 min
Response: 20165813
Conc: 8.81 ng/ml

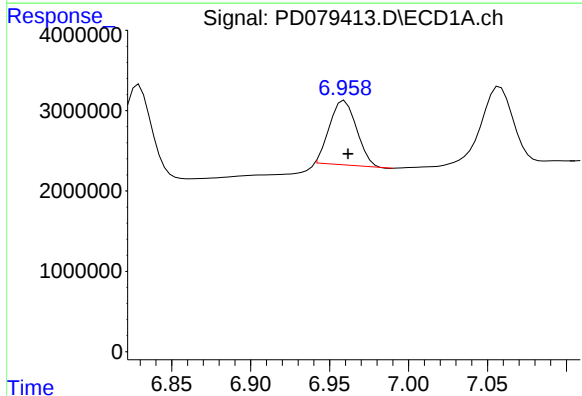


#18 Endrin aldehyde

R.T.: 6.959 min
Delta R.T.: -0.002 min
Response: 9501878
Conc: 6.15 ng/ml

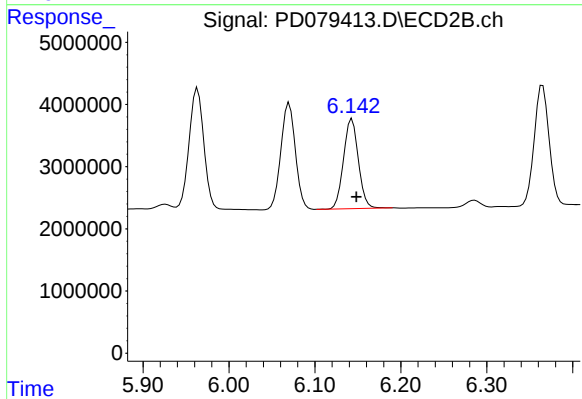

#18 Endrin aldehyde


R.T.: 6.143 min
Delta R.T.: -0.005 min
Response: 17370095
Conc: 9.34 ng/ml

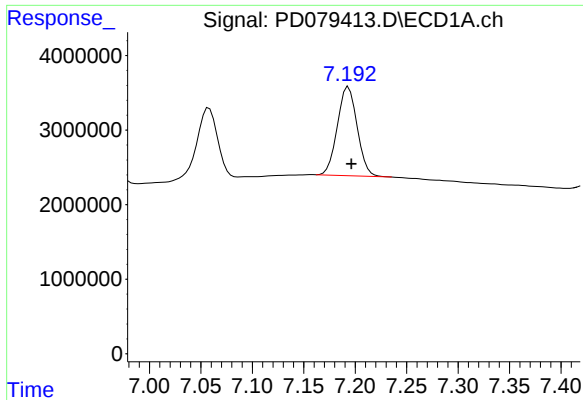

#19 Endosulfan Sulfate


R.T.: 7.193 min
Delta R.T.: -0.003 min
Response: 15960290
Conc: 8.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

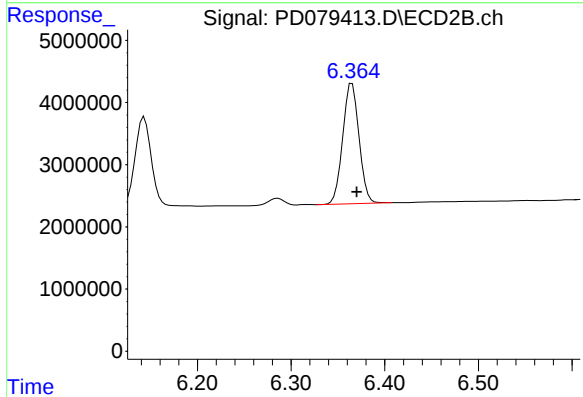


#19 Endosulfan Sulfate

R.T.: 6.365 min
Delta R.T.: -0.005 min
Response: 23466277
Conc: 10.05 ng/ml

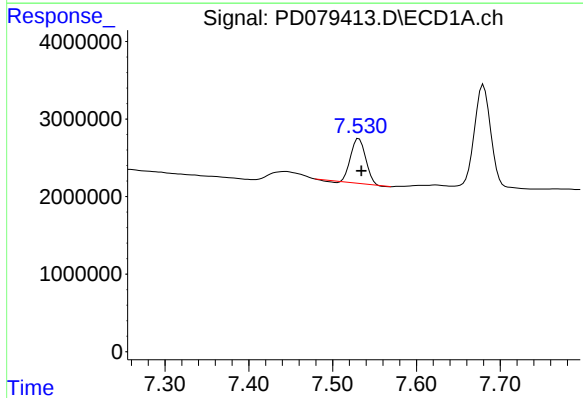


#20 Methoxychlor

R.T.: 7.531 min
Delta R.T.: -0.003 min
Response: 6989899
Conc: 6.38 ng/ml

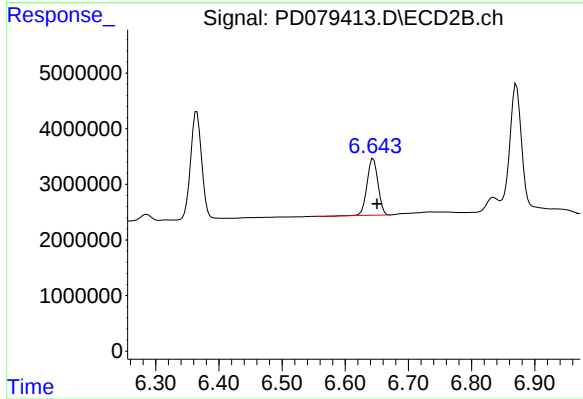

#20 Methoxychlor


R.T.: 6.644 min
Delta R.T.: -0.006 min
Response: 12196104
Conc: 8.98 ng/ml

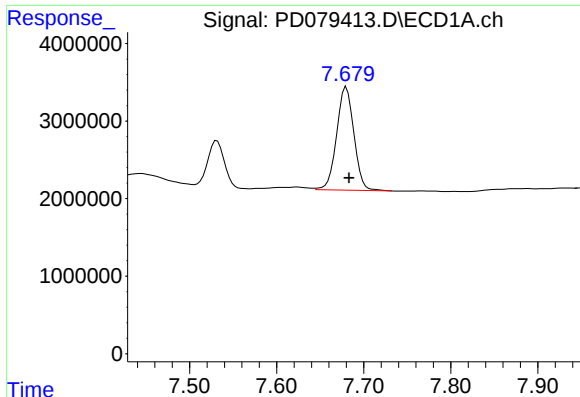

#21 Endrin ketone


R.T.: 7.680 min
Delta R.T.: -0.003 min
Response: 18387346
Conc: 8.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

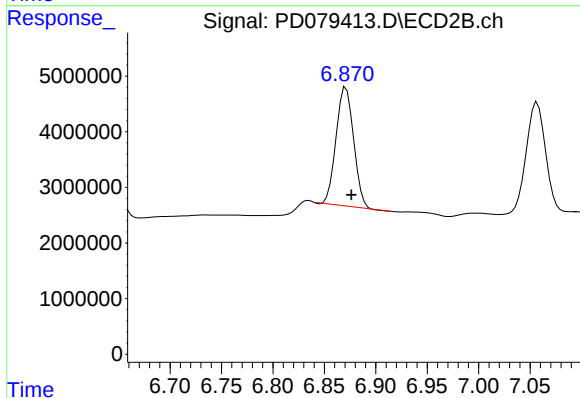


#21 Endrin ketone

R.T.: 6.871 min
Delta R.T.: -0.005 min
Response: 25096857
Conc: 8.98 ng/ml

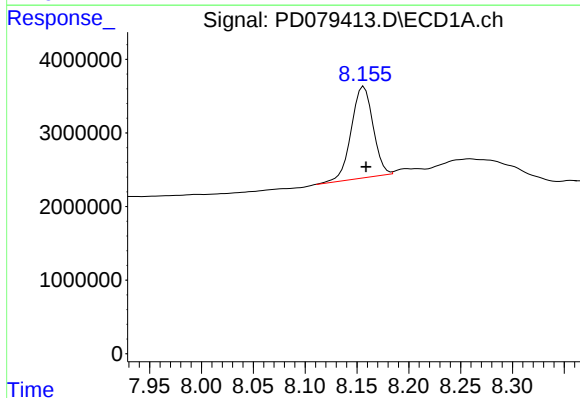


#22 Mirex

R.T.: 8.157 min
Delta R.T.: -0.002 min
Response: 18171857
Conc: 10.74 ng/ml

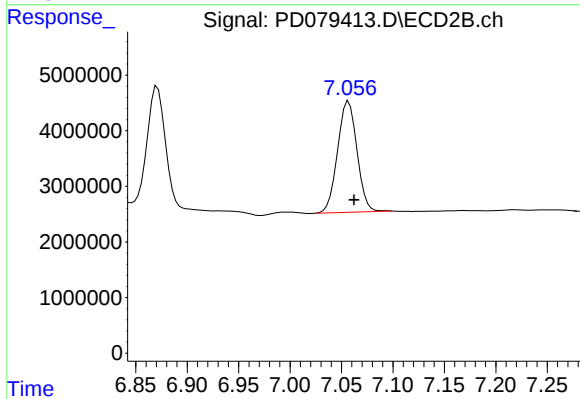

#22 Mirex


R.T.: 7.057 min
Delta R.T.: -0.005 min
Response: 26303182
Conc: 12.31 ng/ml

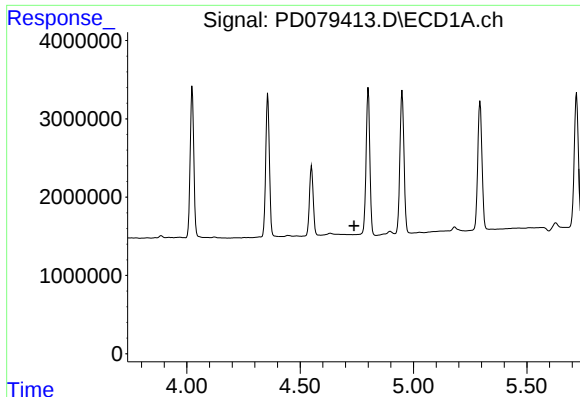

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.738 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

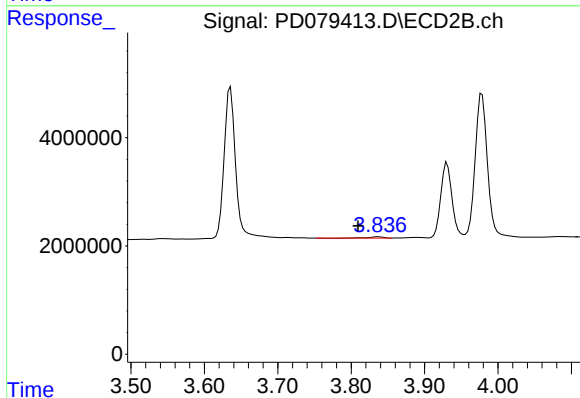


#23 Chlordane-1

R.T.: 3.837 min
Delta R.T.: 0.028 min
Response: 277026
Conc: 3.19 ng/ml

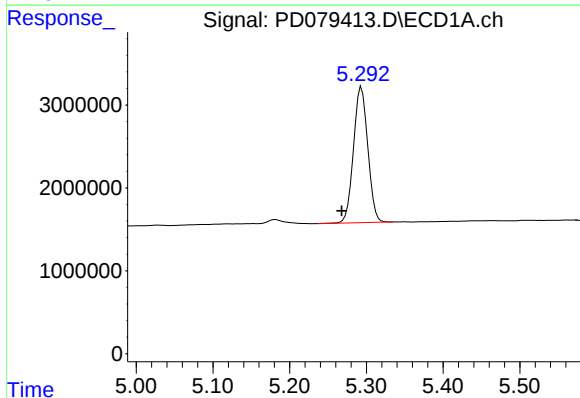


#24 Chlordane-2

R.T.: 5.294 min
Delta R.T.: 0.026 min
Response: 21352508
Conc: 267.48 ng/ml

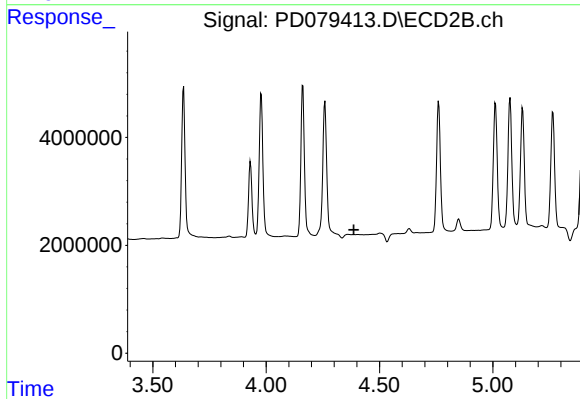

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.386 min
Response: 0
Conc: N.D.

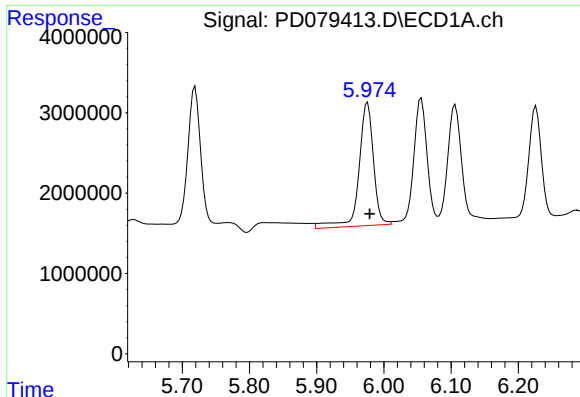

#25 Chlordane-3


R.T.: 5.976 min
Delta R.T.: -0.004 min
Response: 23086306
Conc: 74.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

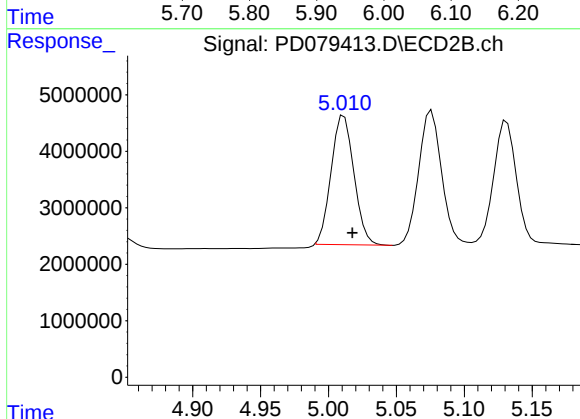


#25 Chlordane-3

R.T.: 5.011 min
Delta R.T.: -0.006 min
Response: 26723745
Conc: 100.19 ng/ml

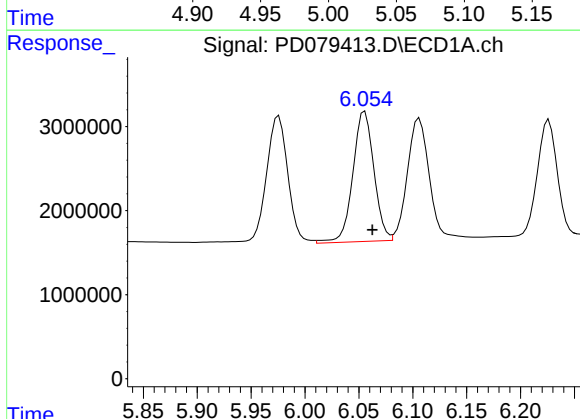


#26 Chlordane-4

R.T.: 6.056 min
Delta R.T.: -0.007 min
Response: 21087367
Conc: 56.76 ng/ml

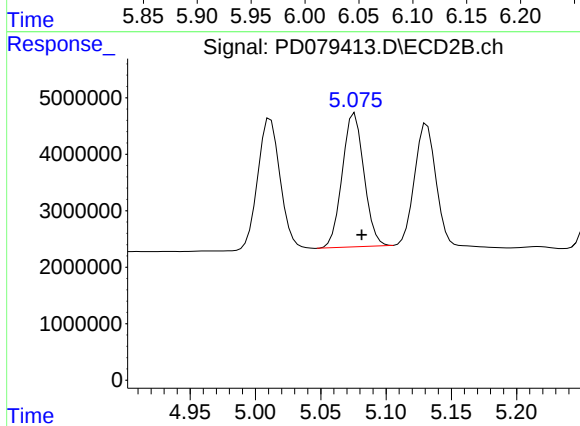

#26 Chlordane-4


R.T.: 5.076 min
Delta R.T.: -0.005 min
Response: 27367884
Conc: 111.53 ng/ml

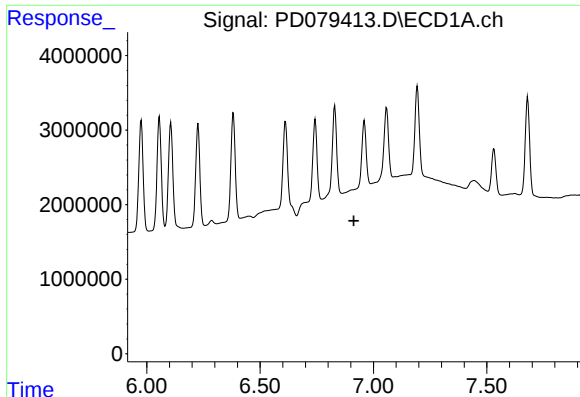

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

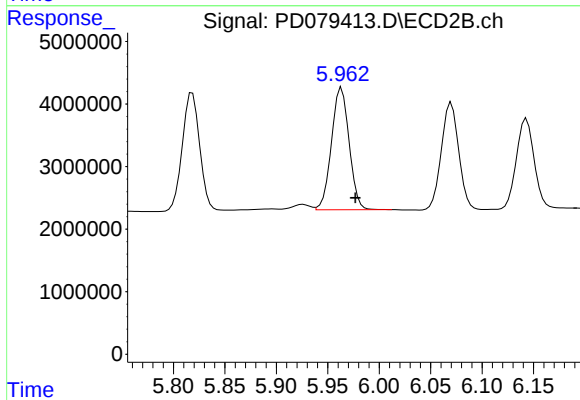


#27 Chlordane-5

R.T.: 5.963 min
Delta R.T.: -0.013 min
Response: 23367060
Conc: 234.46 ng/ml

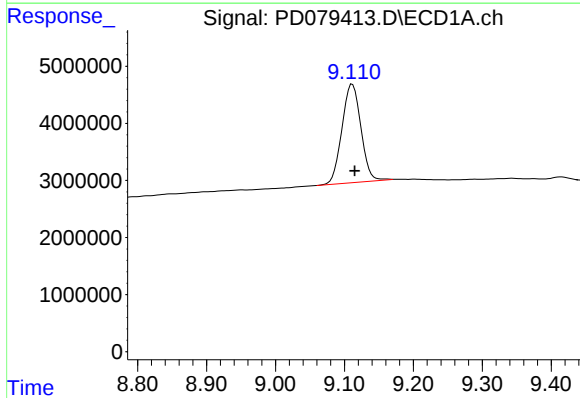

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.003 min
Response: 33144572
Conc: 16.52 ng/ml

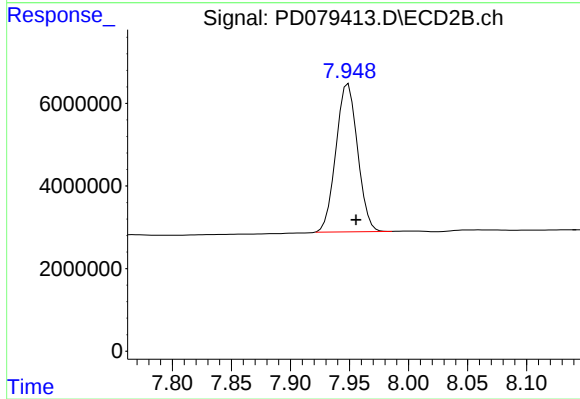

#28 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: -0.006 min
Response: 45709565
Conc: 18.75 ng/ml