

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110524\
 Data File : PD086356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 15:10
 Operator : AR\AJ
 Sample : P4634-19MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CC0R7MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:23:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.888	19815842	140.9E6	15.051	15.186
27)	SA Decachlor...	9.092	8.096	22545488	123.4E6	12.576	13.053
Target Compounds							
2)	A alpha-BHC	4.011	3.402	138.6E6	732.7E6	55.689	50.996
3)	MA gamma-BHC...	4.343	3.739	136.7E6	677.0E6	54.949	50.193
4)	MA Heptachlor	4.944	4.096	131.7E6	655.7E6	53.268	47.993
5)	MB Aldrin	5.286	4.383	129.6E6	661.0E6	53.468	48.719
6)	B beta-BHC	4.526	4.034	52599534	277.5E6	47.363	44.258
7)	B delta-BHC	4.775	4.272	138.7E6	680.1E6	53.573	48.472
8)	B Heptachlo...	5.706	4.887	114.3E6	583.1E6	50.009	46.503
9)	A Endosulfan I	6.089	5.262	106.0E6	544.7E6	52.312	47.444
10)	B trans-Chl...	5.960	5.141	112.1E6	613.6E6	50.821	46.648
11)	B cis-Chlor...	6.042	5.206	114.0E6	596.2E6	51.571	46.940
12)	B 4,4'-DDE	6.210	5.391	222.4E6	1153.9E6	104.130	94.111
13)	MA Dieldrin	6.362	5.529	244.6E6	1167.9E6	107.247	94.662
14)	MA Endrin	6.589	5.804	200.8E6	1045.7E6	106.854	93.049
15)	B Endosulfa...	6.799	6.096	198.9E6	992.1E6	99.228	89.919
16)	A 4,4'-DDD	6.719	5.946	182.0E6	955.0E6	112.340	97.284
17)	MA 4,4'-DDT	7.035	6.201	174.0E6	901.9E6	104.345	87.893
18)	B Endrin al...	6.928	6.275	141.3E6	711.9E6	94.746	85.760
19)	B Endosulfa...	7.163	6.499	186.1E6	947.2E6	100.937	89.857
20)	A Methoxychlor	7.506	6.774	447.7E6	1946.4E6	475.701	409.483
21)	B Endrin ke...	7.643	7.008	207.8E6	1015.0E6	100.861	88.701

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110524\
Data File : PD086356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 15:10
Operator : AR\AJ
Sample : P4634-19MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:23:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

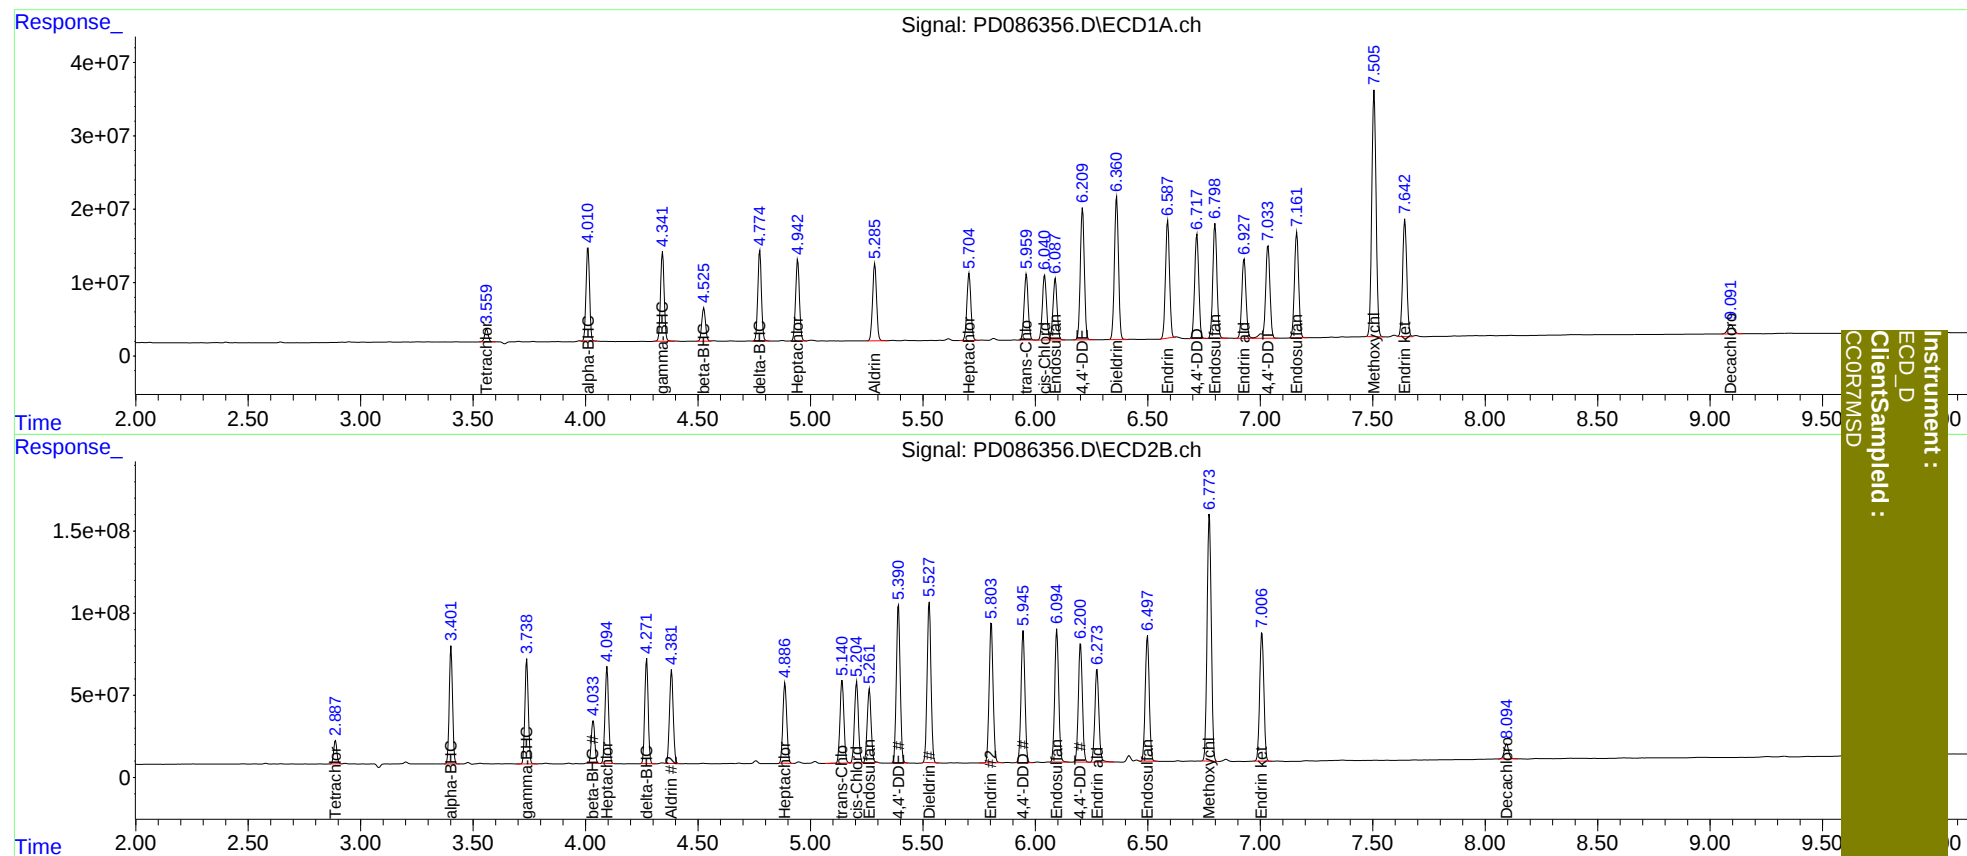

Instrument :
ECD_D
ClientSampled :
CC0R7MSD