

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110524\
 Data File : PD086341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 10:22
 Operator : AR\AJ
 Sample : P4634-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0P18

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/06/2024
 Supervised By : Ankita Jodhani 11/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:18:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.889	18142581	134.5E6	13.780m	14.500
27)	SA Decachlor...	9.094	8.095	20011762	119.7E6	11.163	12.658
Target Compounds							
9)	A Endosulfan I	6.112	5.263	763727	3616181	0.377	0.315
10)	B trans-Chl...	5.960	5.136	1653302	7032273	0.749m	0.535m#
11)	B cis-Chlor...	6.053	5.196	971202	26881179	0.439	2.116 #
16)	A 4,4'-DDD	6.712	5.943	772847	4390089	0.477	0.447
17)	MA 4,4'-DDT	7.034	6.198	1421616	5374133	0.853m	0.524m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:18:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

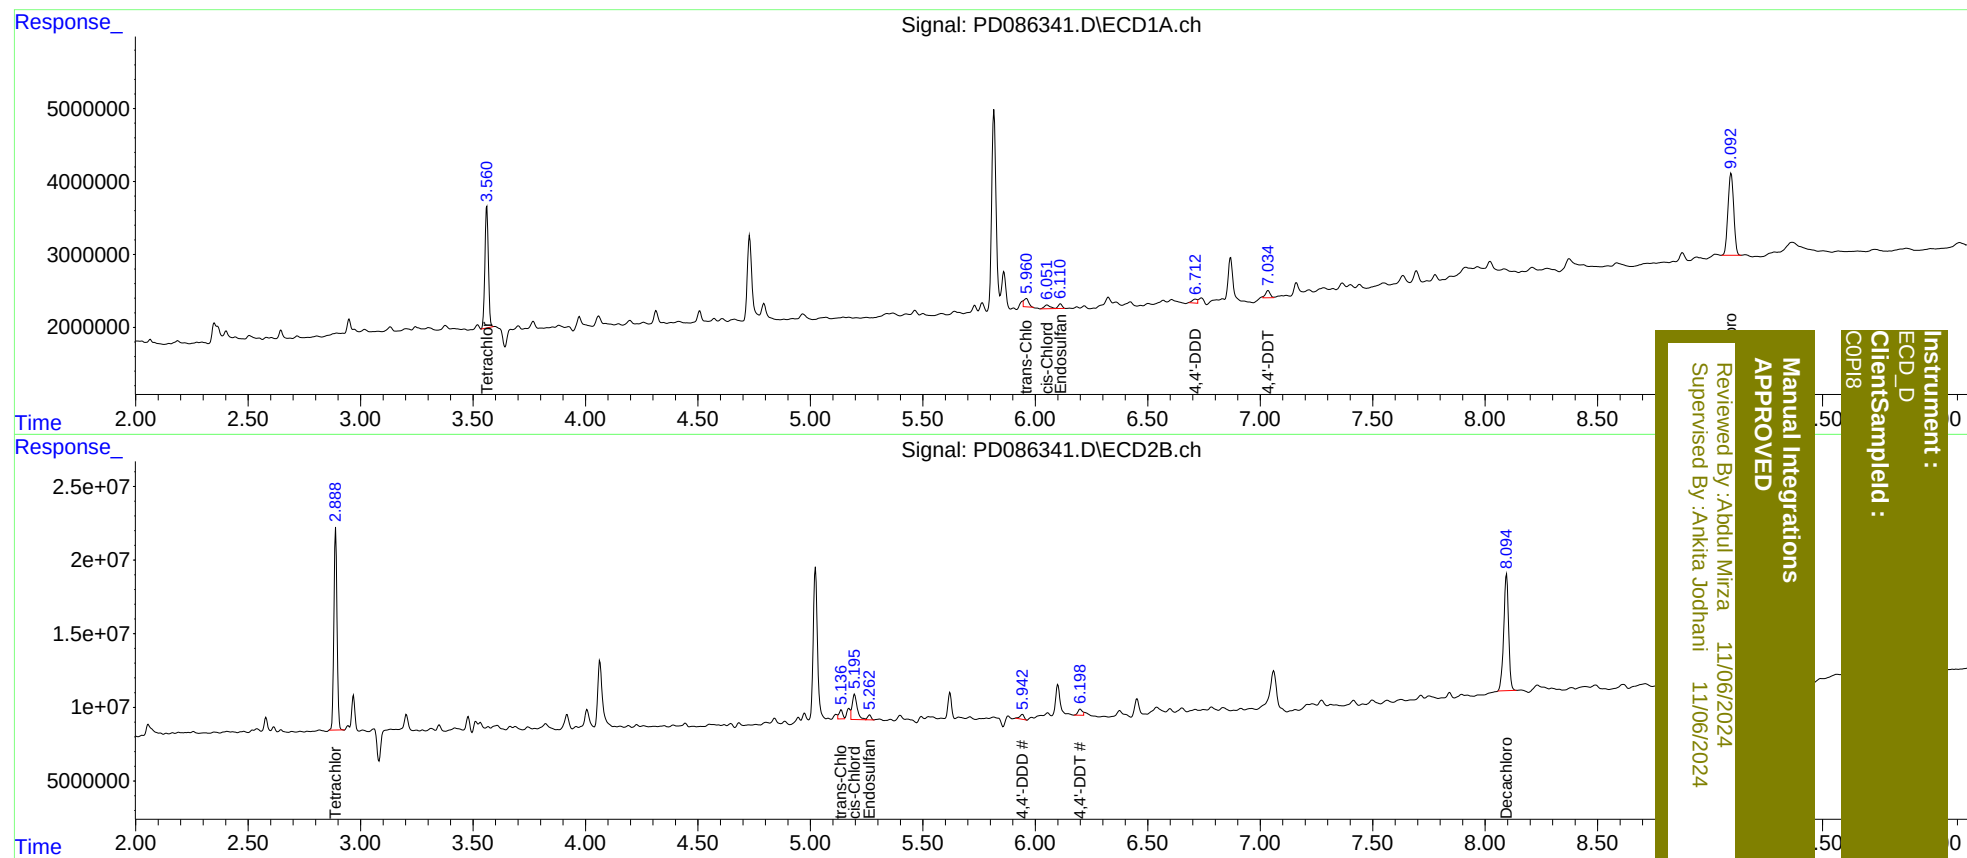

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/06/2024
Supervised By : Ankita Jodhani 11/06/2024

Instrument :
ECD_D
ClientSampled :
C0P18