

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110618\
 Data File : PD050194.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 18:37
 Operator : AJ\SJ
 Sample : TOXAPH101
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 02:50:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 06 02:50:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.060	3240258	153.4E6	5.004	5.372
27)	SA Decachlor...	9.017	9.168	7147190	217.6E6	10.522	11.301
Target Compounds							
22)	Toxaphene-1	6.526	6.462	2856630	75295723	487.802	564.089
23)	Toxaphene-2	6.695	6.754	3118269	86548606	488.752	544.831
24)	Toxaphene-3	7.129	7.162	6328715	118.2E6	482.561	539.819
25)	Toxaphene-4	7.375	7.419	6974105	77691697	468.320	524.938
26)	Toxaphene-5	7.854	7.739	6578847	141.6E6	491.208	550.271

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110618\
Data File : PD050194.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 18:37
Operator : AJ\SJ
Sample : TOXAPH101
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 02:50:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 06 02:50:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

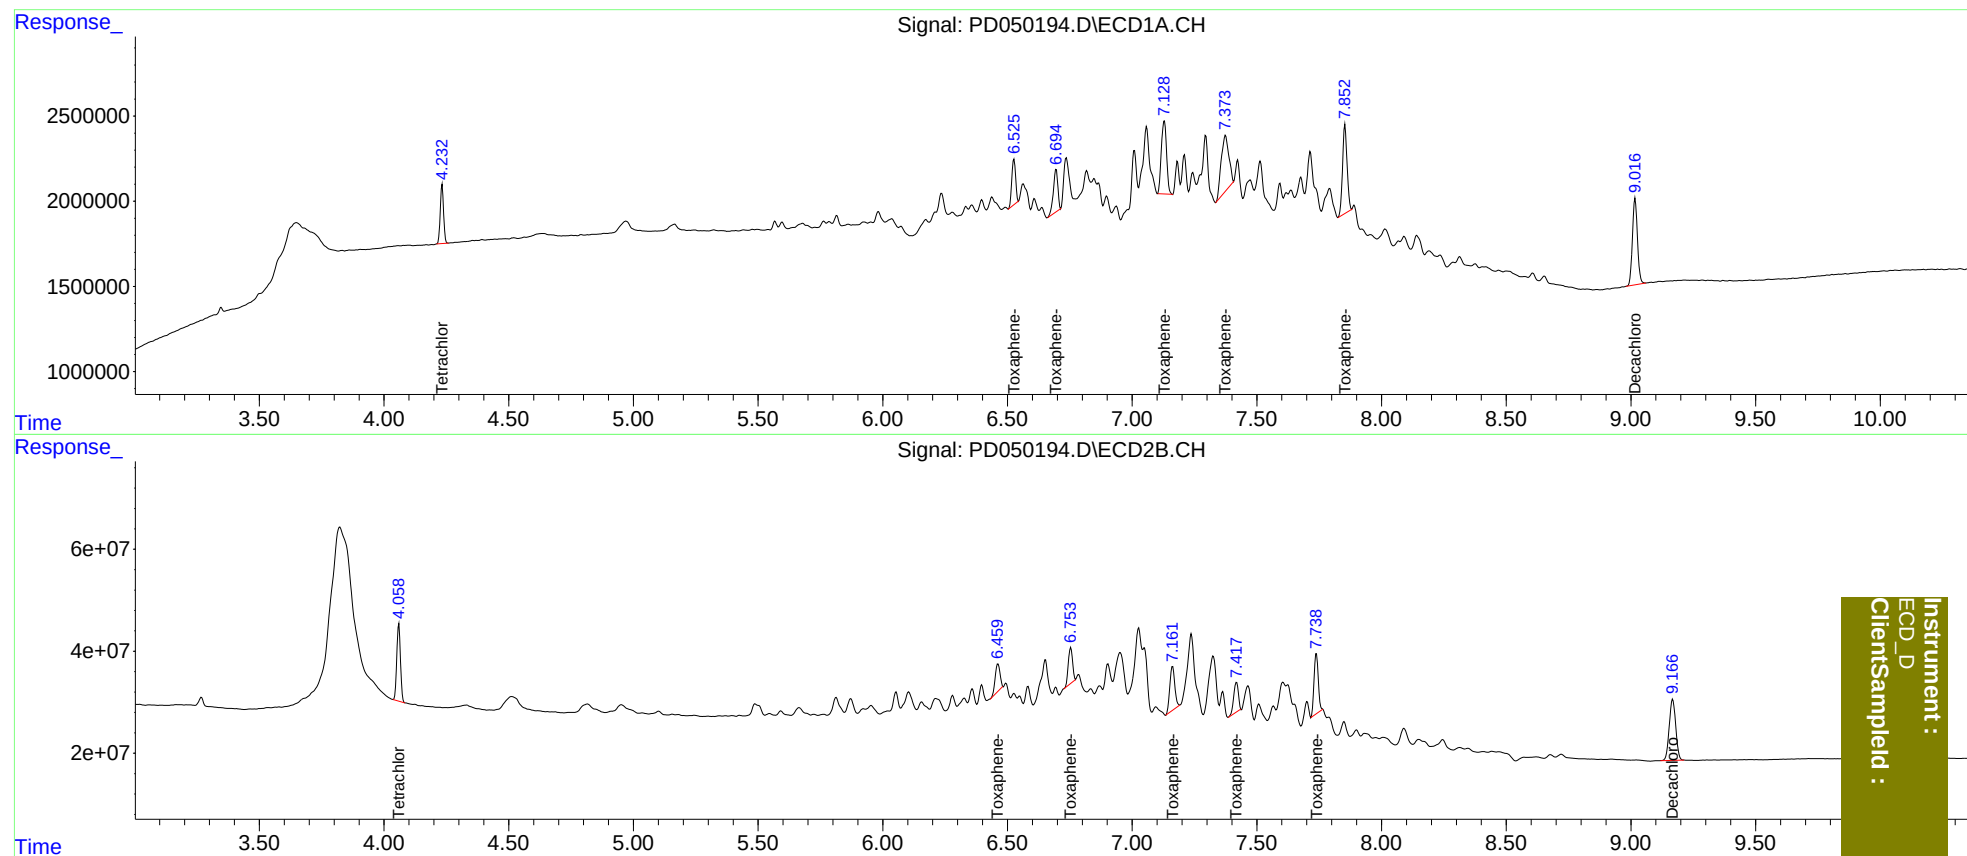

Instrument :
ECD_D
ClientSampled :