


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110618\
Data File : PD050192.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 18:09
Operator : AJ\SJ
Sample : RESC31
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC31

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 03:54:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 06 03:52:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

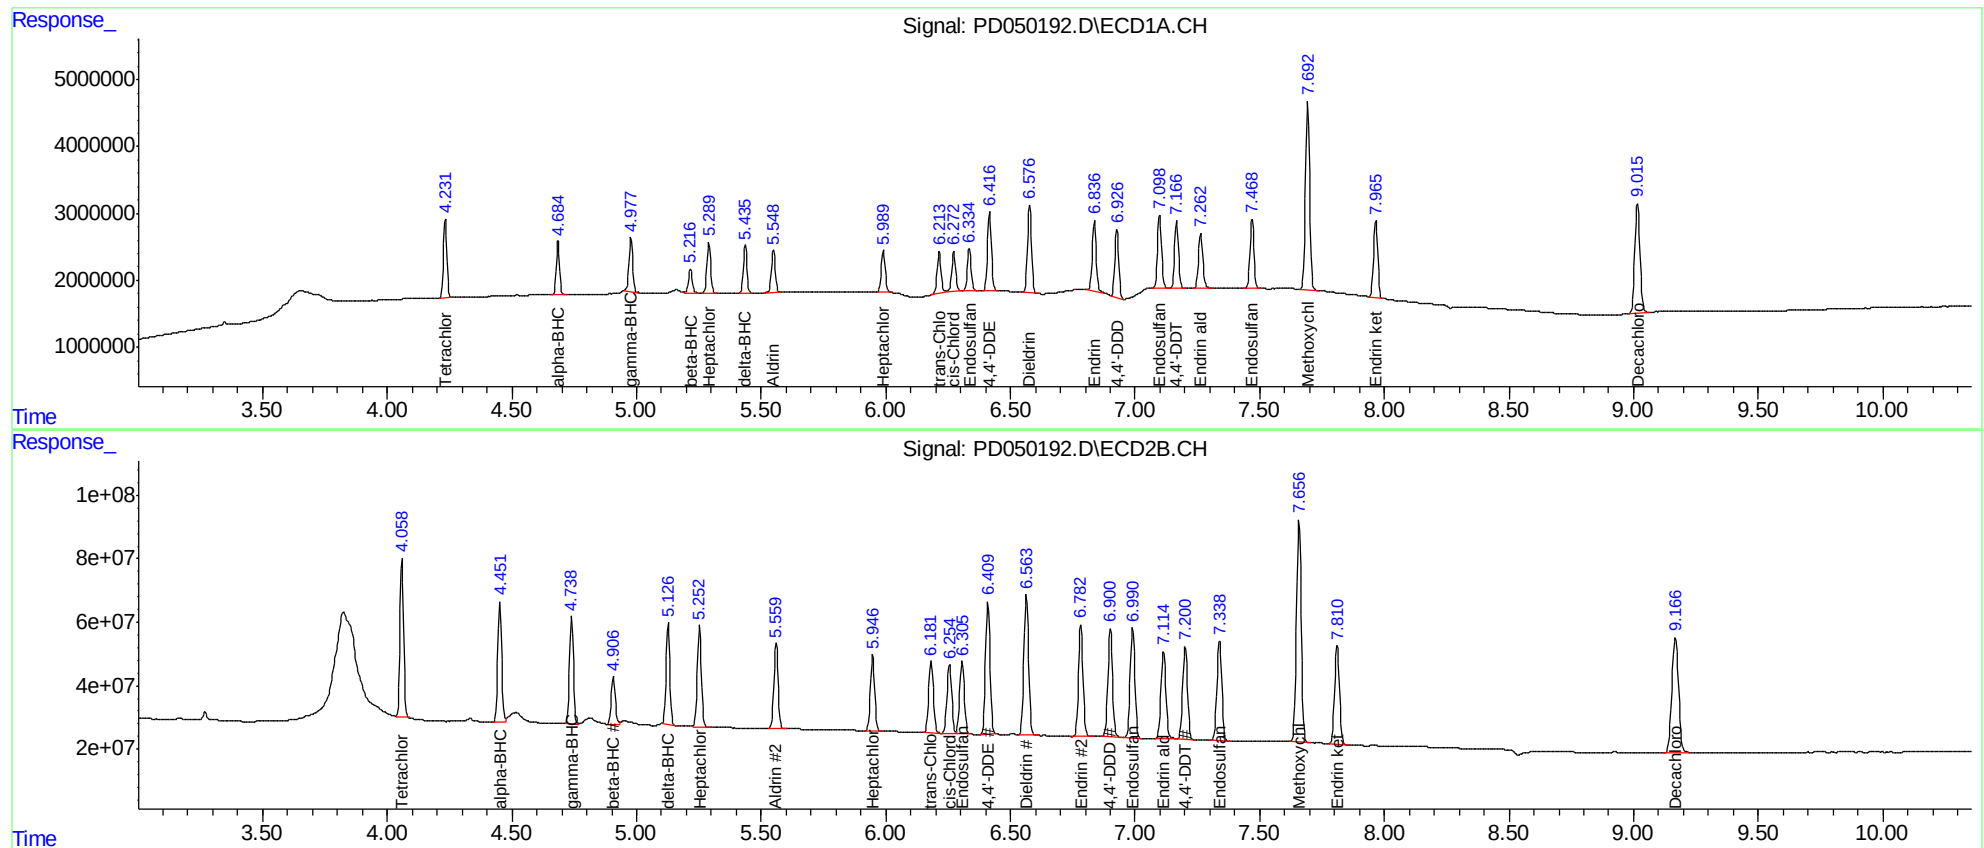

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110618\
 Data File : PD050192.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 18:09
 Operator : AJ\SJ
 Sample : RESC31
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC31

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 03:54:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 06 03:52:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.060	11291053	511.6E6	17.445	17.794
27)	SA Decachlor...	9.016	9.168	23674333	676.0E6	35.434	35.317
Target Compounds							
2)	A alpha-BHC	4.686	4.452	7882032	413.3E6	8.570	9.394
3)	MA gamma-BHC...	4.978	4.739	7987677	374.6E6	8.952	9.410
4)	MA Heptachlor	5.291	5.253	7710120	381.1E6	8.828	9.488
5)	MB Aldrin	5.550	5.561	6797904	327.0E6	8.739	9.395
6)	B beta-BHC	5.217	4.907	3630810	171.3E6	9.317	9.543
7)	B delta-BHC	5.436	5.127	7231806	351.1E6	8.590	9.245
8)	B Heptachlor...	5.991	5.948	6768011	304.1E6	8.944	9.466
9)	A Endosulfan I	6.336	6.306	6861474	294.0E6	9.137	9.681
10)	B trans-Chl...	6.214	6.182	7397196	292.8E6	9.097	9.222
11)	B cis-Chlor...	6.273	6.256	7058230	285.4E6	9.111	9.404
12)	B 4,4'-DDE	6.417	6.411	12622362	530.4E6	17.227	18.600
13)	MA Dieldrin	6.577	6.564	14572592	577.4E6	17.272	18.645
14)	MA Endrin	6.837	6.783	12195869	458.6E6	17.756	19.145
15)	B Endosulfa...	7.099	6.991	12537453	457.0E6	17.616	18.826
16)	A 4,4'-DDD	6.928	6.901	10871296	450.0E6	17.322	18.952
17)	MA 4,4'-DDT	7.168	7.201	11011595	386.3E6	17.025	18.134
18)	B Endrin al...	7.263	7.115	9925315	367.5E6	17.960	19.034
19)	B Endosulfa...	7.470	7.339	11734692	425.9E6	17.739	18.831
20)	A Methoxychlor	7.693	7.658	32275179	949.6E6	89.469	95.055
21)	B Endrin ke...	7.966	7.812	13398234	415.0E6	18.399	19.298

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.