

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
 Data File : PD079434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 22:12
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 06:55:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 06:52:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.803	7808154	11863847	5.337	5.167
27)	SA Decachlor...	9.110	7.949	19642281	25905835	11.075	10.779
Target Compounds							
2)	A alpha-BHC	4.024	3.306	12046180	17523476	4.907	4.819
3)	MA gamma-BHC...	4.357	3.636	11805676	17073183	5.025	4.957
4)	MA Heptachlor	4.950	3.979	13096715	16972123	5.252	5.101
9)	A Endosulfan I	6.107	5.131	11227581	14122026	5.443	5.056
13)	MA Dieldrin	6.382	5.396	22315933	32314379	10.149	10.139
14)	MA Endrin	6.612	5.671	18853614	27543391	10.355	9.999
16)	A 4,4'-DDD	6.743	5.818	16354064	23298586	10.045	9.824
17)	MA 4,4'-DDT	7.058	6.070	17111802	23269627	9.980	9.568
20)	A Methoxychlor	7.532	6.645	48548374	69610806	51.832	52.708


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
Data File : PD079434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 22:12
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 06:55:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 06:52:36 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

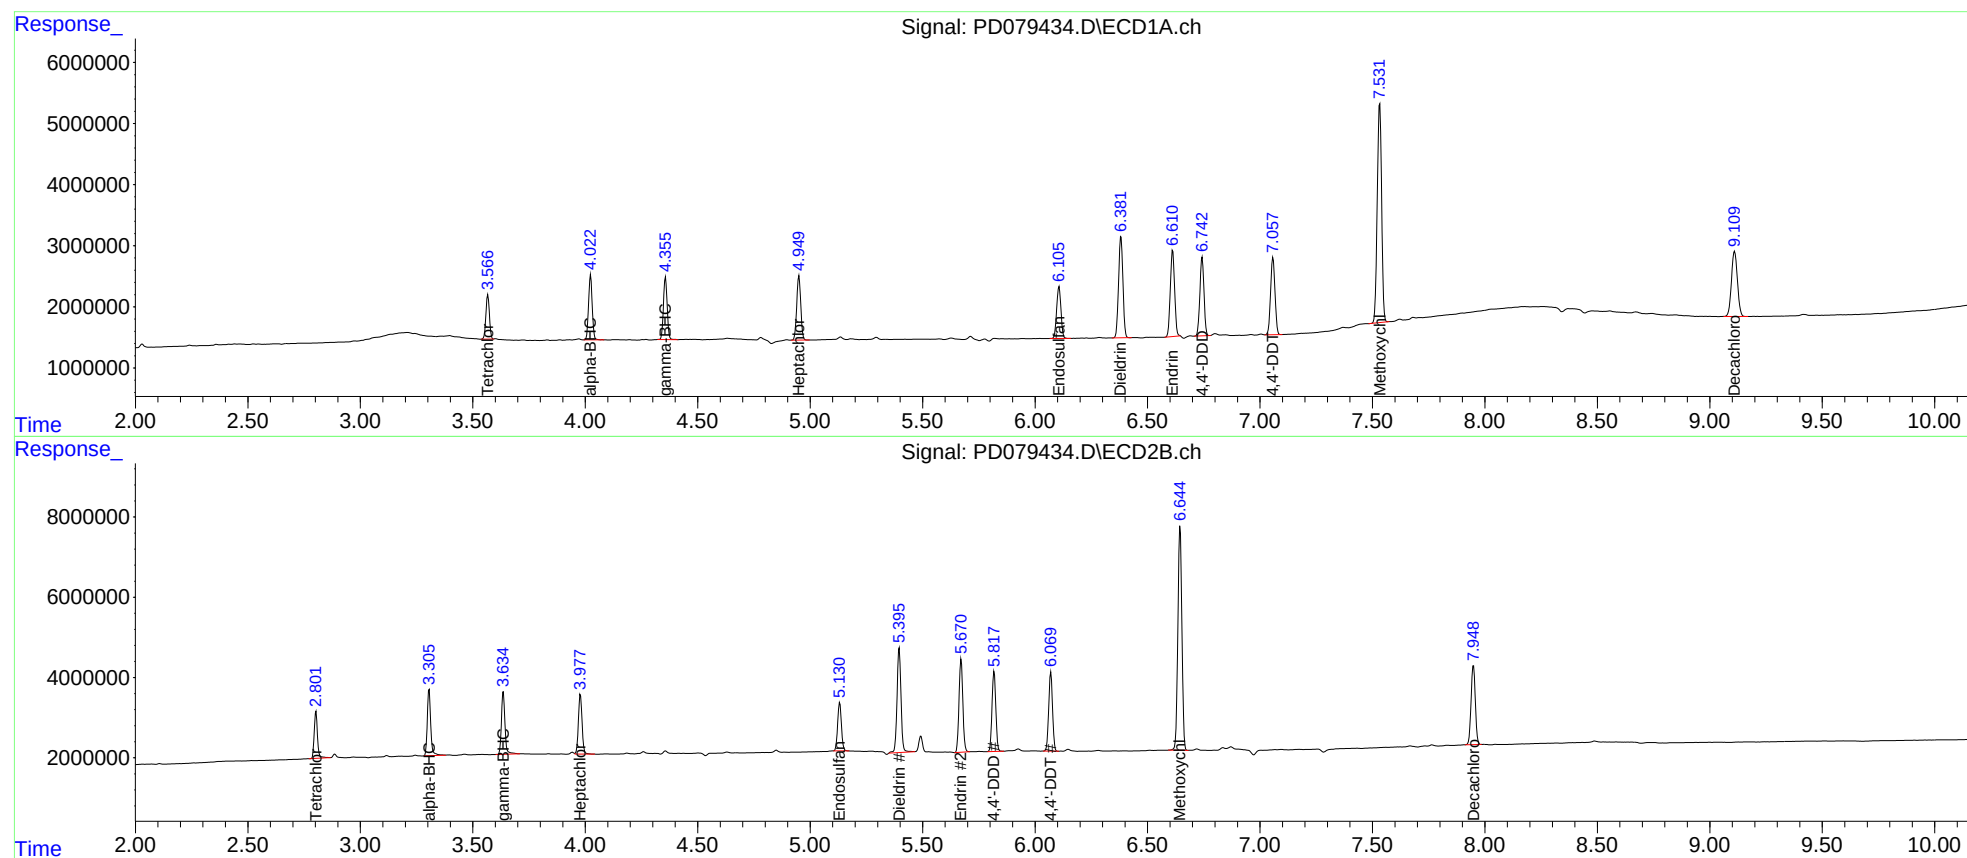

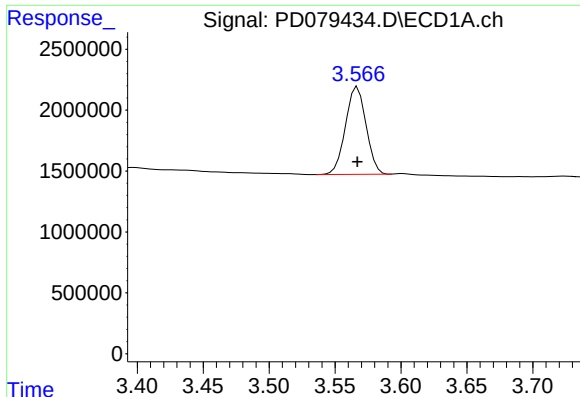


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 7808154
Conc: 5.34 ng/ml

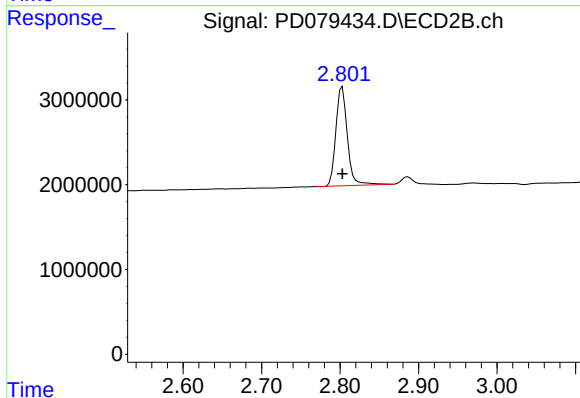


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 11863847
Conc: 5.17 ng/ml

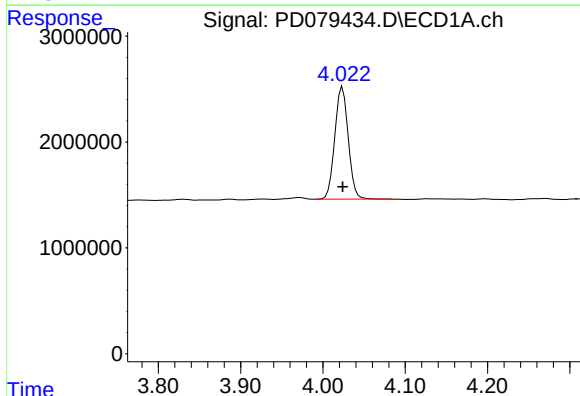


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 12046180
Conc: 4.91 ng/ml

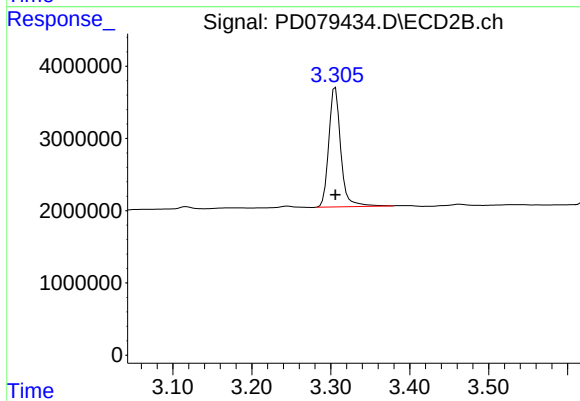


#2 alpha-BHC

R.T.: 3.306 min
Delta R.T.: 0.000 min
Response: 17523476
Conc: 4.82 ng/ml

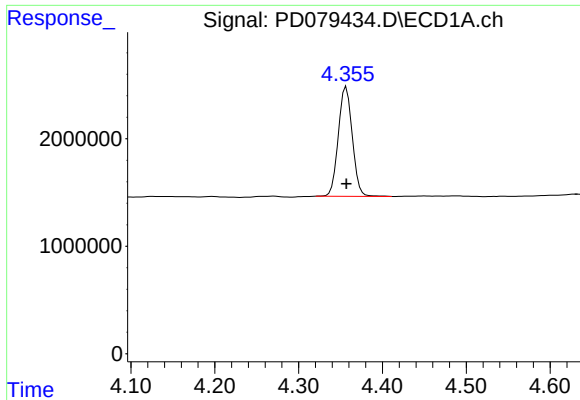


#3 gamma-BHC (Lindane)

R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 11805676
Conc: 5.02 ng/ml

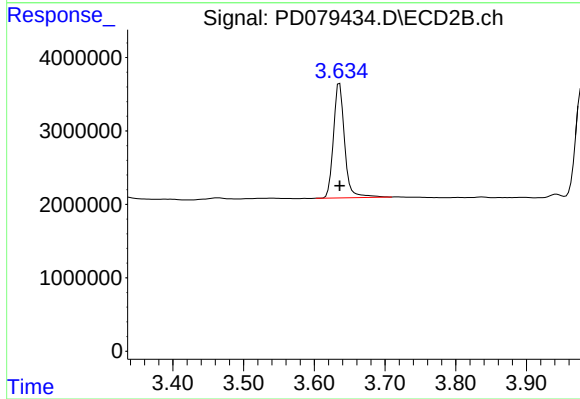


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 17073183
Conc: 4.96 ng/ml

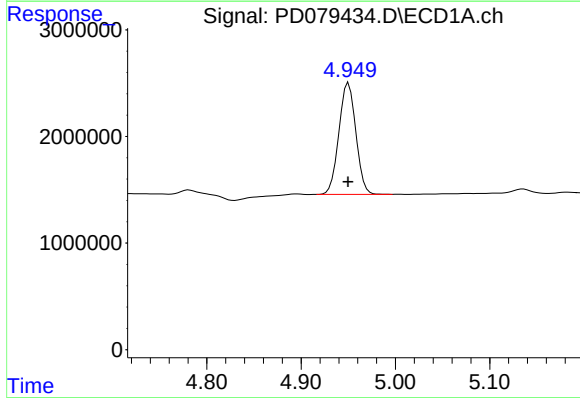


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 13096715
Conc: 5.25 ng/ml

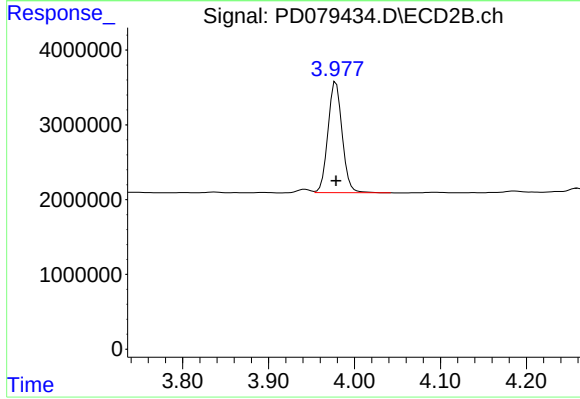


#4 Heptachlor

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 16972123
Conc: 5.10 ng/ml

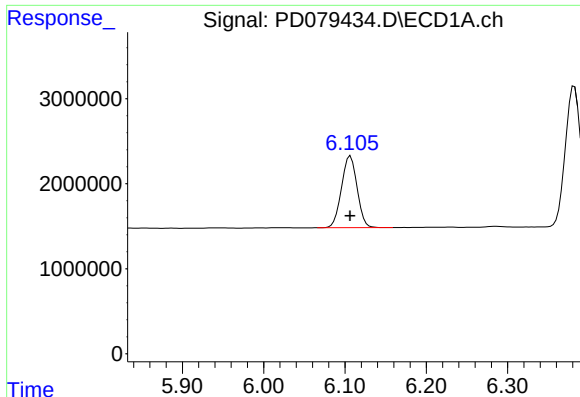


#9 Endosulfan I

R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 11227581
Conc: 5.44 ng/ml

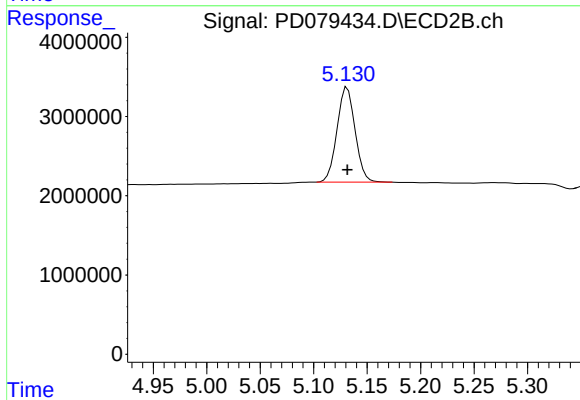


#9 Endosulfan I

R.T.: 5.131 min
Delta R.T.: 0.000 min
Response: 14122026
Conc: 5.06 ng/ml

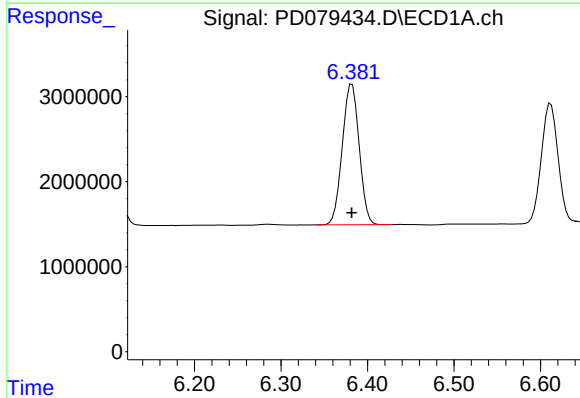


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 22315933
Conc: 10.15 ng/ml

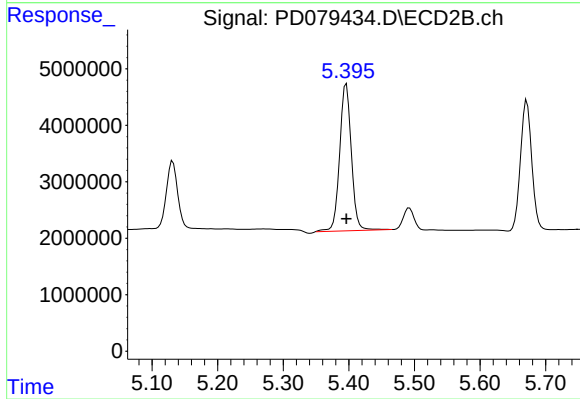


#13 Dieldrin

R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 32314379
Conc: 10.14 ng/ml

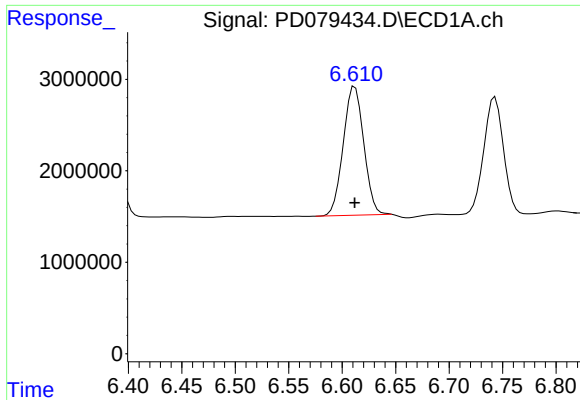


#14 Endrin

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 18853614
Conc: 10.35 ng/ml

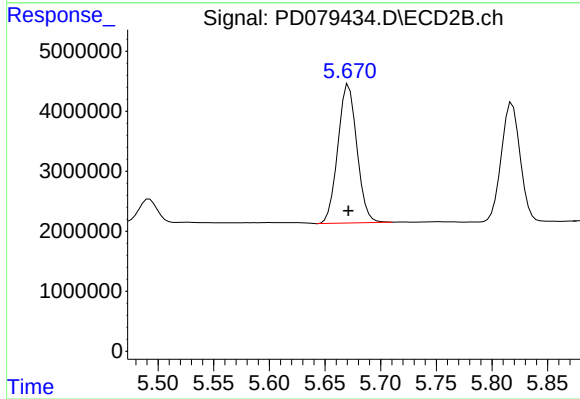


#14 Endrin

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 27543391
Conc: 10.00 ng/ml

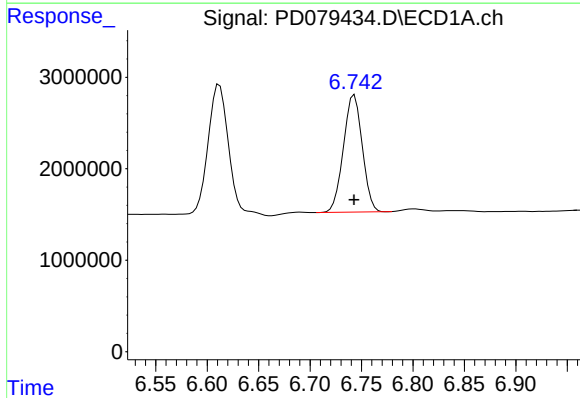


#16 4,4'-DDD

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 16354064
Conc: 10.05 ng/ml

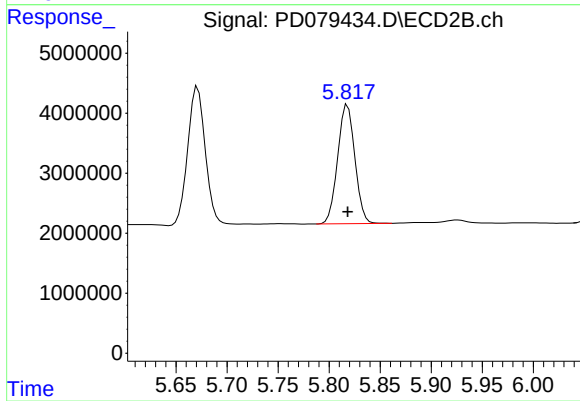


#16 4,4'-DDD

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 23298586
Conc: 9.82 ng/ml

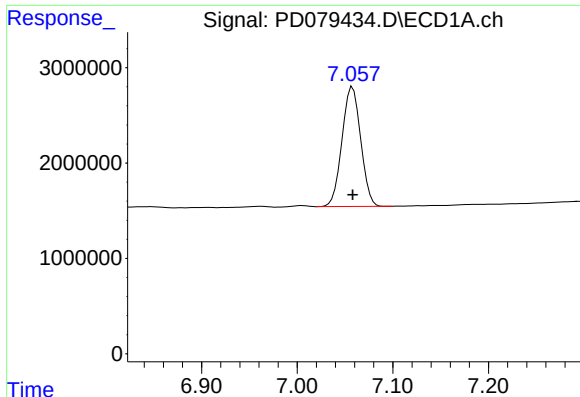


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 17111802
Conc: 9.98 ng/ml

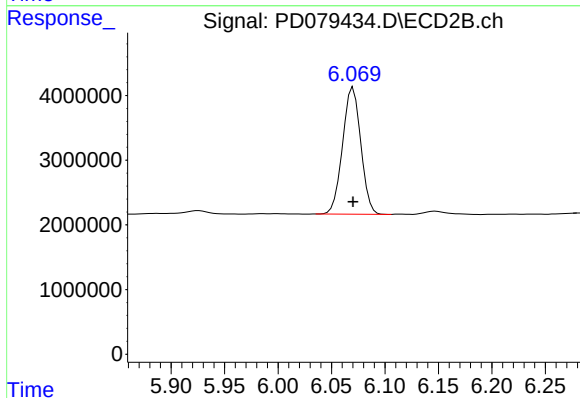


#17 4,4'-DDT

R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 23269627
Conc: 9.57 ng/ml

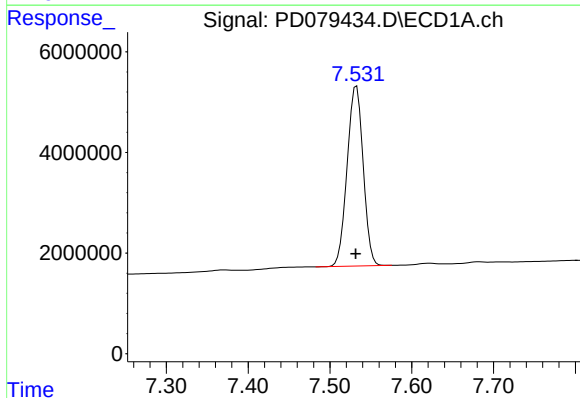


#20 Methoxychlor

R.T.: 7.532 min
Delta R.T.: 0.000 min
Response: 48548374
Conc: 51.83 ng/ml

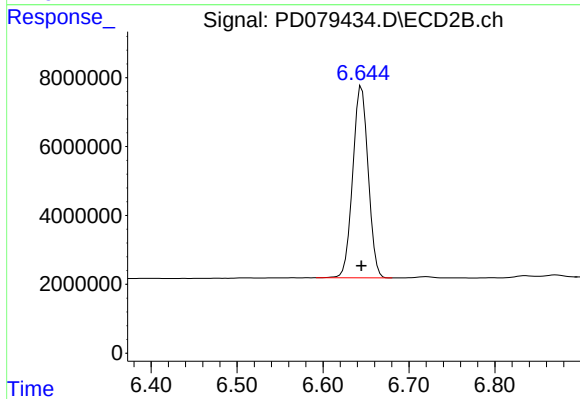


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 69610806
Conc: 52.71 ng/ml

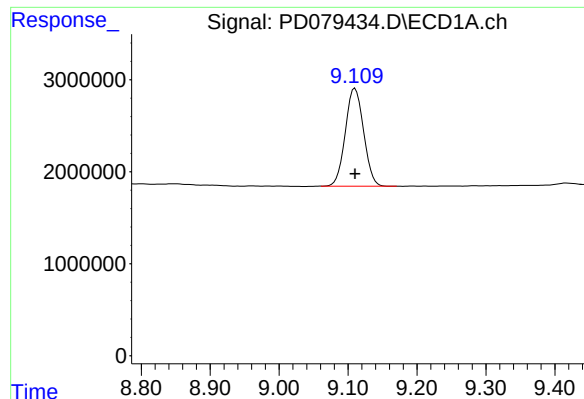

#27 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 19642281
Conc: 11.07 ng/ml

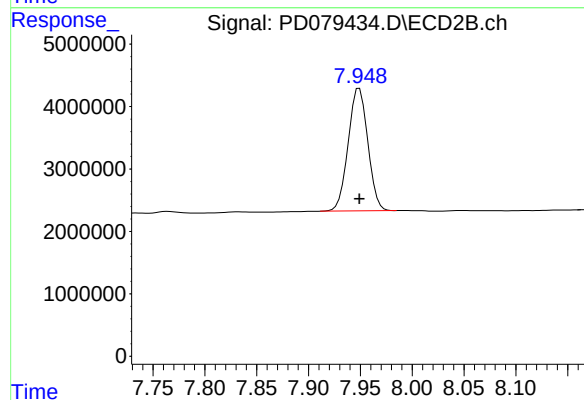

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 25905835
Conc: 10.78 ng/ml