

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
 Data File : PD079436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 22:39
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 06:55:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 06:52:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.803	14802497	22992325	10.118	10.013
27)	SA Decachlor...	9.112	7.949	37135475	48689152	20.938	20.259
Target Compounds							
2)	A alpha-BHC	4.024	3.306	23757954	35166356	9.678	9.670
3)	MA gamma-BHC...	4.357	3.636	22970185	33558097	9.777	9.743
4)	MA Heptachlor	4.950	3.979	24873564	33195503	9.976	9.977
9)	A Endosulfan I	6.106	5.132	21009750	27832378	10.185	9.964
13)	MA Dieldrin	6.382	5.397	43295343	62221344	19.691	19.523
14)	MA Endrin	6.612	5.672	35939348	53660609	19.738	19.480
16)	A 4,4'-DDD	6.743	5.819	31896483	46274739	19.592	19.512
17)	MA 4,4'-DDT	7.058	6.070	33381779	46743800	19.470	19.220
20)	A Methoxychlor	7.532	6.645	92365526	133.8E6	98.613	101.305


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
Data File : PD079436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 22:39
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 06:55:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 06:52:36 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

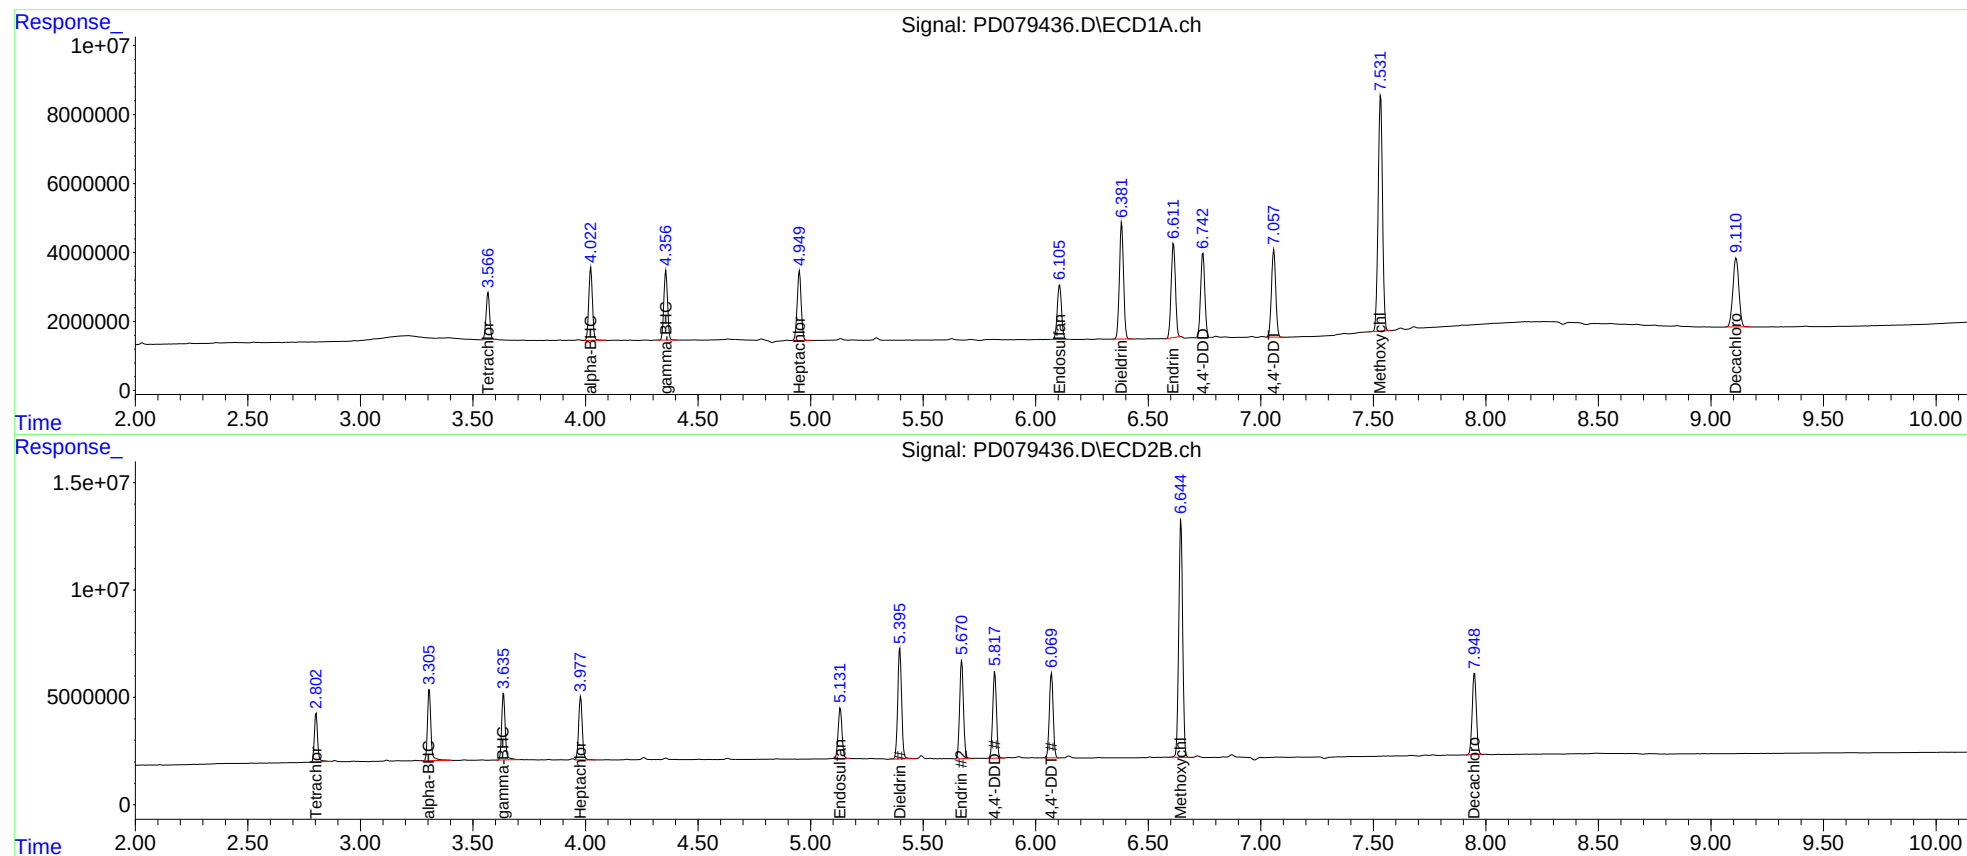

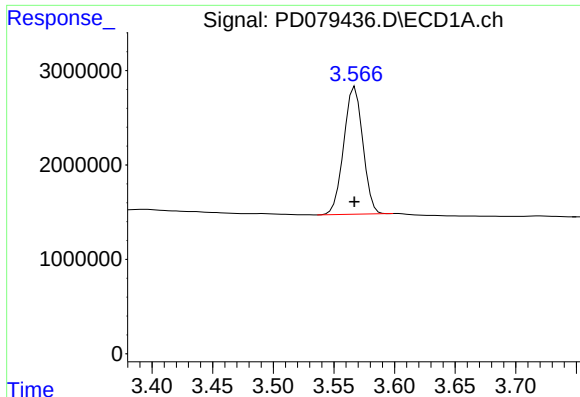


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 14802497
Conc: 10.12 ng/ml

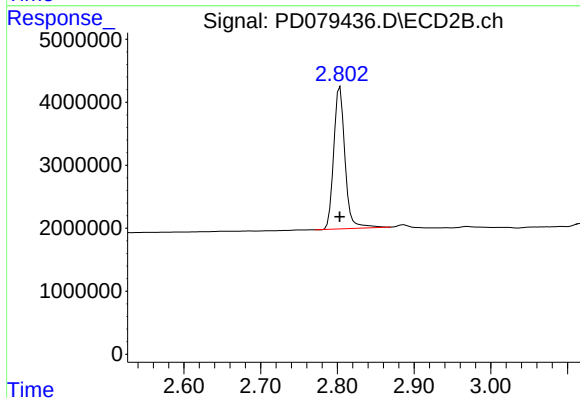


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 22992325
Conc: 10.01 ng/ml

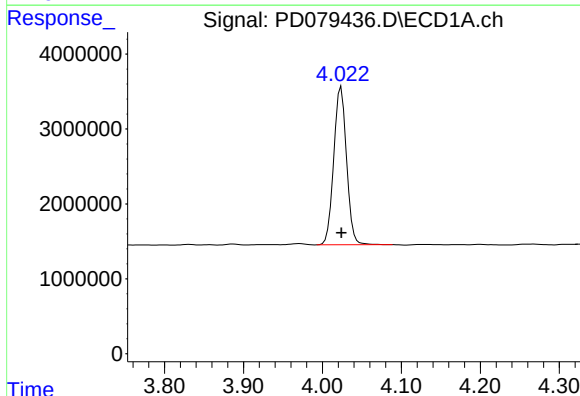


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 23757954
Conc: 9.68 ng/ml

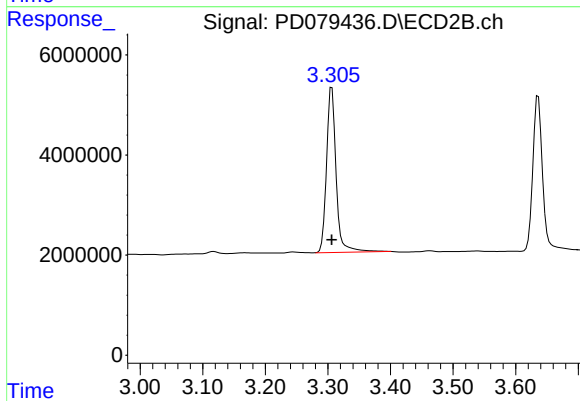


#2 alpha-BHC

R.T.: 3.306 min
Delta R.T.: 0.000 min
Response: 35166356
Conc: 9.67 ng/ml

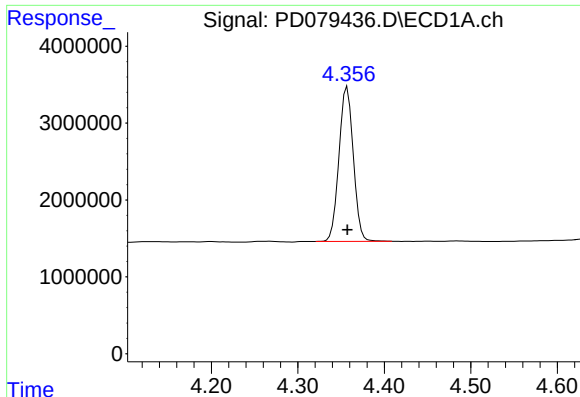


#3 gamma-BHC (Lindane)

R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 22970185
Conc: 9.78 ng/ml

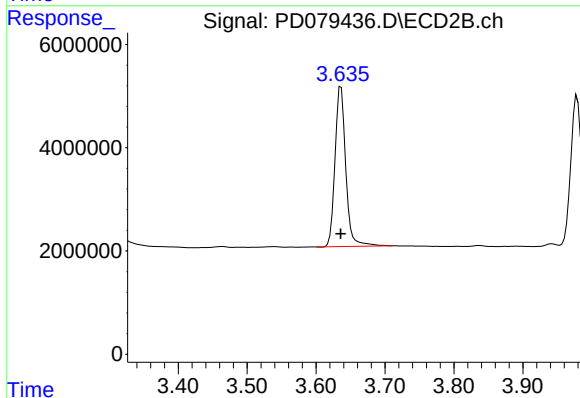


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 33558097
Conc: 9.74 ng/ml

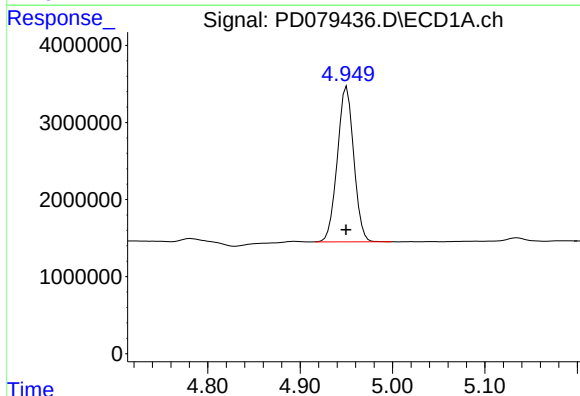


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 24873564
Conc: 9.98 ng/ml

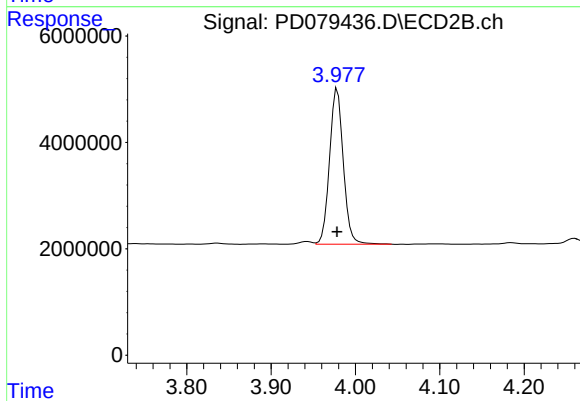


#4 Heptachlor

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 33195503
Conc: 9.98 ng/ml

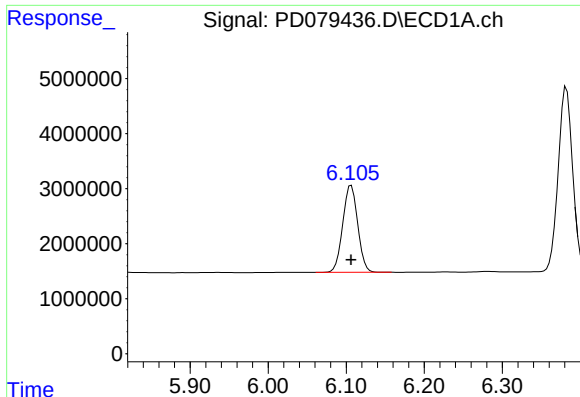


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 21009750
Conc: 10.18 ng/ml

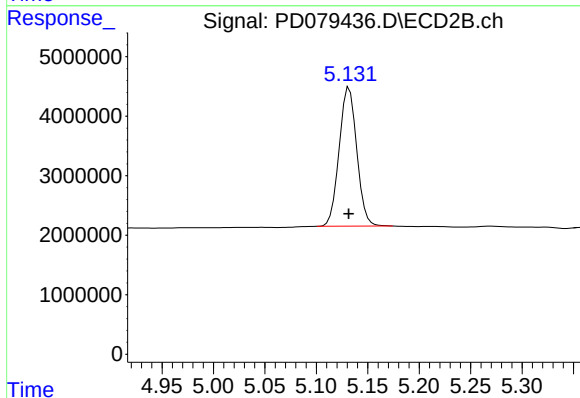


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 27832378
Conc: 9.96 ng/ml

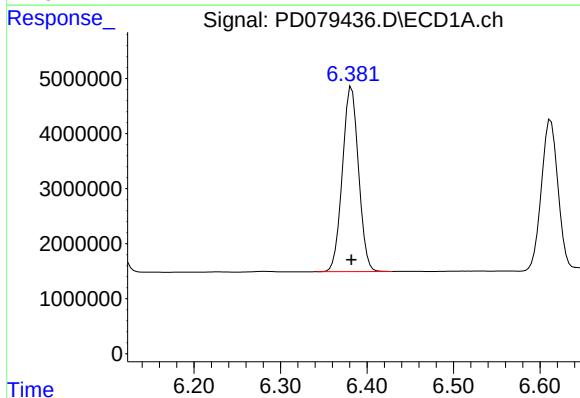


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 43295343
Conc: 19.69 ng/ml

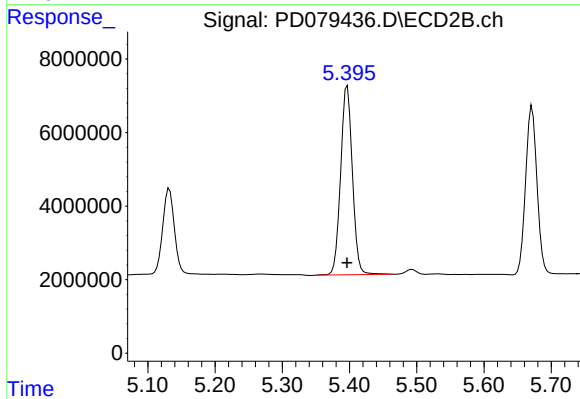


#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 62221344
Conc: 19.52 ng/ml

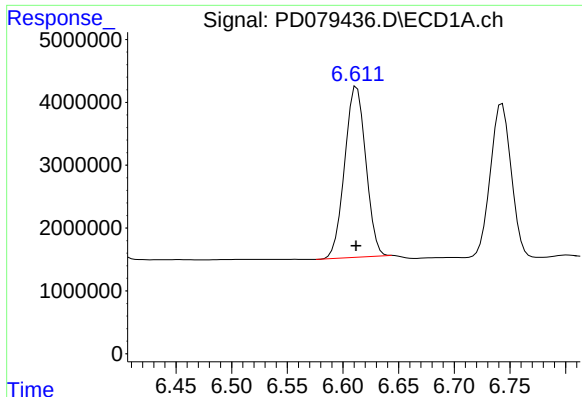


#14 Endrin

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 35939348
Conc: 19.74 ng/ml

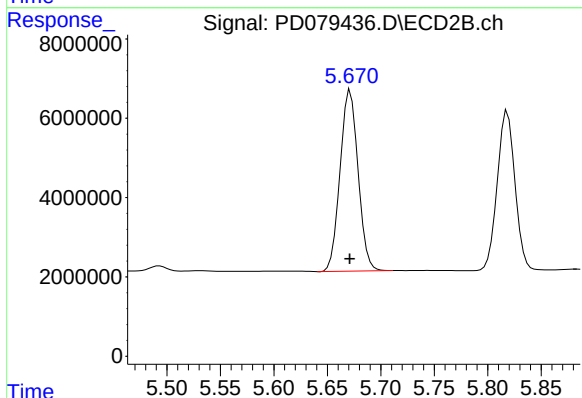


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 53660609
Conc: 19.48 ng/ml

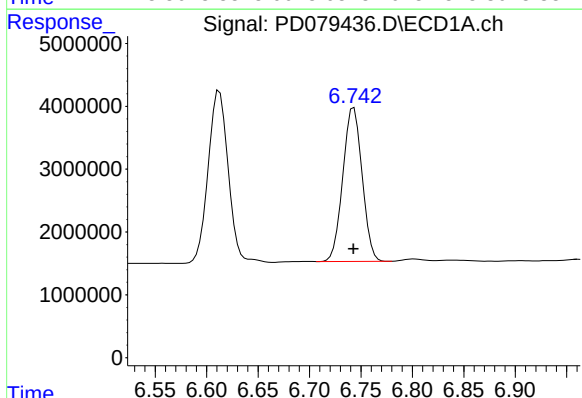


#16 4,4'-DDD

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 31896483
Conc: 19.59 ng/ml

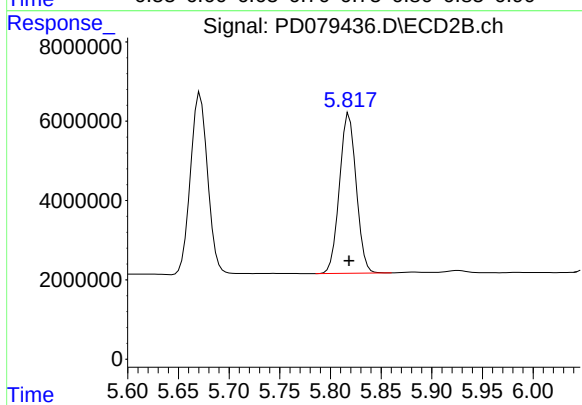


#16 4,4'-DDD

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 46274739
Conc: 19.51 ng/ml

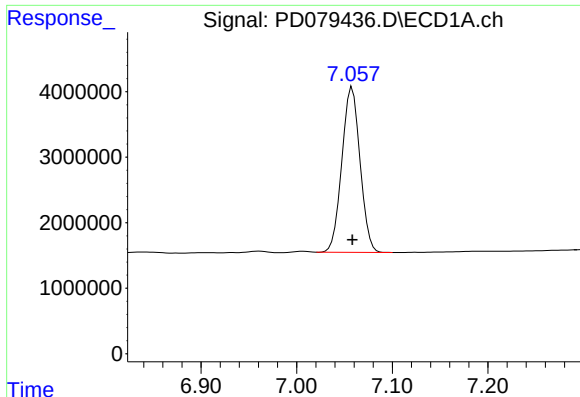


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 33381779
Conc: 19.47 ng/ml

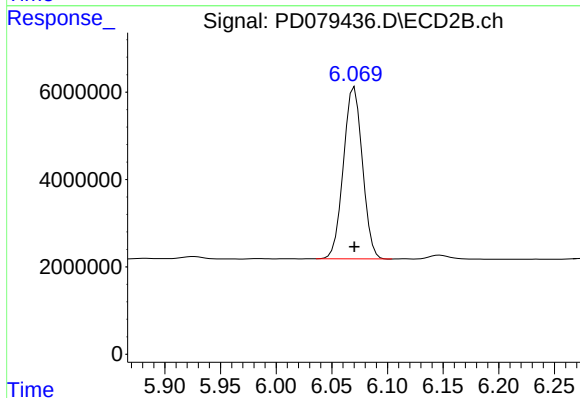


#17 4,4'-DDT

R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 46743800
Conc: 19.22 ng/ml

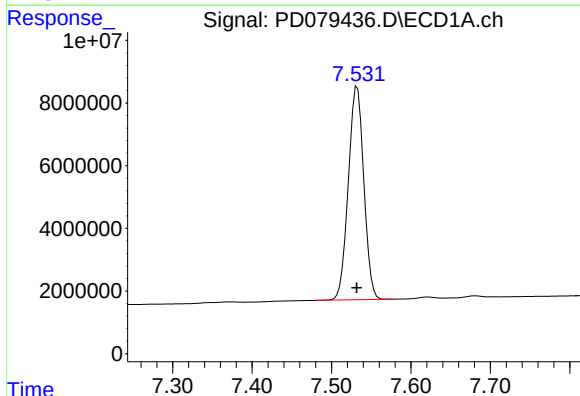


#20 Methoxychlor

R.T.: 7.532 min
Delta R.T.: 0.000 min
Response: 92365526
Conc: 98.61 ng/ml

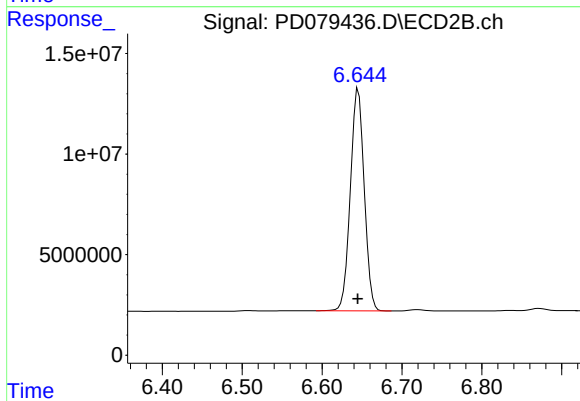


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 133792276
Conc: 101.31 ng/ml

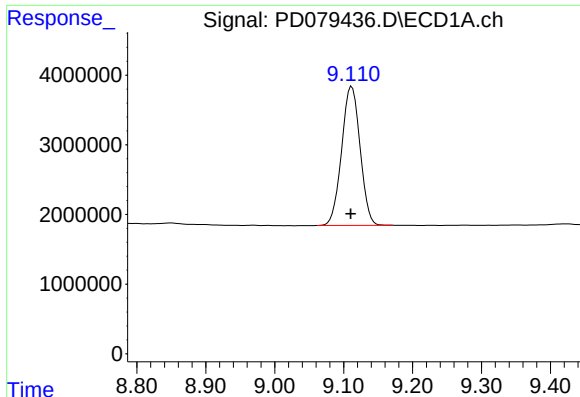

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.002 min
Response: 37135475
Conc: 20.94 ng/ml

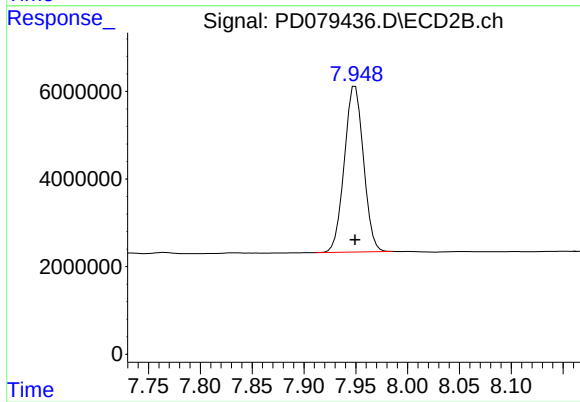

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 48689152
Conc: 20.26 ng/ml