

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
 Data File : PD079438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 23:06
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 06:55:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 06:52:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.803	29258493	45925201	20.000	20.000
27)	SA Decachlor...	9.110	7.949	70944890	96134747	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.024	3.306	49095550	72732222	20.000	20.000
3)	MA gamma-BHC...	4.357	3.636	46988853	68885395	20.000	20.000
4)	MA Heptachlor	4.950	3.978	49868675	66543317	20.000	20.000
9)	A Endosulfan I	6.106	5.131	41256651	55865361	20.000	20.000
13)	MA Dieldrin	6.382	5.396	87951601	127.5E6	40.000	40.000
14)	MA Endrin	6.612	5.671	72831961	110.2E6	40.000	40.000
16)	A 4,4'-DDD	6.743	5.818	65121616	94864559	40.000	40.000
17)	MA 4,4'-DDT	7.058	6.070	68581670	97279923	40.000	40.000
20)	A Methoxychlor	7.532	6.645	187.3E6	264.1E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
Data File : PD079438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 23:06
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 06:55:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 06:52:36 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

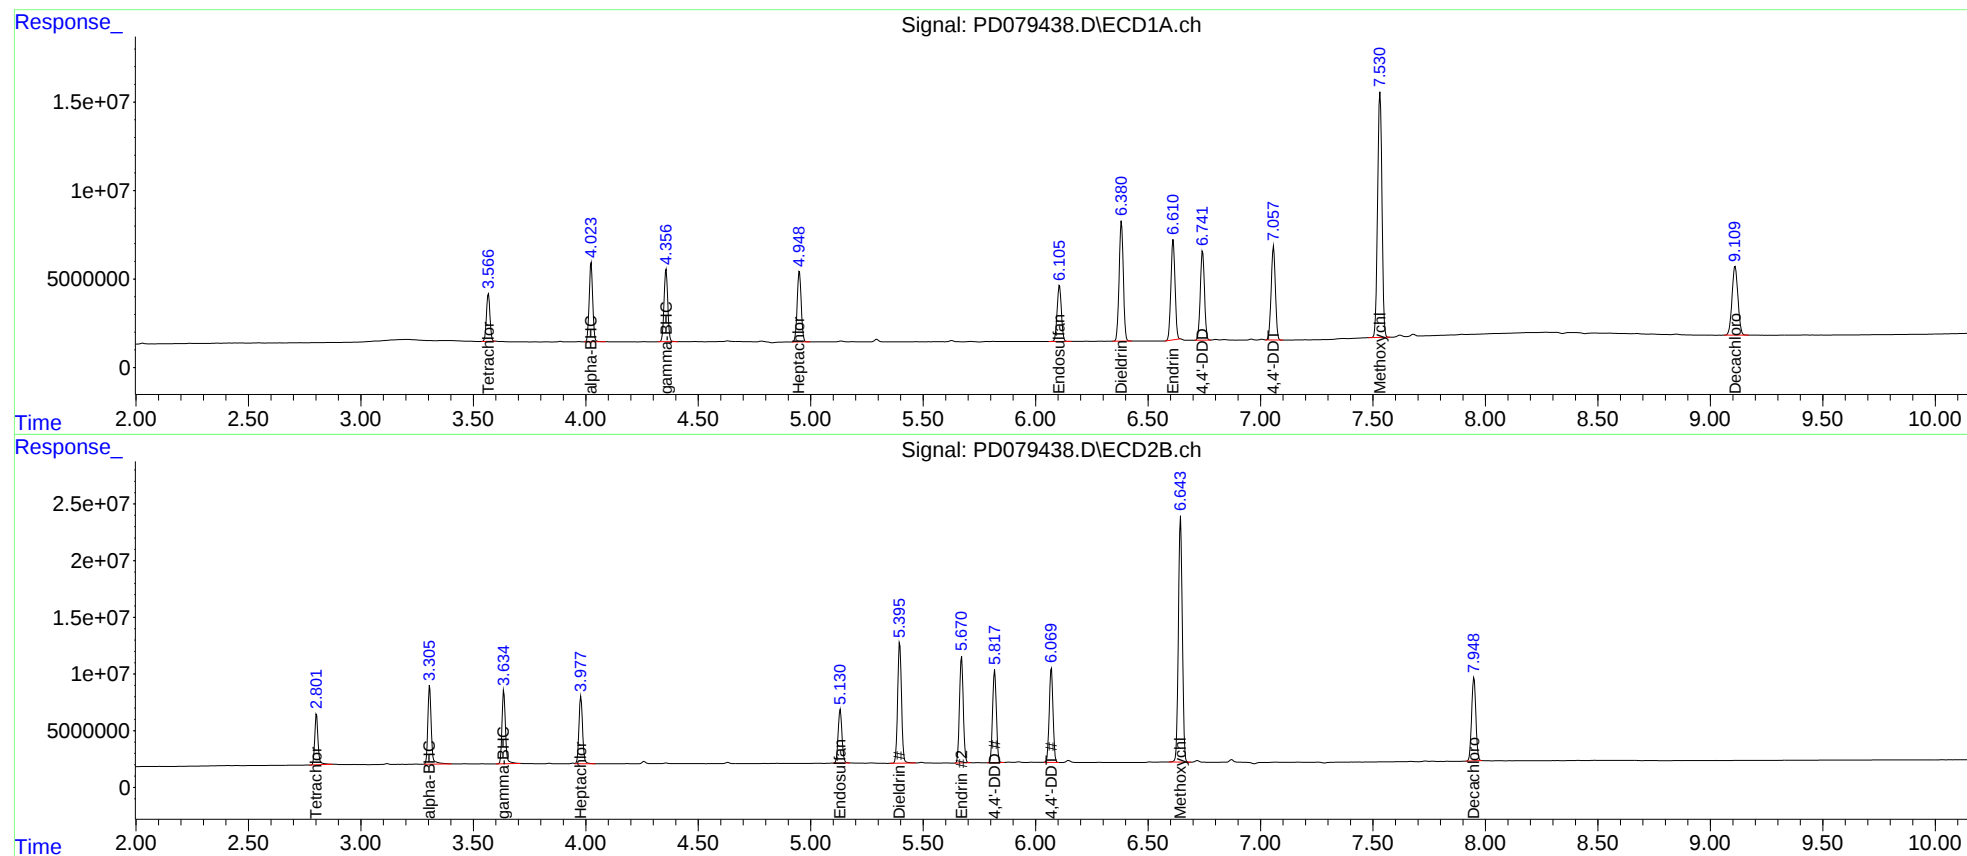

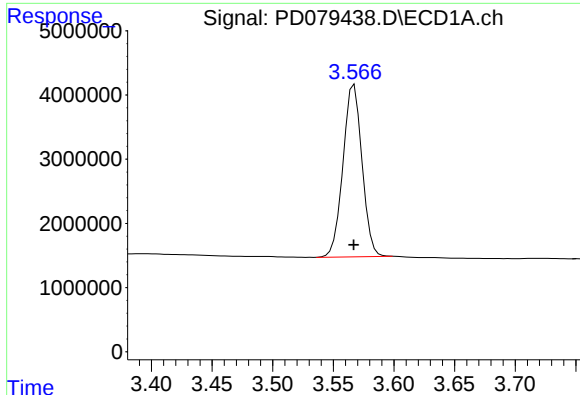


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 29258493
Conc: 20.00 ng/ml

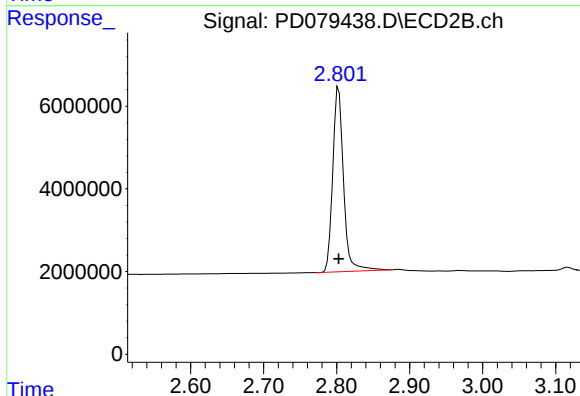


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 45925201
Conc: 20.00 ng/ml

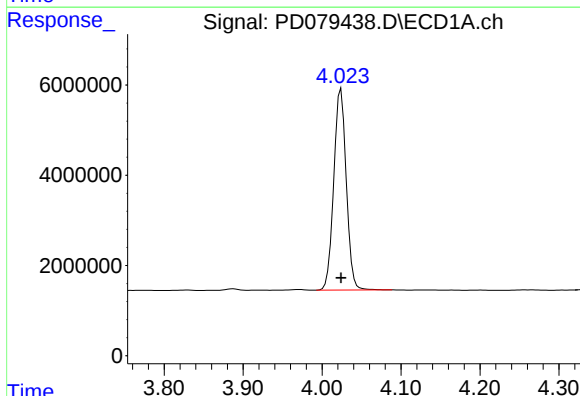


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 49095550
Conc: 20.00 ng/ml

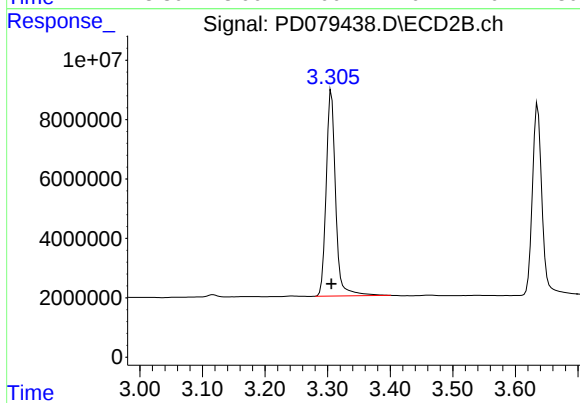


#2 alpha-BHC

R.T.: 3.306 min
Delta R.T.: 0.000 min
Response: 72732222
Conc: 20.00 ng/ml

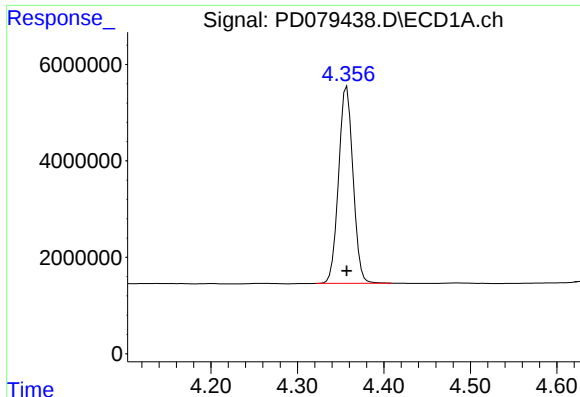


#3 gamma-BHC (Lindane)

R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 46988853
Conc: 20.00 ng/ml

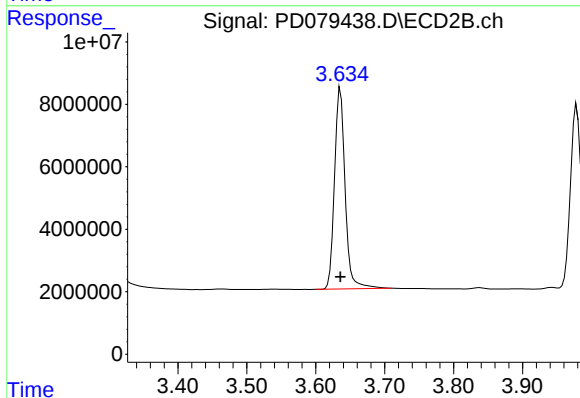


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 68885395
Conc: 20.00 ng/ml

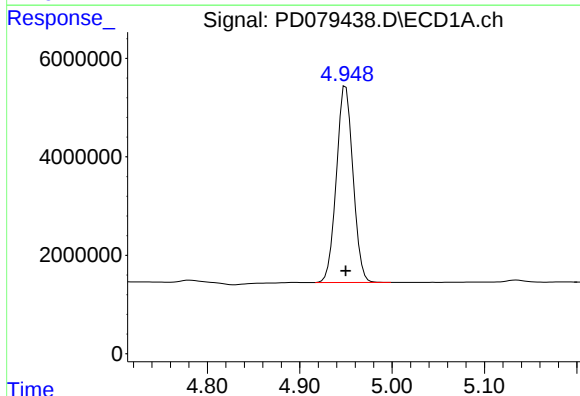


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 49868675
Conc: 20.00 ng/ml

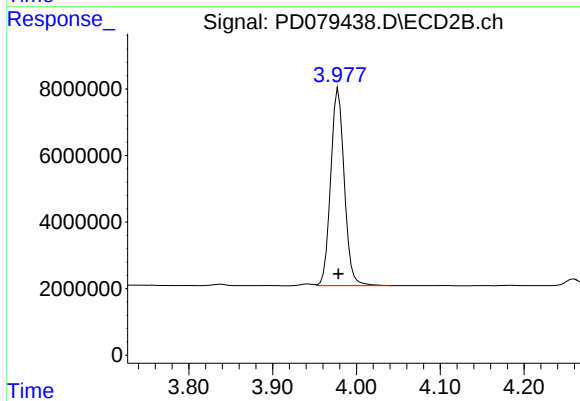


#4 Heptachlor

R.T.: 3.978 min
Delta R.T.: 0.000 min
Response: 66543317
Conc: 20.00 ng/ml

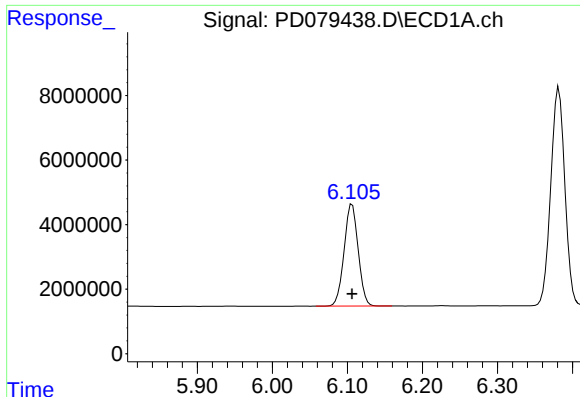


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 41256651
Conc: 20.00 ng/ml

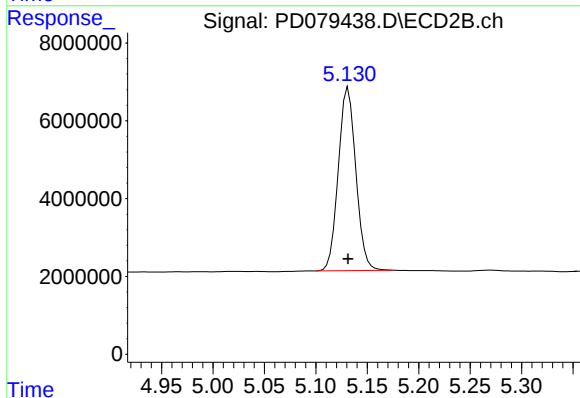


#9 Endosulfan I

R.T.: 5.131 min
Delta R.T.: 0.000 min
Response: 55865361
Conc: 20.00 ng/ml

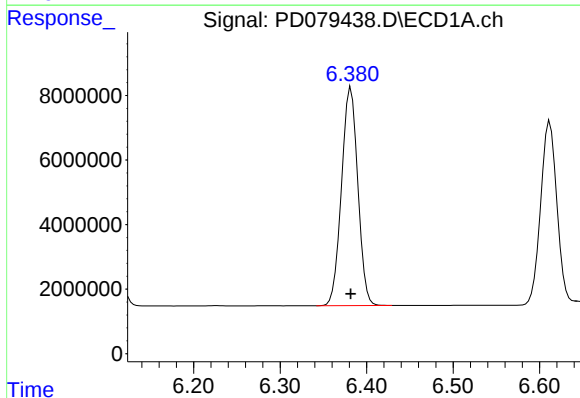


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 87951601
Conc: 40.00 ng/ml

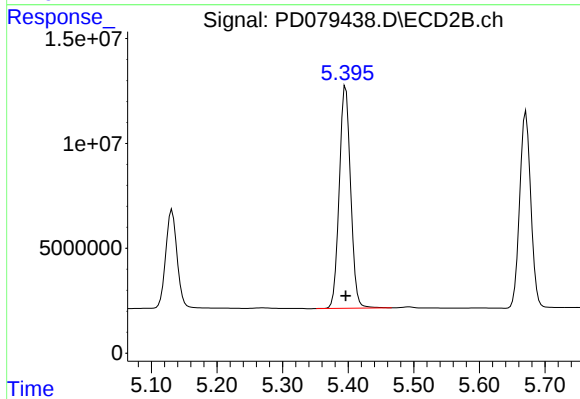


#13 Dieldrin

R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 127484493
Conc: 40.00 ng/ml

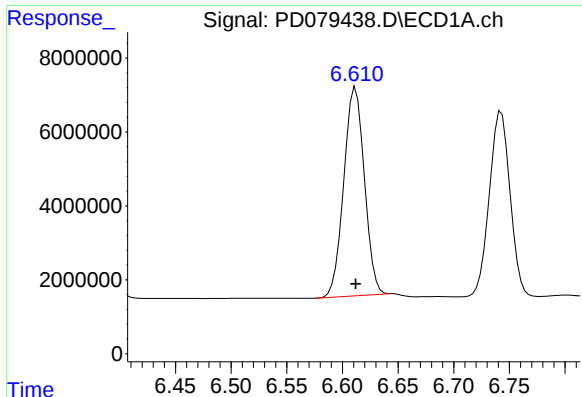


#14 Endrin

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 72831961
Conc: 40.00 ng/ml

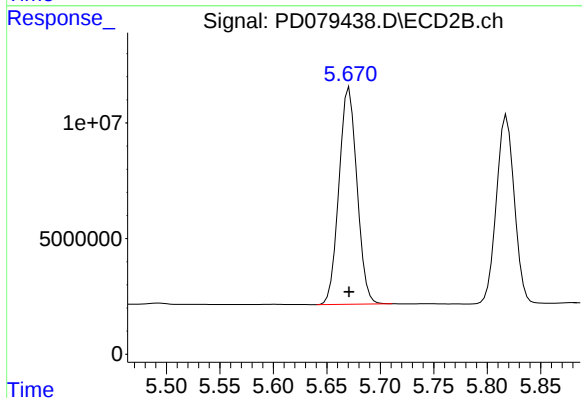


#14 Endrin

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 110183769
Conc: 40.00 ng/ml

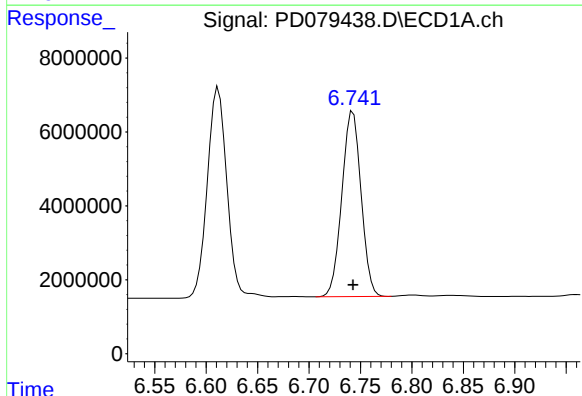


#16 4,4'-DDD

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 65121616
Conc: 40.00 ng/ml

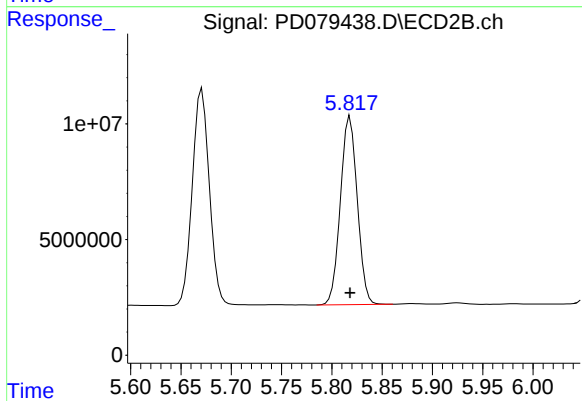


#16 4,4'-DDD

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 94864559
Conc: 40.00 ng/ml

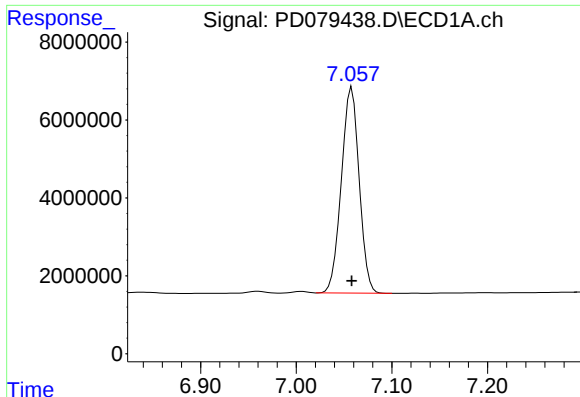


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 68581670
Conc: 40.00 ng/ml

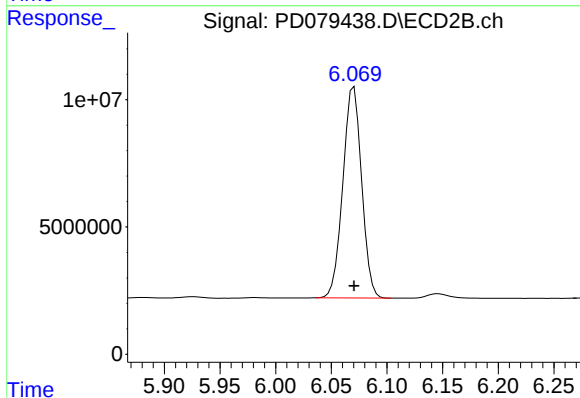


#17 4,4'-DDT

R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 97279923
Conc: 40.00 ng/ml

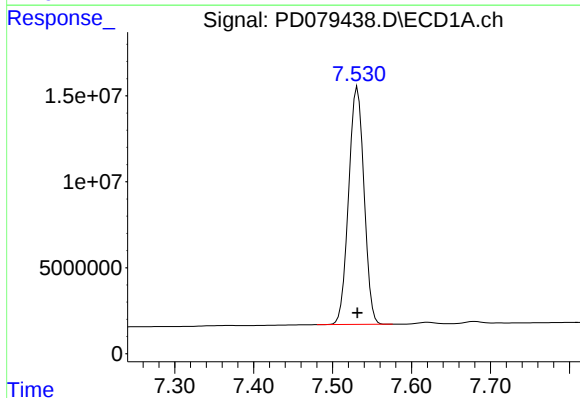


#20 Methoxychlor

R.T.: 7.532 min
Delta R.T.: 0.000 min
Response: 187329447
Conc: 200.00 ng/ml

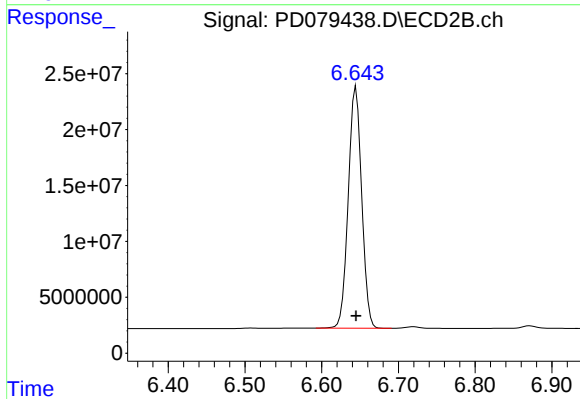


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 264137425
Conc: 200.00 ng/ml

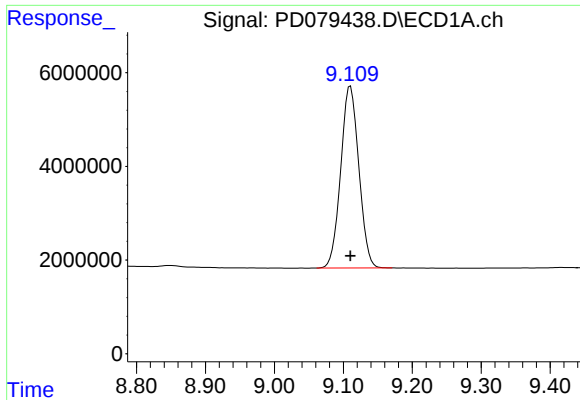

#27 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 70944890
Conc: 40.00 ng/ml

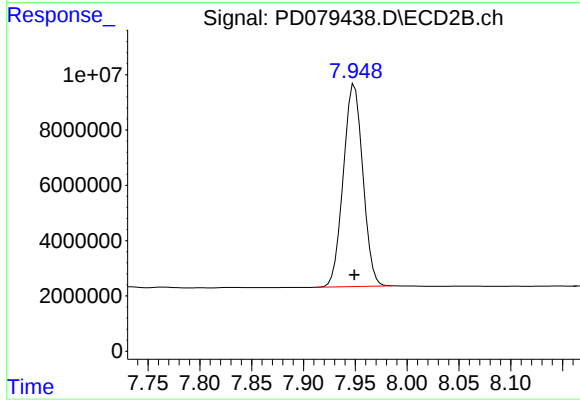

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 96134747
Conc: 40.00 ng/ml