

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
 Data File : PD079440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 23:32
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 06:55:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 06:52:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.803	56443640	90227774	38.583	39.293
27)	SA Decachlor...	9.111	7.949	134.3E6	183.1E6	75.709	76.181
Target Compounds							
2)	A alpha-BHC	4.024	3.307	101.2E6	148.8E6	41.232	40.904
3)	MA gamma-BHC...	4.357	3.636	95119161	138.8E6	40.486	40.303
4)	MA Heptachlor	4.950	3.979	99008049	133.3E6	39.708	40.053
9)	A Endosulfan I	6.106	5.132	79612836	109.9E6	38.594	39.354
13)	MA Dieldrin	6.382	5.396	176.2E6	256.1E6	80.131	80.365
14)	MA Endrin	6.612	5.671	145.0E6	221.3E6	79.653	80.326
16)	A 4,4'-DDD	6.742	5.818	129.5E6	190.5E6	79.531	80.315
17)	MA 4,4'-DDT	7.057	6.070	136.8E6	195.9E6	79.781	80.554
20)	A Methoxychlor	7.531	6.645	362.7E6	494.5E6	387.264	374.450


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
Data File : PD079440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 23:32
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 06:55:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 06:52:36 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

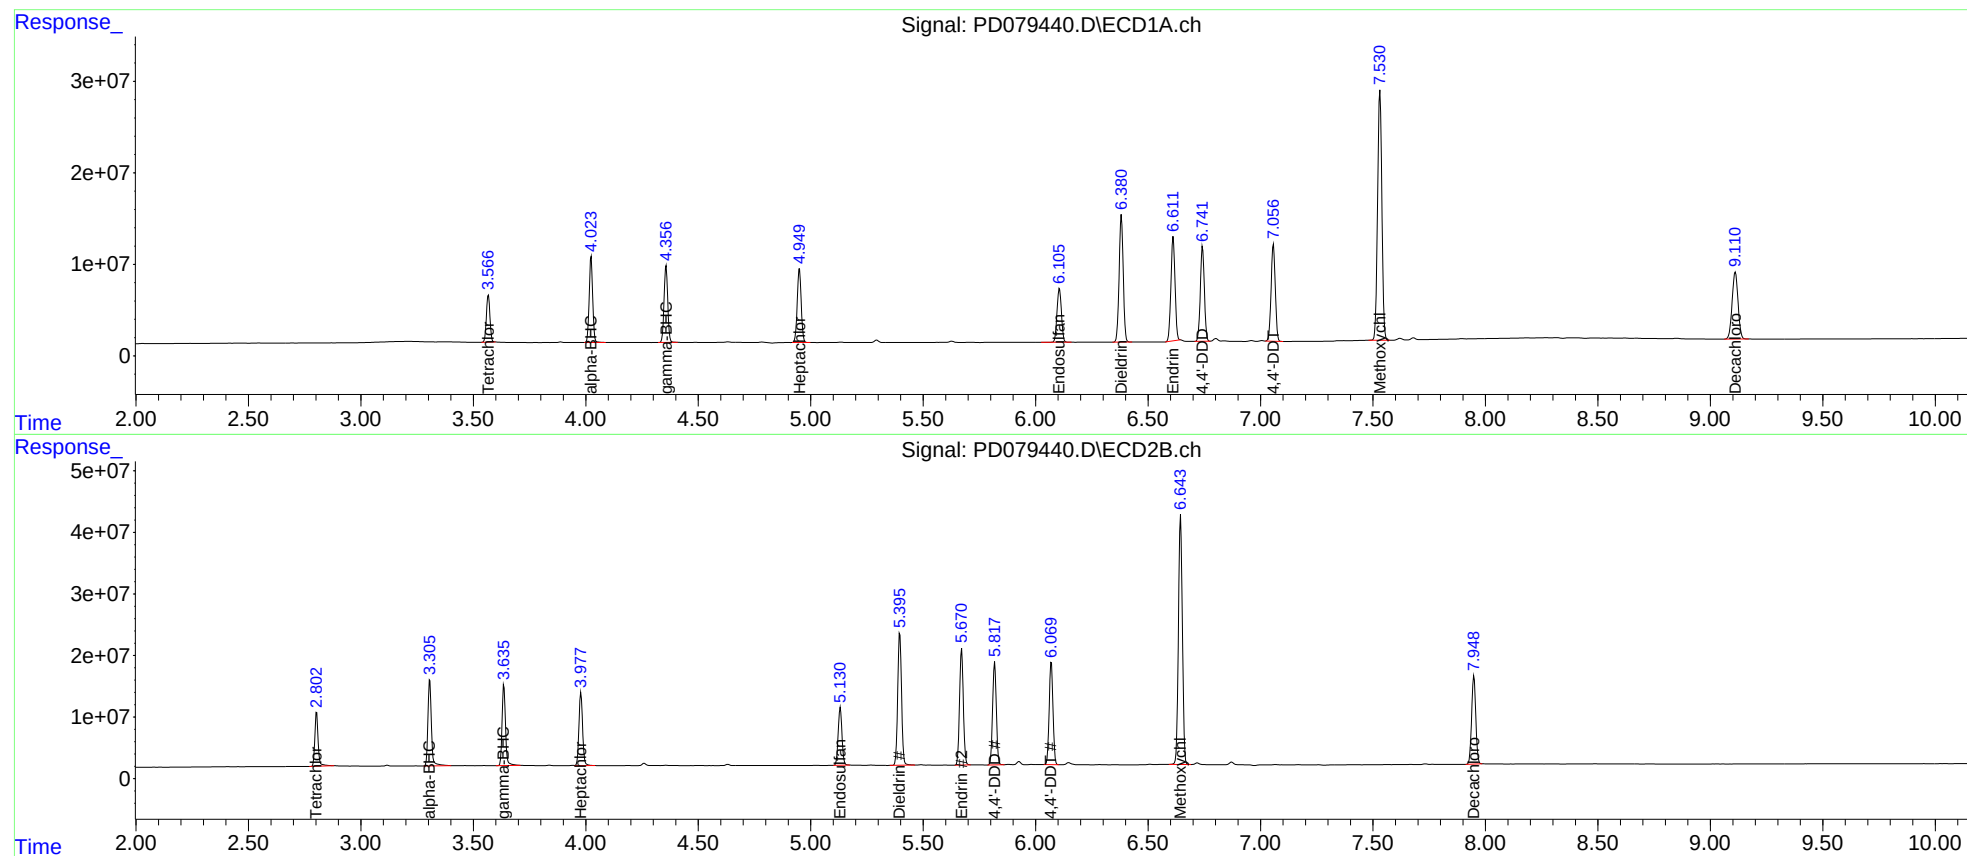

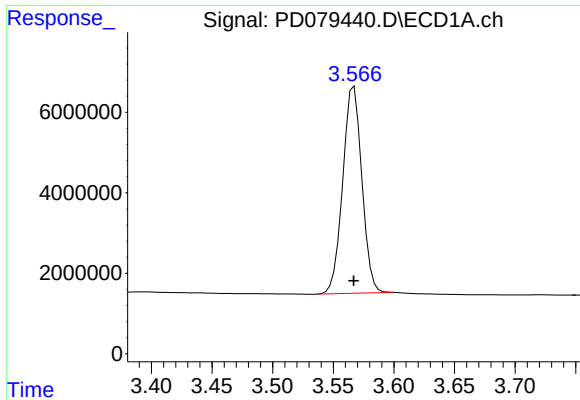


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 56443640
Conc: 38.58 ng/ml

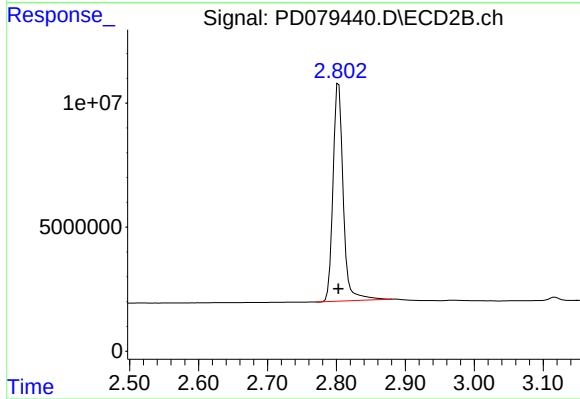


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 90227774
Conc: 39.29 ng/ml

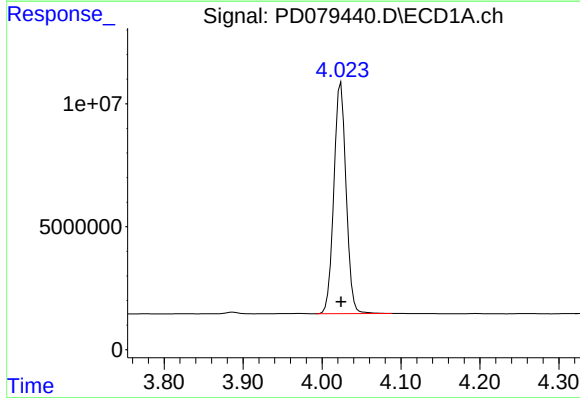


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 101216355
Conc: 41.23 ng/ml

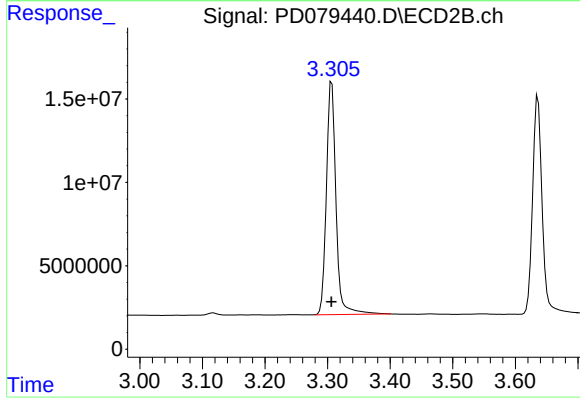

#2 alpha-BHC

R.T.: 3.307 min
Delta R.T.: 0.000 min
Response: 148751086
Conc: 40.90 ng/ml

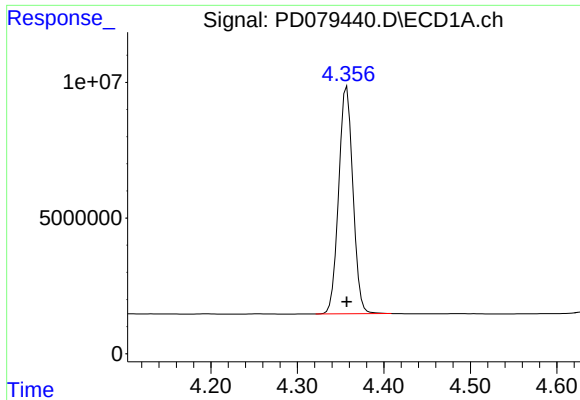


#3 gamma-BHC (Lindane)

R.T.: 4.357 min

Delta R.T.: 0.000 min

Response: 95119161

Conc: 40.49 ng/ml

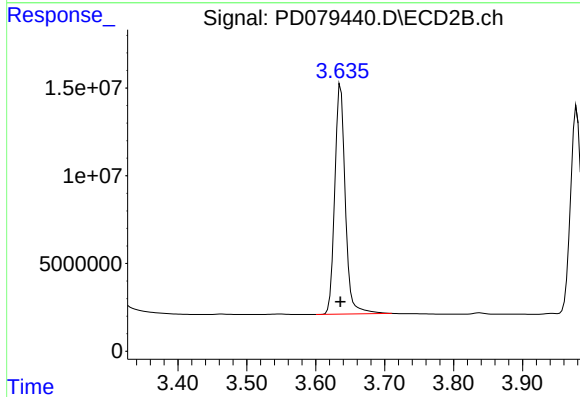


#3 gamma-BHC (Lindane)

R.T.: 3.636 min

Delta R.T.: 0.000 min

Response: 138814657

Conc: 40.30 ng/ml

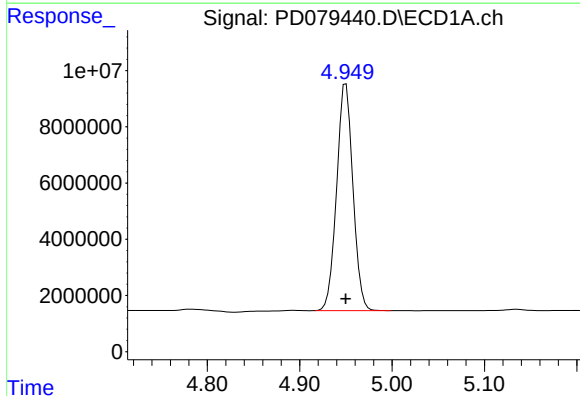


#4 Heptachlor

R.T.: 4.950 min

Delta R.T.: 0.000 min

Response: 99008049

Conc: 39.71 ng/ml

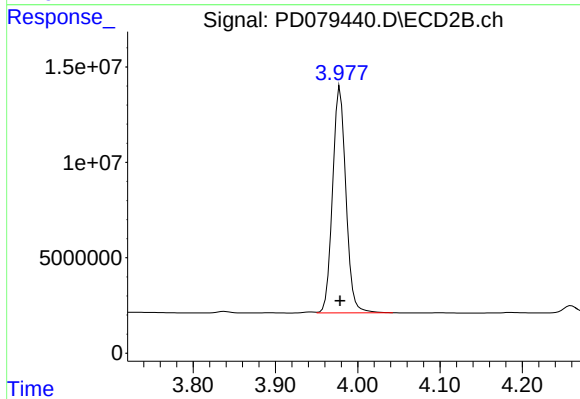


#4 Heptachlor

R.T.: 3.979 min

Delta R.T.: 0.000 min


Response: 133261589

Conc: 40.05 ng/ml

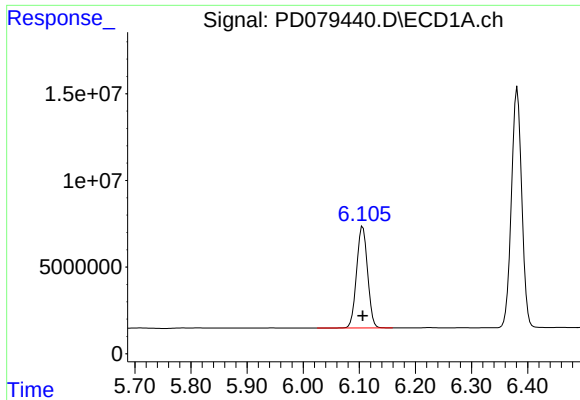


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 79612836
Conc: 38.59 ng/ml

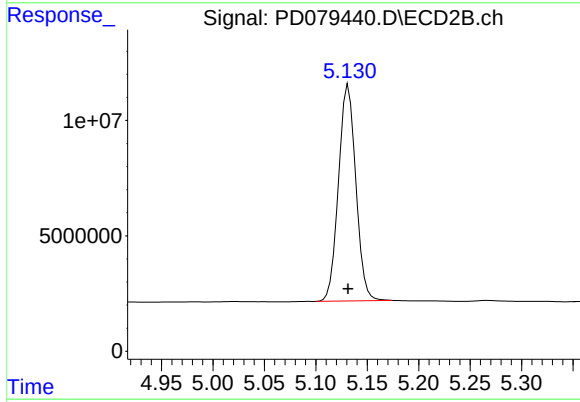


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 109926116
Conc: 39.35 ng/ml

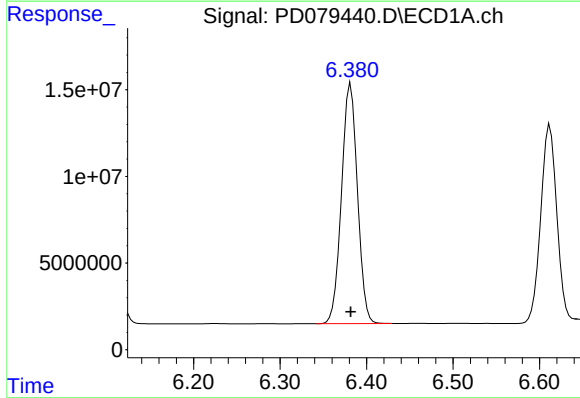


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 176190385
Conc: 80.13 ng/ml

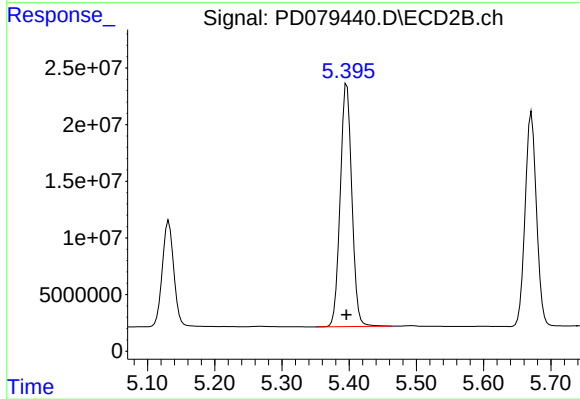


#13 Dieldrin

R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 256133564
Conc: 80.37 ng/ml

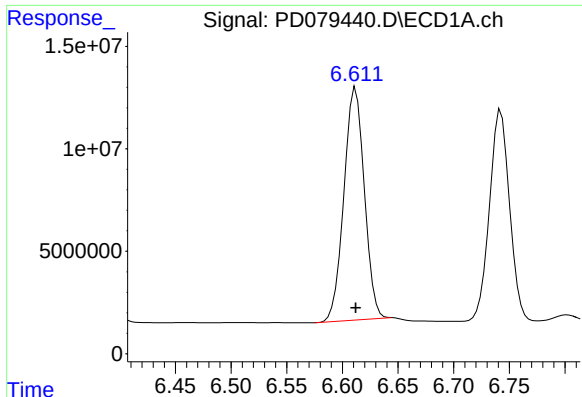


#14 Endrin

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 145032914
Conc: 79.65 ng/ml

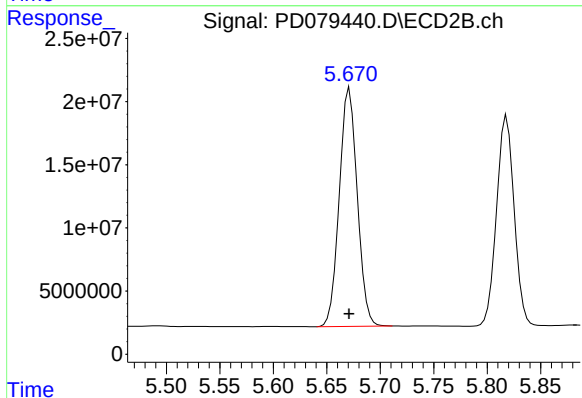


#14 Endrin

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 221265670
Conc: 80.33 ng/ml

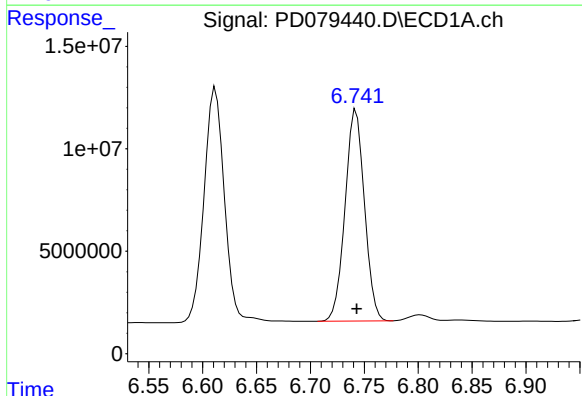


#16 4,4'-DDD

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 129480477
Conc: 79.53 ng/ml

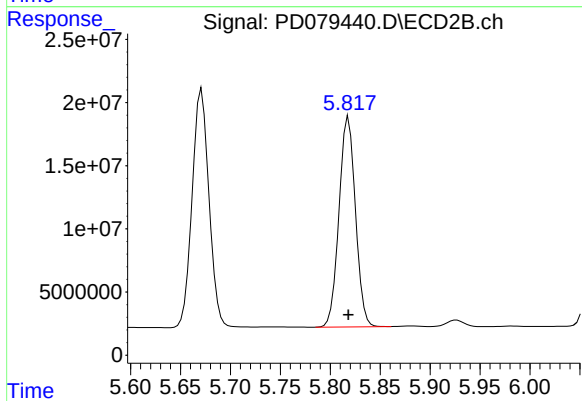


#16 4,4'-DDD

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 190476331
Conc: 80.32 ng/ml

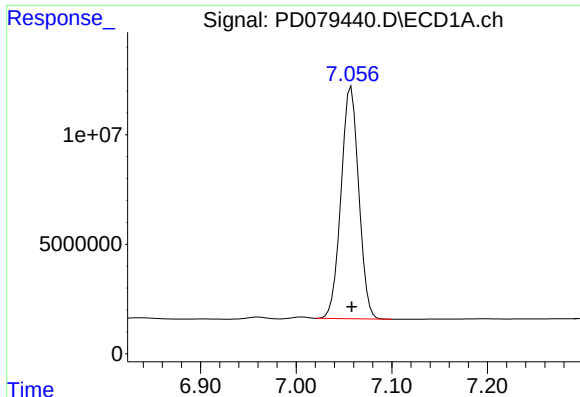


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 136787123
Conc: 79.78 ng/ml

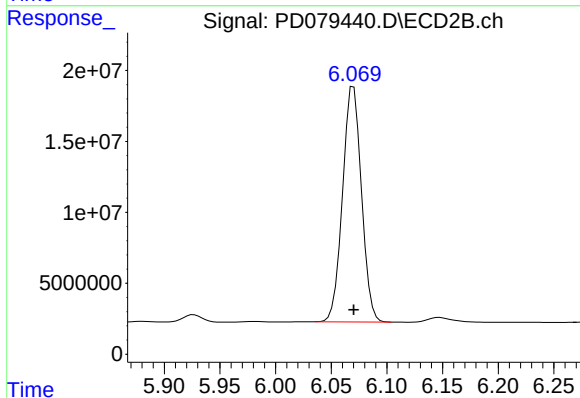


#17 4,4'-DDT

R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 195906245
Conc: 80.55 ng/ml

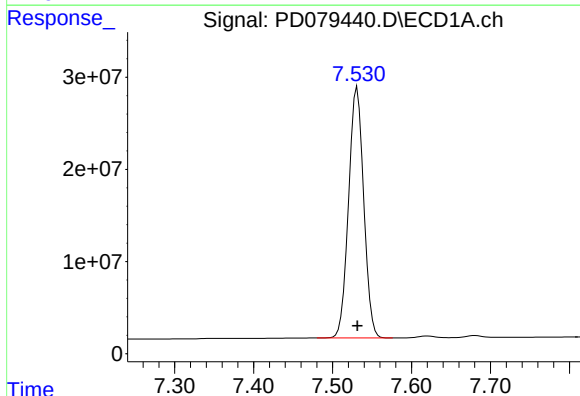


#20 Methoxychlor

R.T.: 7.531 min
Delta R.T.: 0.000 min
Response: 362729774
Conc: 387.26 ng/ml

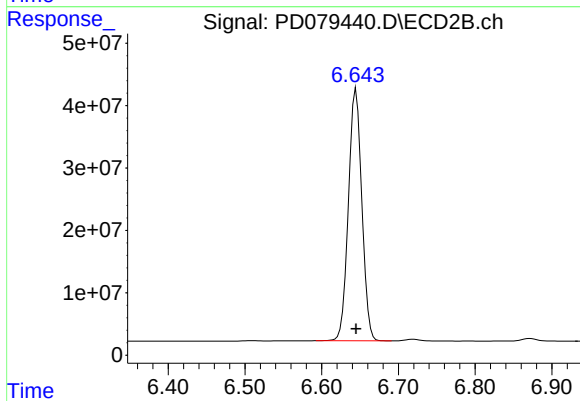


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 494531673
Conc: 374.45 ng/ml

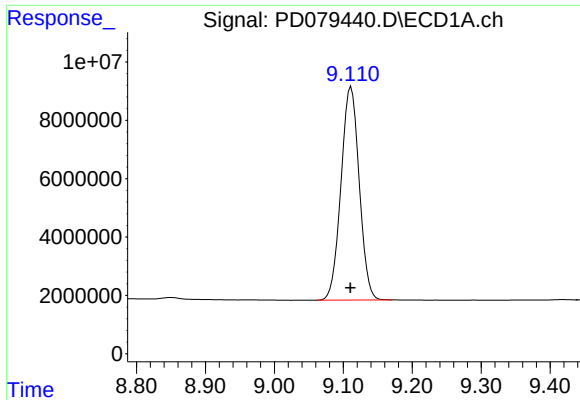

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.001 min
Response: 134278592
Conc: 75.71 ng/ml

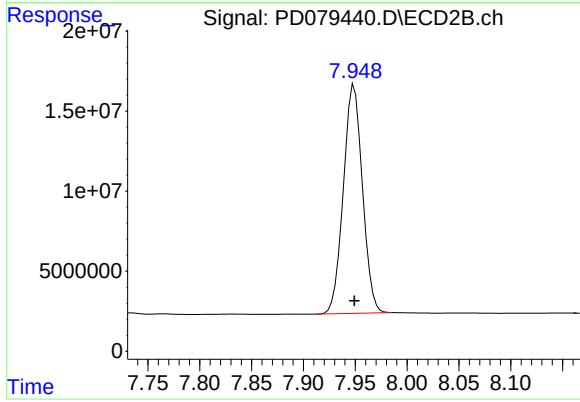

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 183092016
Conc: 76.18 ng/ml