

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
 Data File : PD079442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 23:59
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 06:56:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 06:52:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.803	110.9E6	177.0E6	75.793	77.084
27)	SA Decachlor...	9.111	7.949	255.9E6	355.2E6	144.303	147.813
Target Compounds							
2)	A alpha-BHC	4.024	3.306	209.4E6	300.2E6	85.320	82.545
3)	MA gamma-BHC...	4.358	3.636	194.2E6	279.4E6	82.659	81.119
4)	MA Heptachlor	4.950	3.979	195.8E6	264.7E6	78.538	79.552
9)	A Endosulfan I	6.106	5.132	154.9E6	217.0E6	75.095	77.678
13)	MA Dieldrin	6.382	5.397	352.3E6	510.4E6	160.211	160.138
14)	MA Endrin	6.612	5.672	289.1E6	437.8E6	158.766	158.923
16)	A 4,4'-DDD	6.743	5.818	259.7E6	379.9E6	159.492	160.196
17)	MA 4,4'-DDT	7.058	6.071	274.2E6	394.5E6	159.921	162.203
20)	A Methoxychlor	7.532	6.645	696.9E6	911.8E6	744.086	690.373


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
Data File : PD079442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 23:59
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 06:56:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 06:52:36 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

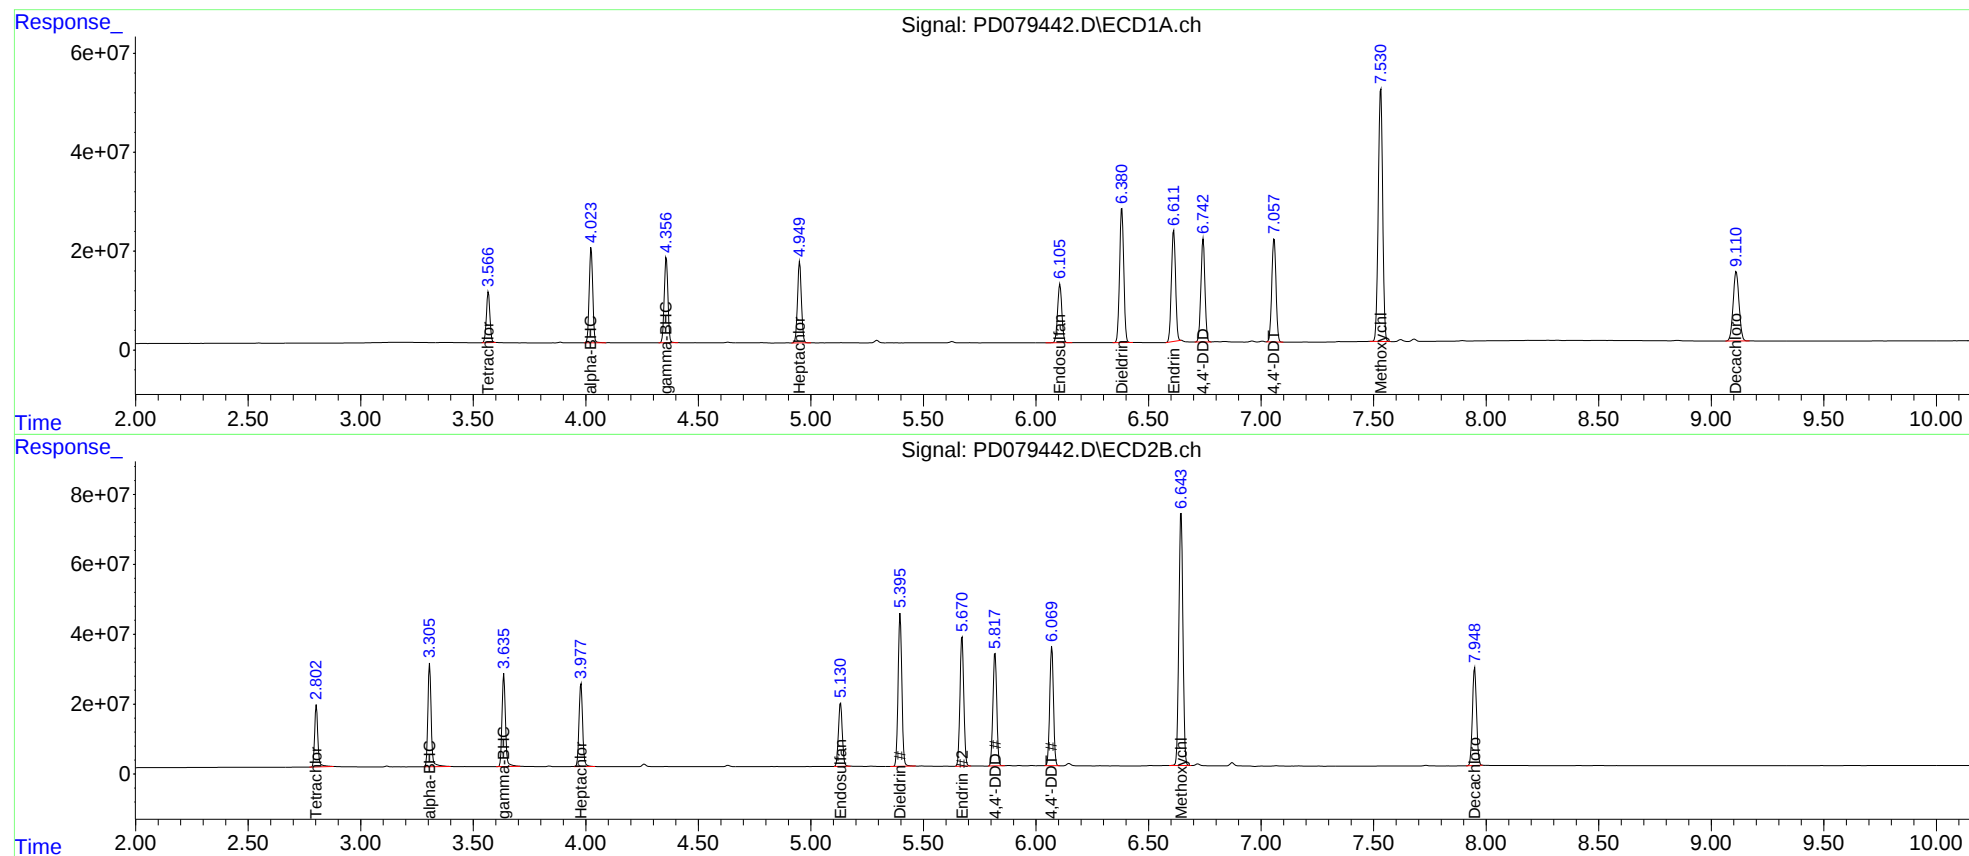

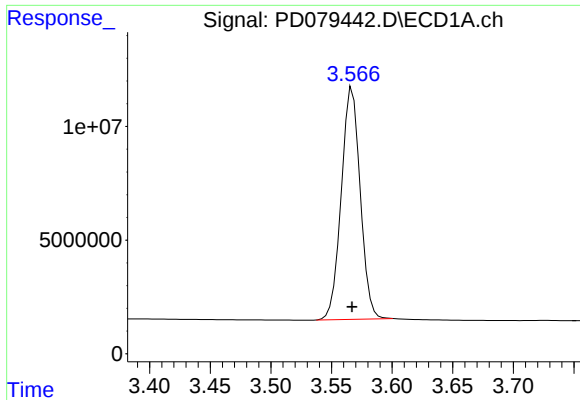


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 110878825
Conc: 75.79 ng/ml

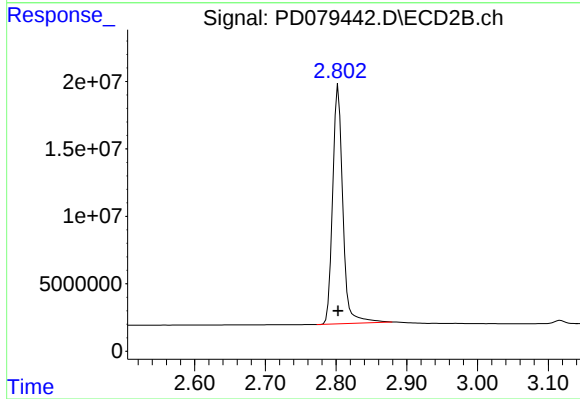


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 177005536
Conc: 77.08 ng/ml

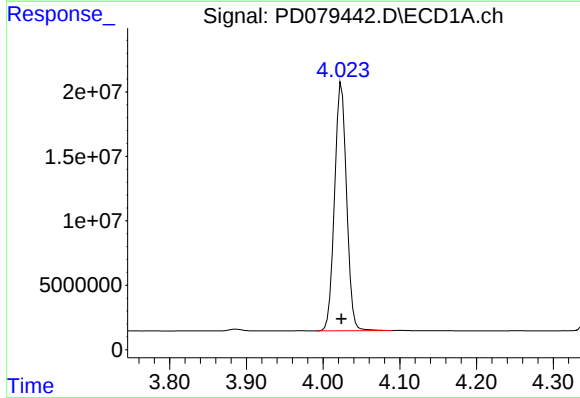


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 209440427
Conc: 85.32 ng/ml

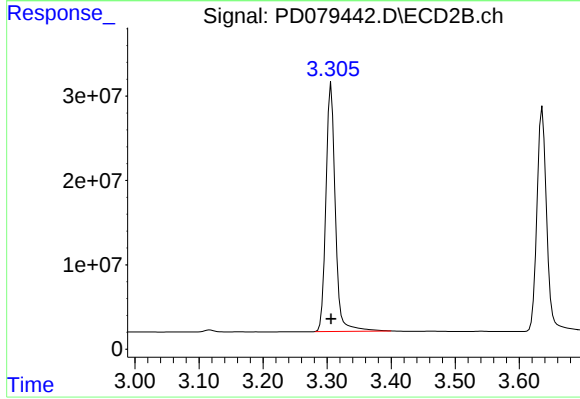


#2 alpha-BHC

R.T.: 3.306 min
Delta R.T.: 0.000 min
Response: 300185668
Conc: 82.55 ng/ml

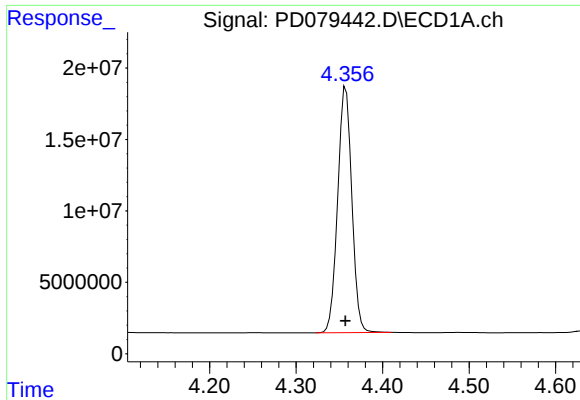


#3 gamma-BHC (Lindane)

R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 194202231
Conc: 82.66 ng/ml

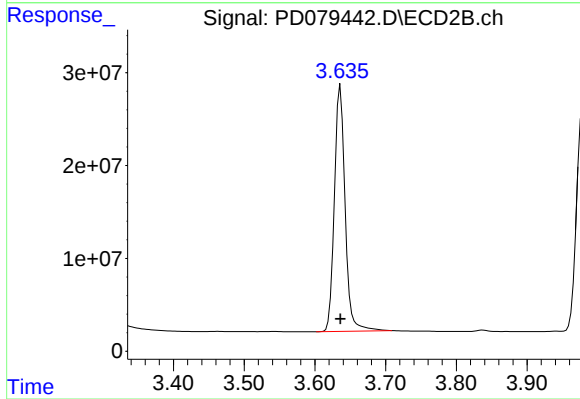


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 279396615
Conc: 81.12 ng/ml

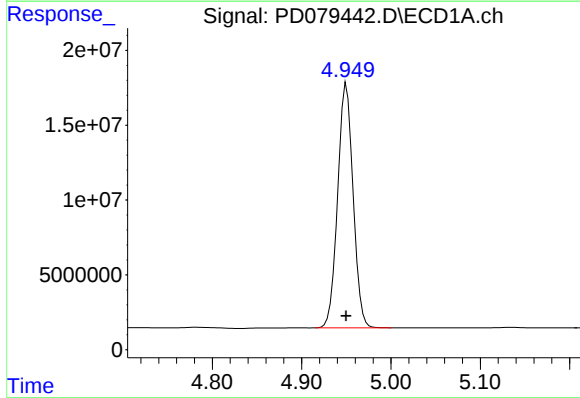


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 195830394
Conc: 78.54 ng/ml

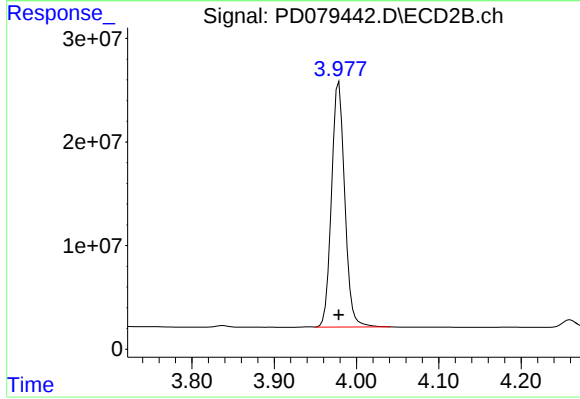


#4 Heptachlor

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 264682574
Conc: 79.55 ng/ml

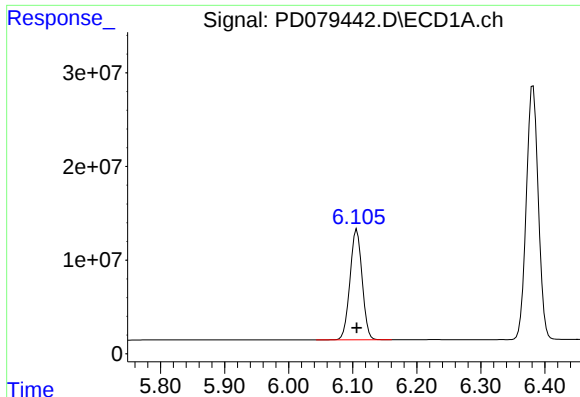


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 154908962
Conc: 75.10 ng/ml

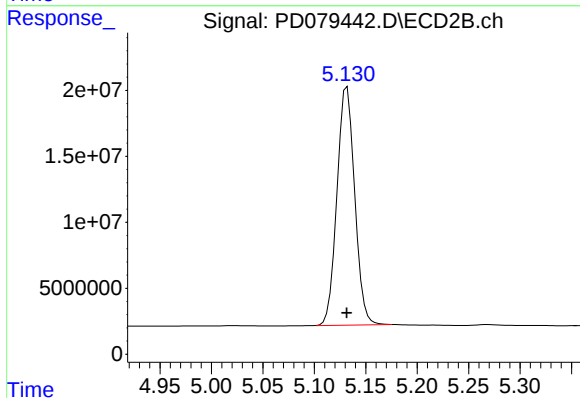


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 216975733
Conc: 77.68 ng/ml

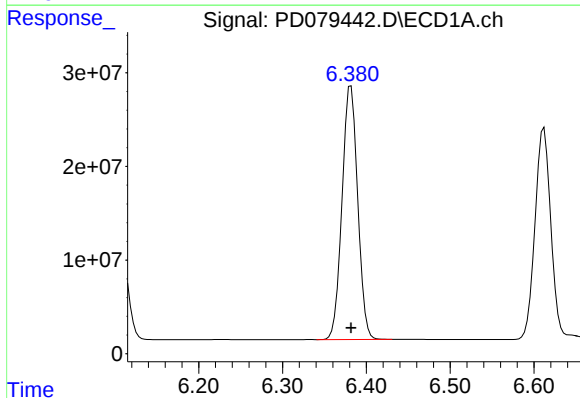


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 352271295
Conc: 160.21 ng/ml

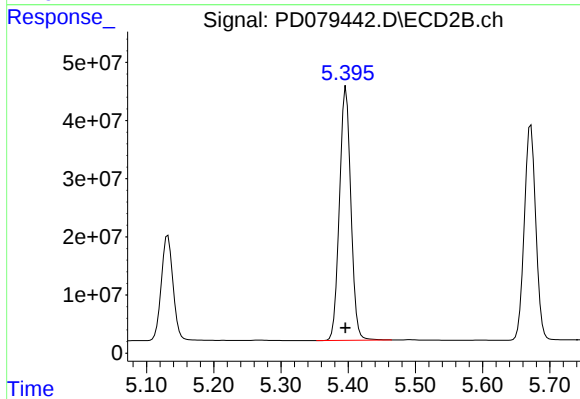


#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 510378316
Conc: 160.14 ng/ml

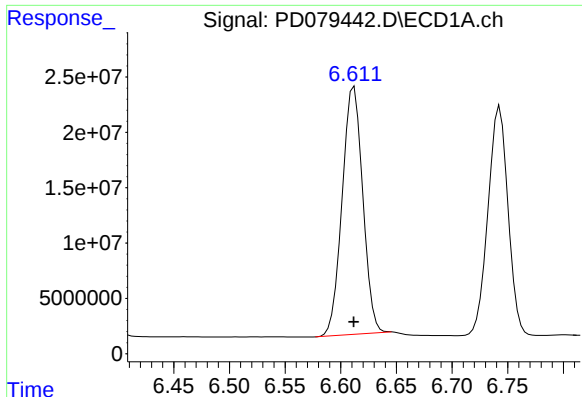


#14 Endrin

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 289080548
Conc: 158.77 ng/ml

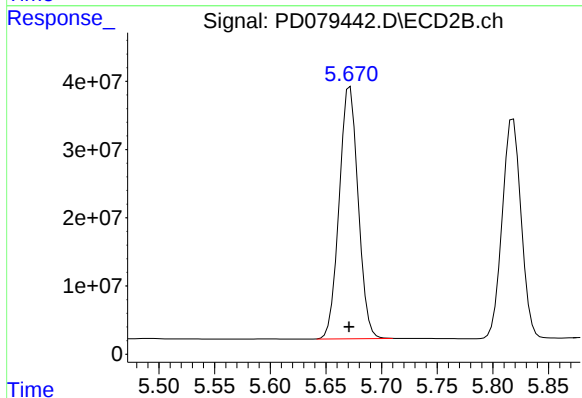


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 437769693
Conc: 158.92 ng/ml

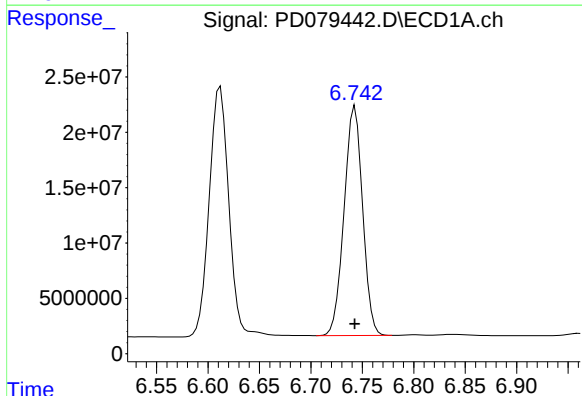


#16 4,4'-DDD

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 259659905
Conc: 159.49 ng/ml

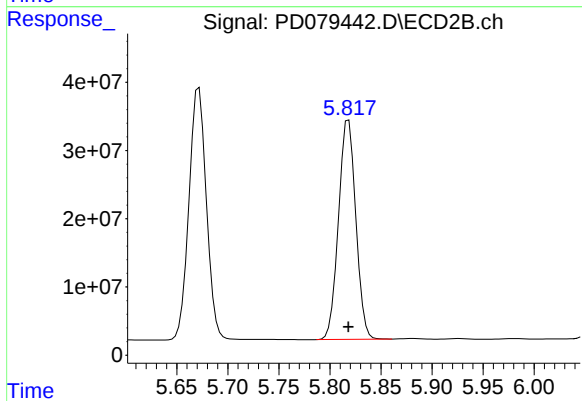


#16 4,4'-DDD

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 379923742
Conc: 160.20 ng/ml

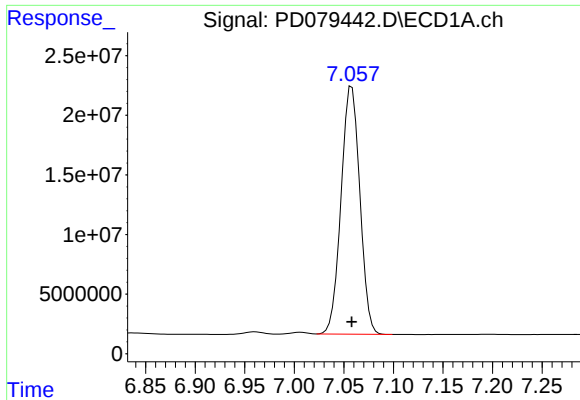


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 274191136
Conc: 159.92 ng/ml

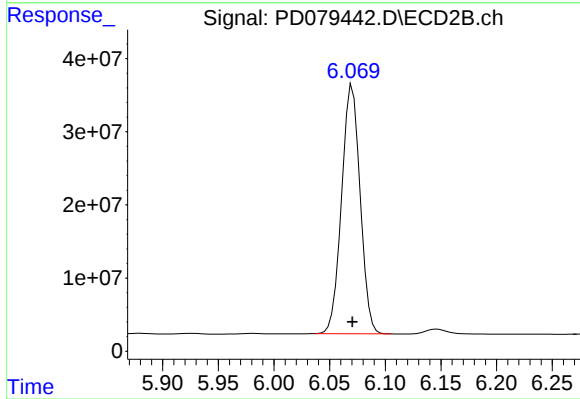


#17 4,4'-DDT

R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 394477354
Conc: 162.20 ng/ml

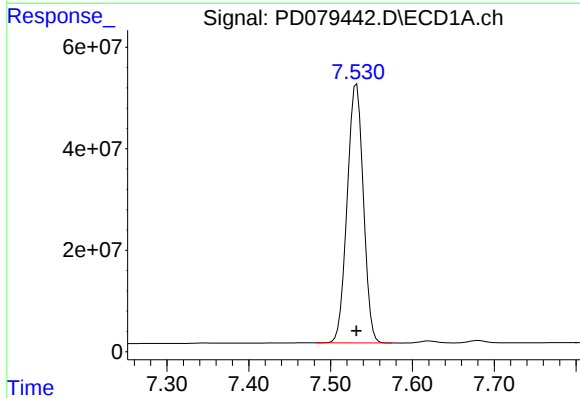


#20 Methoxychlor

R.T.: 7.532 min
Delta R.T.: 0.000 min
Response: 696946154
Conc: 744.09 ng/ml

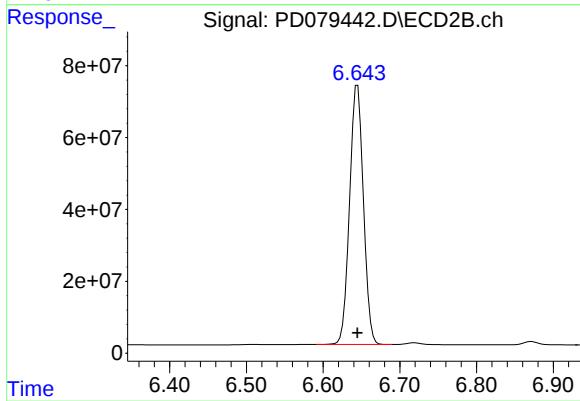


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 911766699
Conc: 690.37 ng/ml

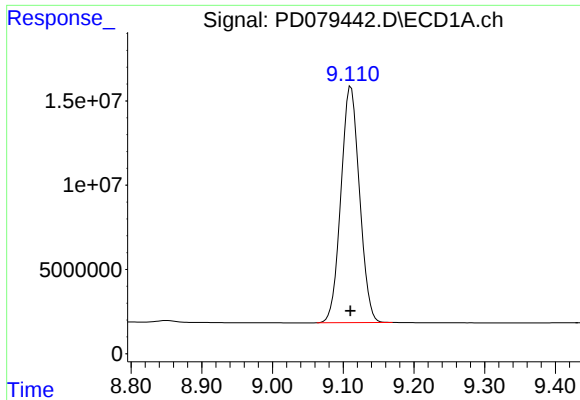

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 255938135
Conc: 144.30 ng/ml

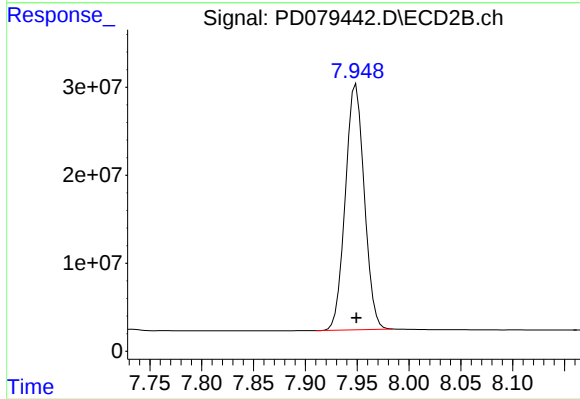

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 355248142
Conc: 147.81 ng/ml