

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
 Data File : PD079427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 20:39
 Operator : AR\AJ
 Sample : RESC013
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 07:16:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.803	29393211	46028661	20.127	20.124
27)	SA Decachlor...	9.111	7.949	70424015	93099368	39.686	38.995
Target Compounds							
2)	A alpha-BHC	4.024	3.306	24466626	36242144	9.875	9.996
3)	MA gamma-BHC...	4.358	3.635	23649195	34868504	10.010	10.149
4)	MA Heptachlor	4.950	3.978	25692325	34081753	10.258	10.216
5)	MB Aldrin	5.293	4.259	24170887	33477289	10.307	10.289
6)	B beta-BHC	4.550	3.931	11436450	16396319	10.533	10.012
7)	B delta-BHC	4.799	4.162	24927090	34767332	10.003	9.731
8)	B Heptachlo...	5.719	4.761	22683480	31091030	10.232	10.052
9)	A Endosulfan I	6.106	5.131	21693975	27408081	10.494	9.887
10)	B trans-Chl...	5.975	5.011	21467250	29298988	10.089	9.869
11)	B cis-Chlor...	6.055	5.075	22131698	29021712	10.162	9.561
12)	B 4,4'-DDE	6.225	5.264	38720621	54393536	19.613	19.425
13)	MA Dieldrin	6.381	5.396	44542572	63540105	20.248	19.955
14)	MA Endrin	6.612	5.671	37126648	55405235	20.348	20.230
15)	B Endosulfa...	6.829	5.963	39002420	50710025	20.501	19.525
16)	A 4,4'-DDD	6.742	5.818	32699514	47393398	20.186	20.132
17)	MA 4,4'-DDT	7.057	6.070	34570337	47752889	20.292	19.880
18)	B Endrin al...	6.959	6.143	30119549	41194790	20.208	20.357
19)	B Endosulfa...	7.193	6.365	37368862	49538510	20.069	19.937
20)	A Methoxychlor	7.532	6.645	94049230	135.9E6	102.022	105.728
21)	B Endrin ke...	7.680	6.871	39068022	57810900	19.996	20.335

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
Data File : PD079427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 20:39
Operator : AR\AJ
Sample : RESC013
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 07:16:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

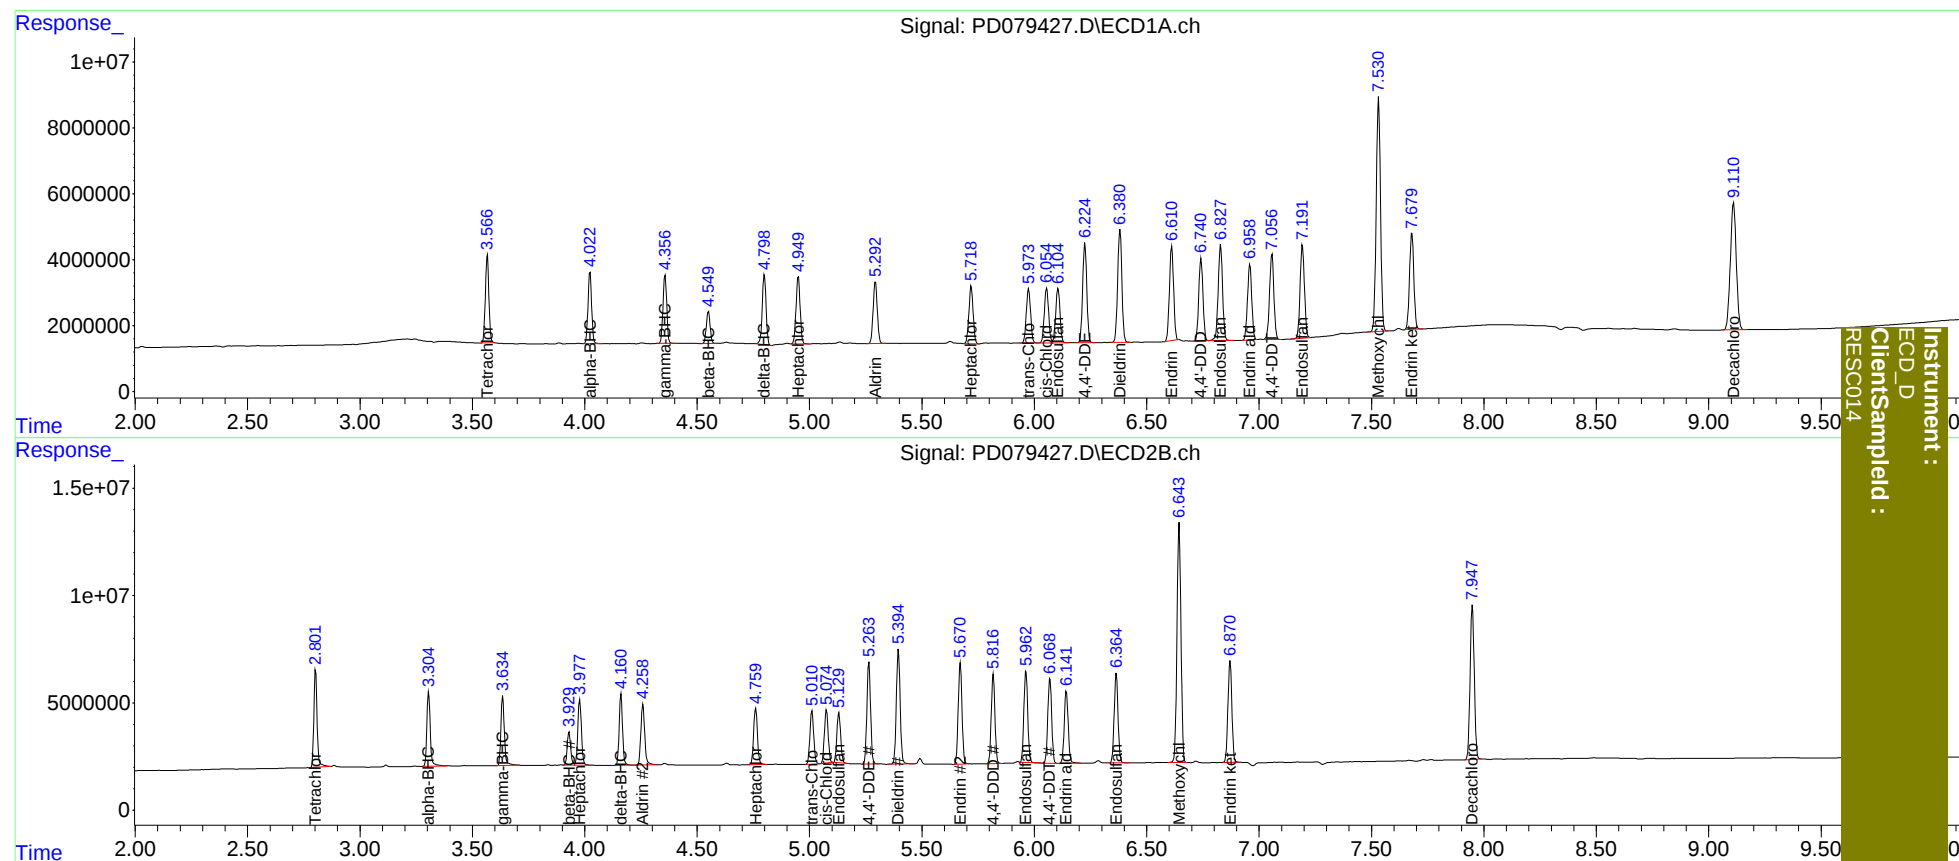

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
Data File : PD079427.D
Acq On : 03 Nov 2023 20:39
Operator : AR\AJ
Sample : RESC013
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Title : GC Extractables
Last Update : Sat Nov 04 07:14:58 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.567	4.024	100.00%
4.024	4.358	100.00%
4.358	4.550	100.00%
4.550	4.799	100.00%
4.799	4.950	100.00%
4.950	5.293	100.00%
5.293	5.719	100.00%
5.719	5.975	100.00%
5.975	6.055	100.00%
6.055	6.106	97.60%
6.106	6.225	100.00%
6.225	6.381	100.00%
6.381	6.612	100.00%
6.612	6.742	100.00%
6.742	6.829	100.00%
6.829	6.959	100.00%
6.959	7.057	100.00%
7.057	7.193	100.00%
7.193	7.532	100.00%
7.532	7.680	100.00%
7.680	9.111	100.00%

Signal #2



2.803	3.306	100.00%
3.306	3.635	100.00%
3.635	3.931	100.00%
3.931	3.978	96.92%
3.978	4.162	100.00%
4.162	4.761	100.00%
4.761	5.011	100.00%
5.011	5.075	100.00%
5.075	5.131	100.00%
5.131	5.264	100.00%
5.264	5.396	100.00%
5.396	5.671	100.00%
5.671	5.818	100.00%
5.818	5.963	100.00%
5.963	6.070	100.00%
6.070	6.143	100.00%
6.143	6.365	100.00%
6.365	6.645	100.00%
6.645	6.871	100.00%
6.871	7.949	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
Data File : PD079427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 20:39
Operator : AR\AJ
Sample : RESC013
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 07:16:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

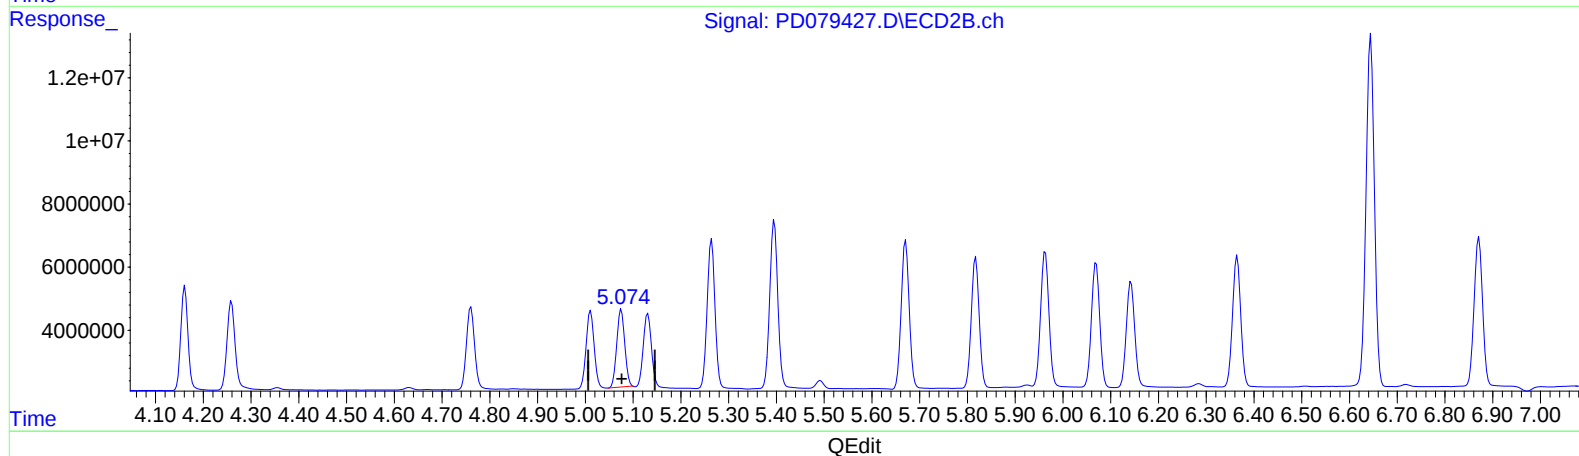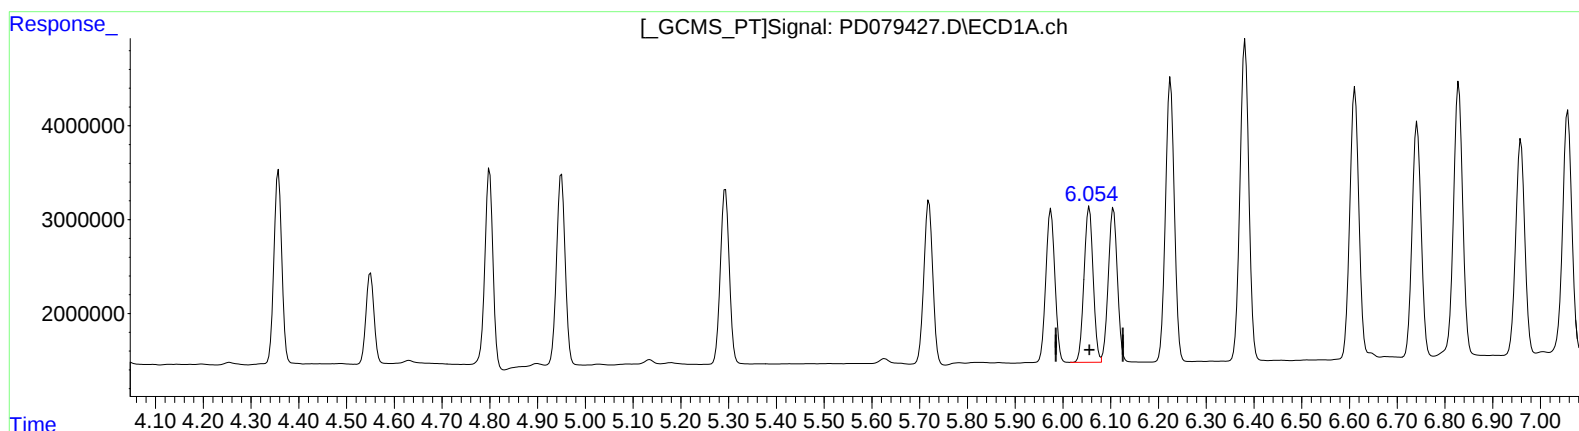

(11) cis-Chlordane (B)

6.055min 10.162 ng/ml

response 22131698

(11) cis-Chlordane #2 (B)

5.075min 9.561 ng/ml


response 29021712

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110623\
Data File : PD079427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 20:39
Operator : AR\AJ
Sample : RESC013
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 07:16:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

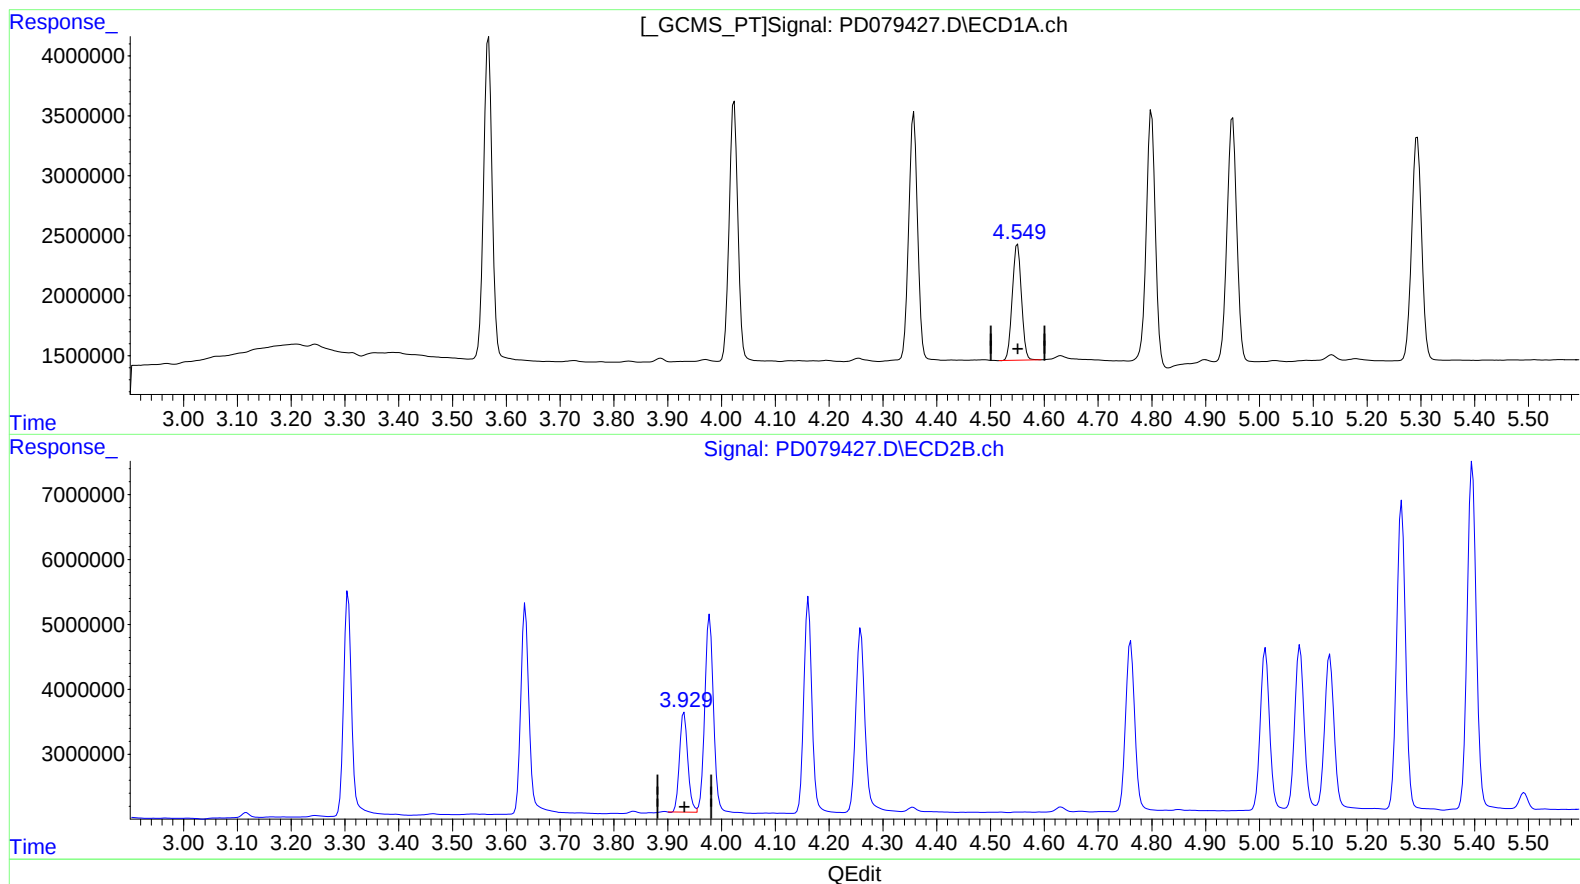

(6) beta-BHC (B)
4.550min 10.533 ng/ml
response 11436450

(6) beta-BHC #2 (B)
3.931min 10.012 ng/ml
response 16396319