

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110625\
 Data File : PD091002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2025 16:40
 Operator : AR\AJ
 Sample : Q3534-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MW-EB-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:28:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.874	240.5E6	954.3E6	77.212	32.050 #
28)	SA Decachlor...	9.062	8.061	79881482	760.3E6	17.076	25.100 #
Target Compounds							
2)	A alpha-BHC	3.981	0.000	45724168	0	6.371	N.D. #
4)	MA Heptachlor	0.000	4.099f	0	46185659	N.D.	1.035 #
7)	B delta-BHC	4.782f	0.000	1077.7E6	0	159.381	N.D. #
8)	B Heptachlo...	0.000	4.891f	0	131916.8E6	N.D.	3093.809 #
19)	B Endosulfa...	0.000	6.460	0	4305329	N.D.	0.120 #
20)	A Methoxychlor	7.510f	6.742	4417847	43103765	2.078	2.473
27)	Chlordane-5	6.861	0.000	10123828	0	67.376	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110625\
Data File : PD091002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2025 16:40
Operator : AR\AJ
Sample : Q3534-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MW-EB-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:28:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

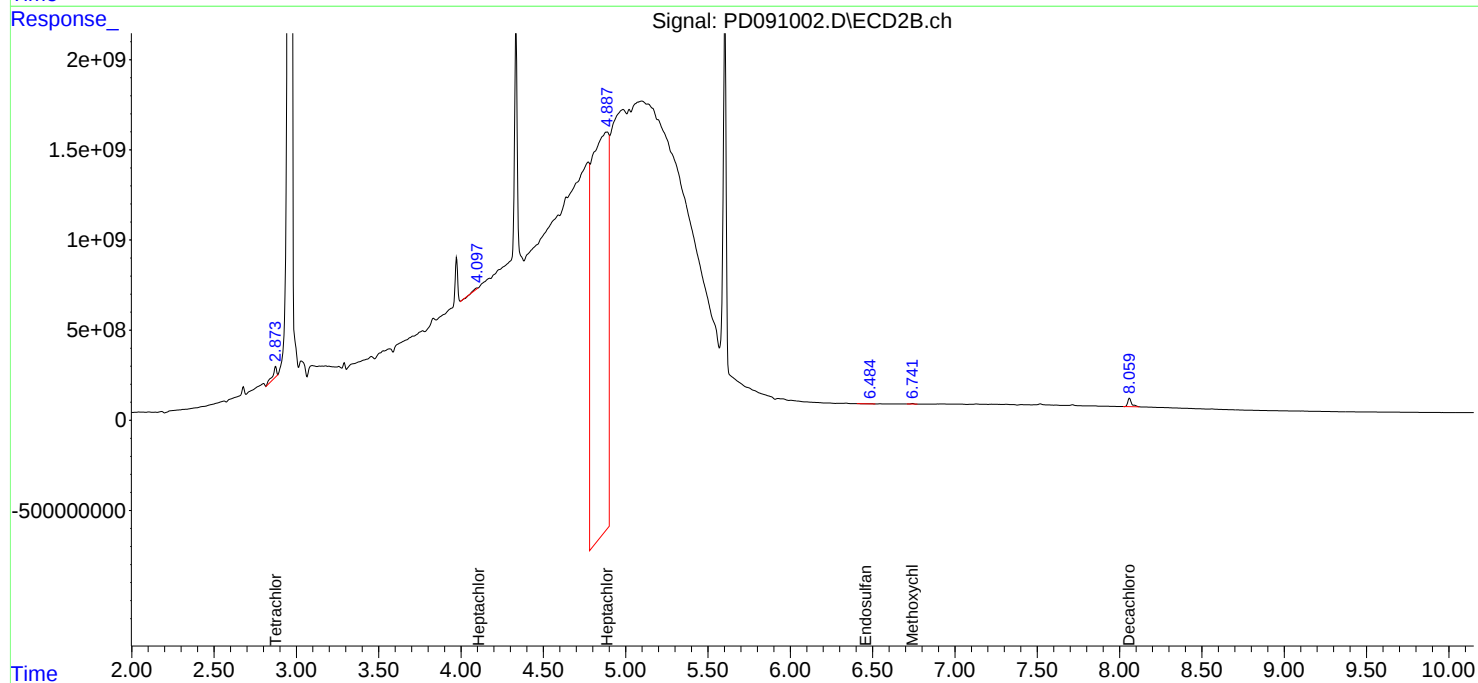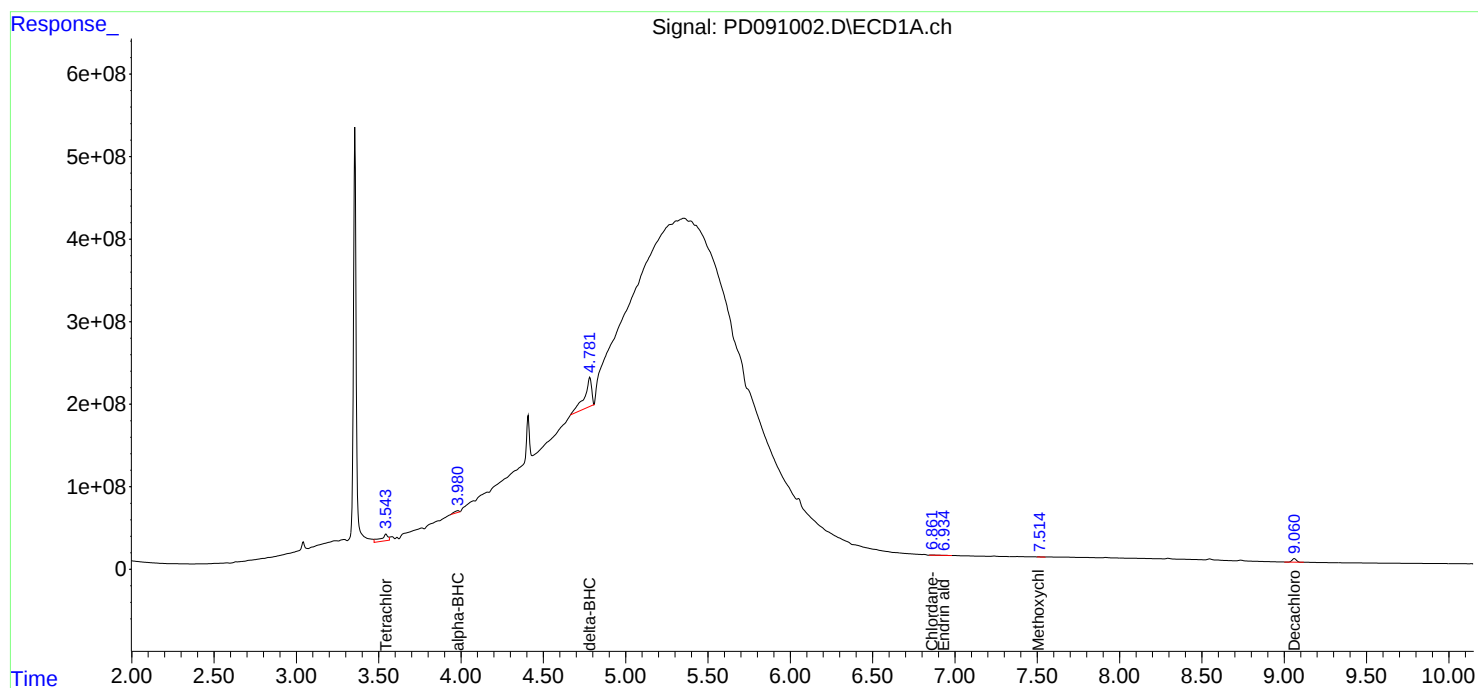


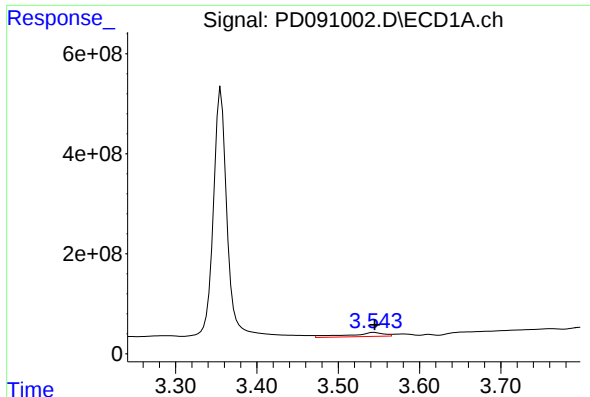

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 240451570
Conc: 77.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
MW-EB-3

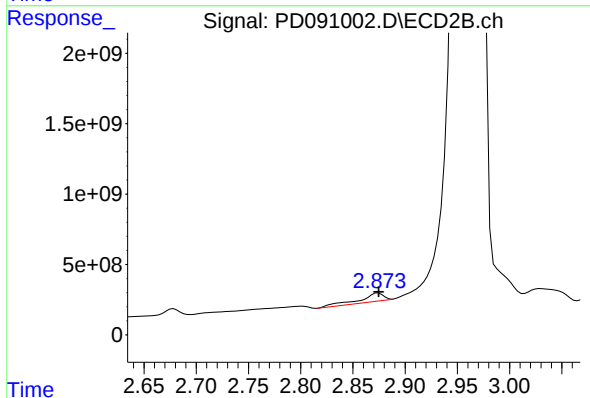


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: 0.000 min
Response: 954342961
Conc: 32.05 ng/ml

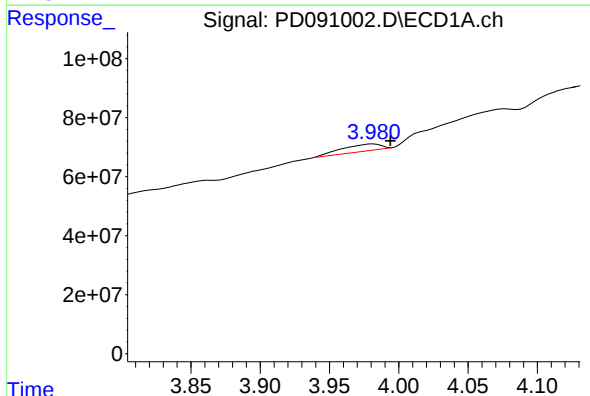


#2 alpha-BHC

R.T.: 3.981 min
Delta R.T.: -0.013 min
Response: 45724168
Conc: 6.37 ng/ml

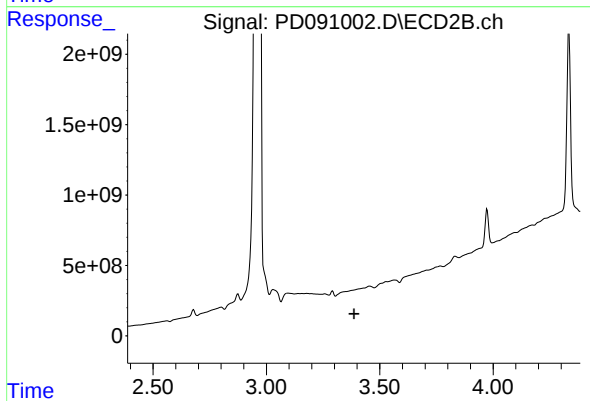

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.387 min
Response: 0
Conc: N.D.

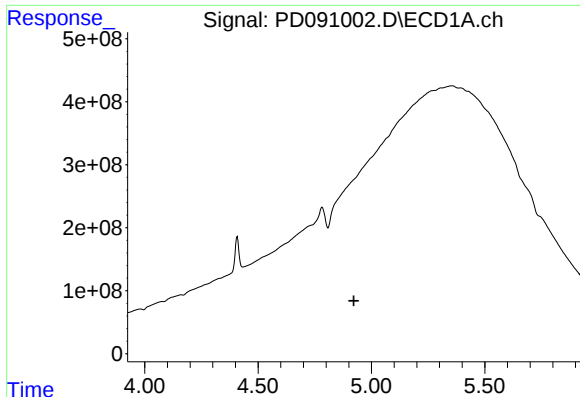

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.923 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
MW-EB-3

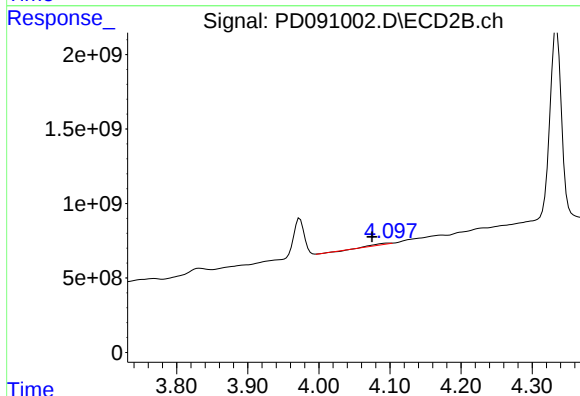


#4 Heptachlor

R.T.: 4.099 min
Delta R.T.: 0.024 min
Response: 46185659
Conc: 1.04 ng/ml

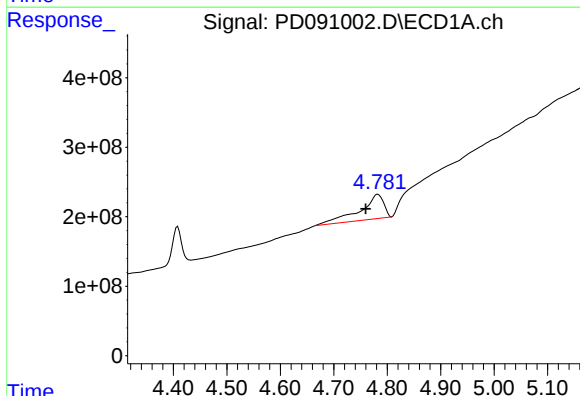


#7 delta-BHC

R.T.: 4.782 min
Delta R.T.: 0.022 min
Response: 1077691373
Conc: 159.38 ng/ml

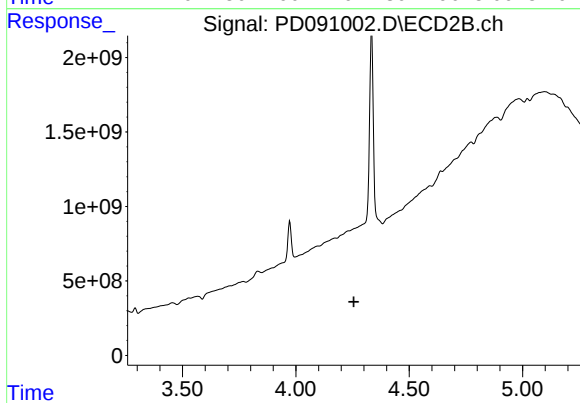

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.255 min
Response: 0
Conc: N.D.

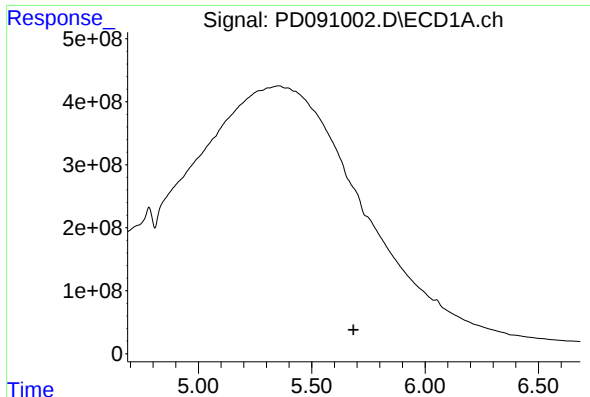

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.684 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
MW-EB-3

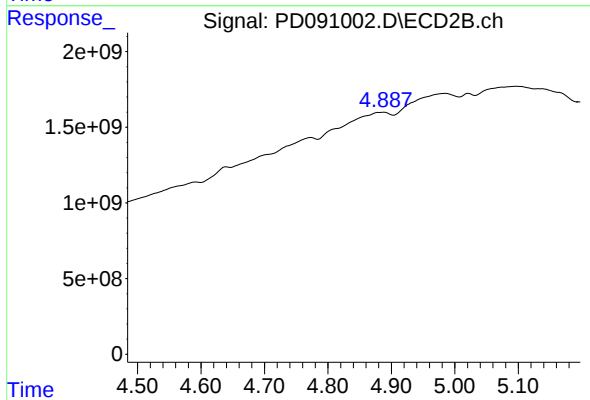


#8 Heptachlor epoxide

R.T.: 4.891 min
Delta R.T.: 0.027 min
Response: 1.31917e+011
Conc: 3093.81 ng/ml

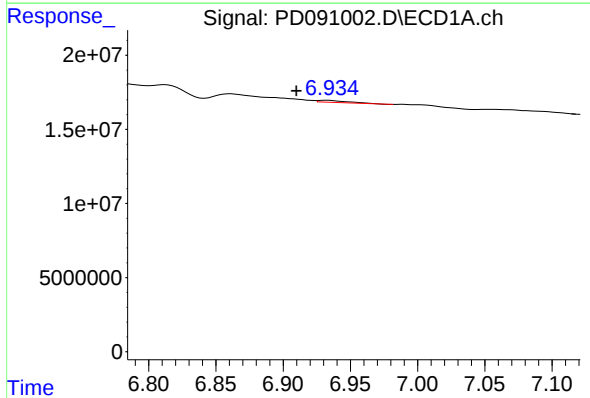


#18 Endrin aldehyde

R.T.: 6.933 min
Delta R.T.: 0.023 min
Response: 2185768
Conc: 0.60 ng/ml

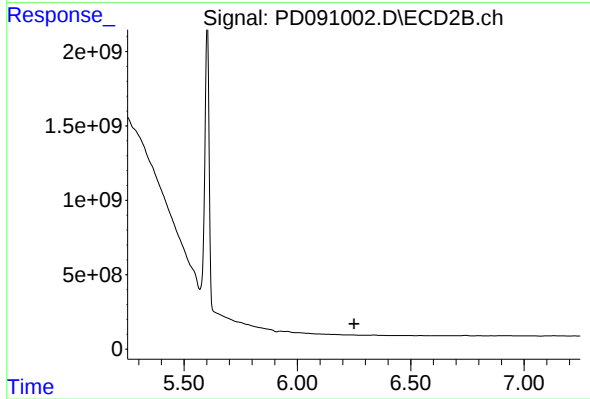

#18 Endrin aldehyde


R.T.: 6.224 min
Delta R.T.: -0.026 min
Response: -40207589
Conc: N.D.

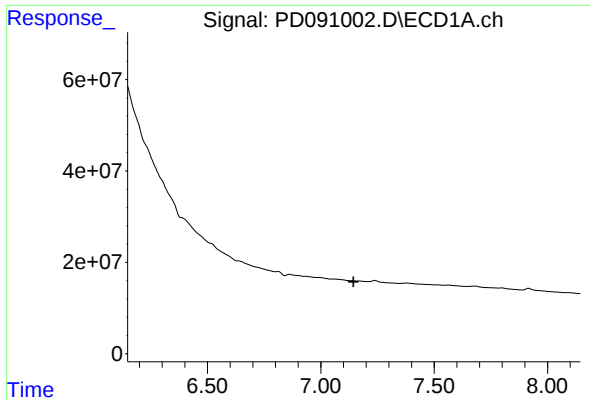

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
MW-EB-3

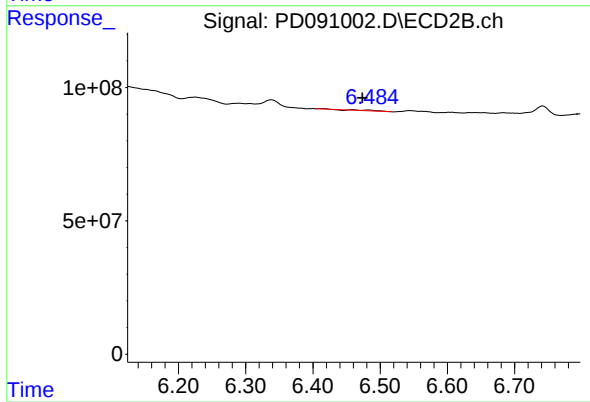


#19 Endosulfan Sulfate

R.T.: 6.460 min
Delta R.T.: -0.014 min
Response: 4305329
Conc: 0.12 ng/ml

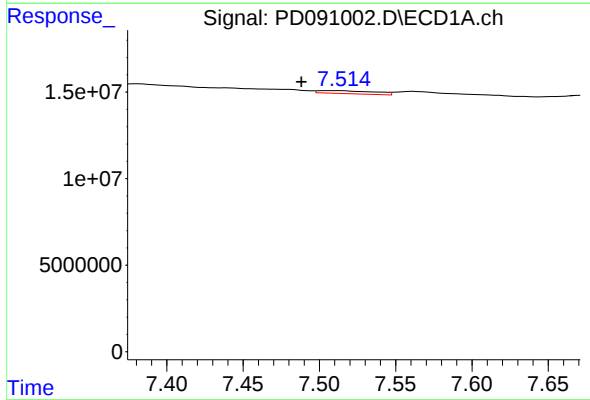


#20 Methoxychlor

R.T.: 7.510 min
Delta R.T.: 0.022 min
Response: 4417847
Conc: 2.08 ng/ml

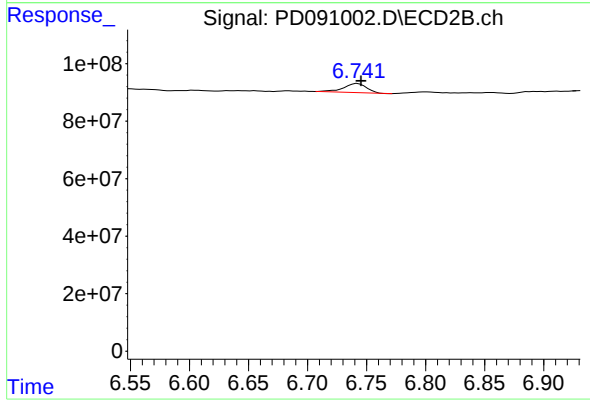

#20 Methoxychlor


R.T.: 6.742 min
Delta R.T.: -0.003 min
Response: 43103765
Conc: 2.47 ng/ml

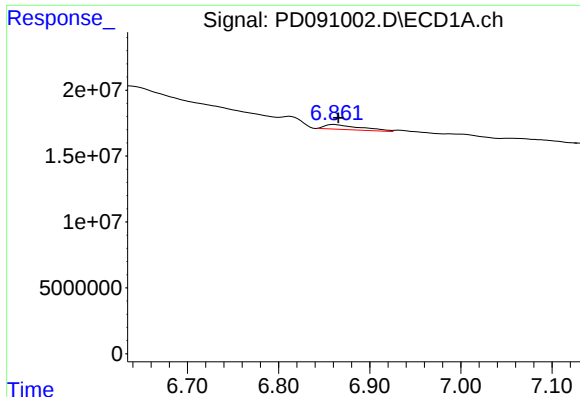

#27 Chlordane-5


R.T.: 6.861 min
Delta R.T.: -0.004 min
Response: 10123828
Conc: 67.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
MW-EB-3

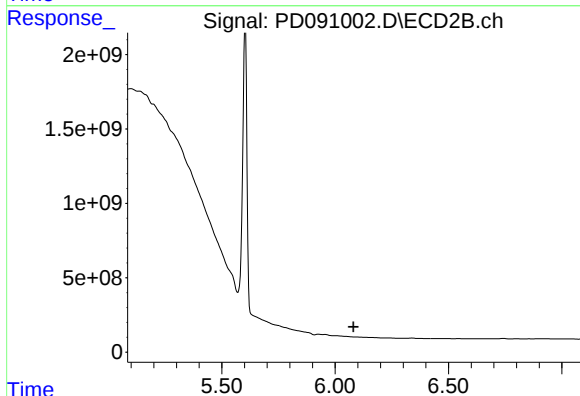


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.081 min
Response: 0
Conc: N.D.

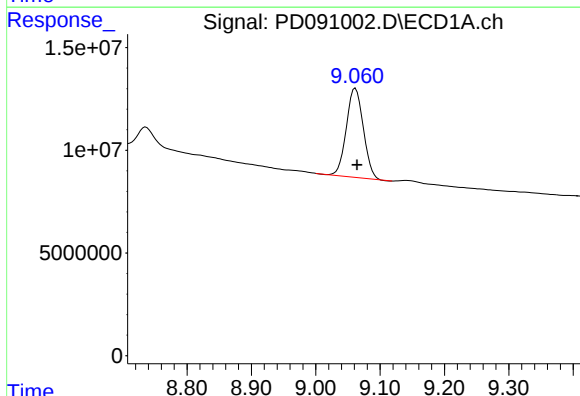

#28 Decachlorobiphenyl

R.T.: 9.062 min
Delta R.T.: -0.003 min
Response: 79881482
Conc: 17.08 ng/ml

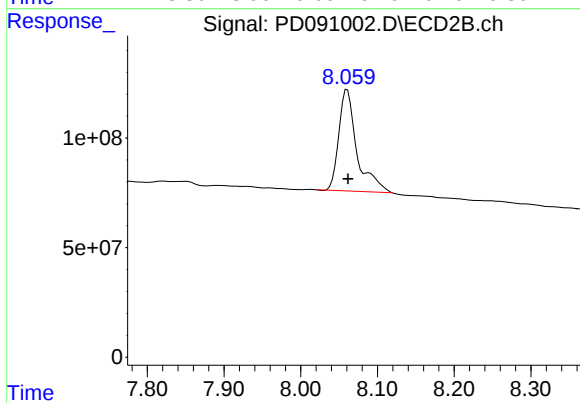

#28 Decachlorobiphenyl

R.T.: 8.061 min
Delta R.T.: -0.001 min
Response: 760320417
Conc: 25.10 ng/ml