

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
 Data File : PD079447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2023 10:55
 Operator : AR\AJ
 Sample : PIBLK066
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 05:01:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.803	34497751	54116837	23.623	23.660
27)	SA Decachlor...	9.115	7.950	80958375	111.1E6	45.622	46.551
Target Compounds							
2)	A alpha-BHC	0.000	3.295	0	117410	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.656	0	648020	N.D.	0.189
4)	MA Heptachlor	0.000	3.943f	0	978827	N.D.	0.293
5)	MB Aldrin	0.000	4.266	0	809564	N.D.	0.249
6)	B beta-BHC	0.000	3.943	0	978827	N.D.	0.598
7)	B delta-BHC	4.794	4.185	4927563	326924	1.977	<MDL #
8)	B Heptachlo...	0.000	4.790	0	866975	N.D.	0.280
10)	B trans-Chl...	6.008	0.000	1625307	0	0.764	N.D. #
11)	B cis-Chlor...	6.008f	0.000	1625307	0	0.746	N.D. #
13)	MA Dieldrin	0.000	5.446f	0	175756	N.D.	<MDL
15)	B Endosulfa...	0.000	5.996	0	213810	N.D.	<MDL
16)	A 4,4'-DDD	0.000	5.843	0	76486	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
Data File : PD079447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2023 10:55
Operator : AR\AJ
Sample : PIBLK066
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 05:01:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

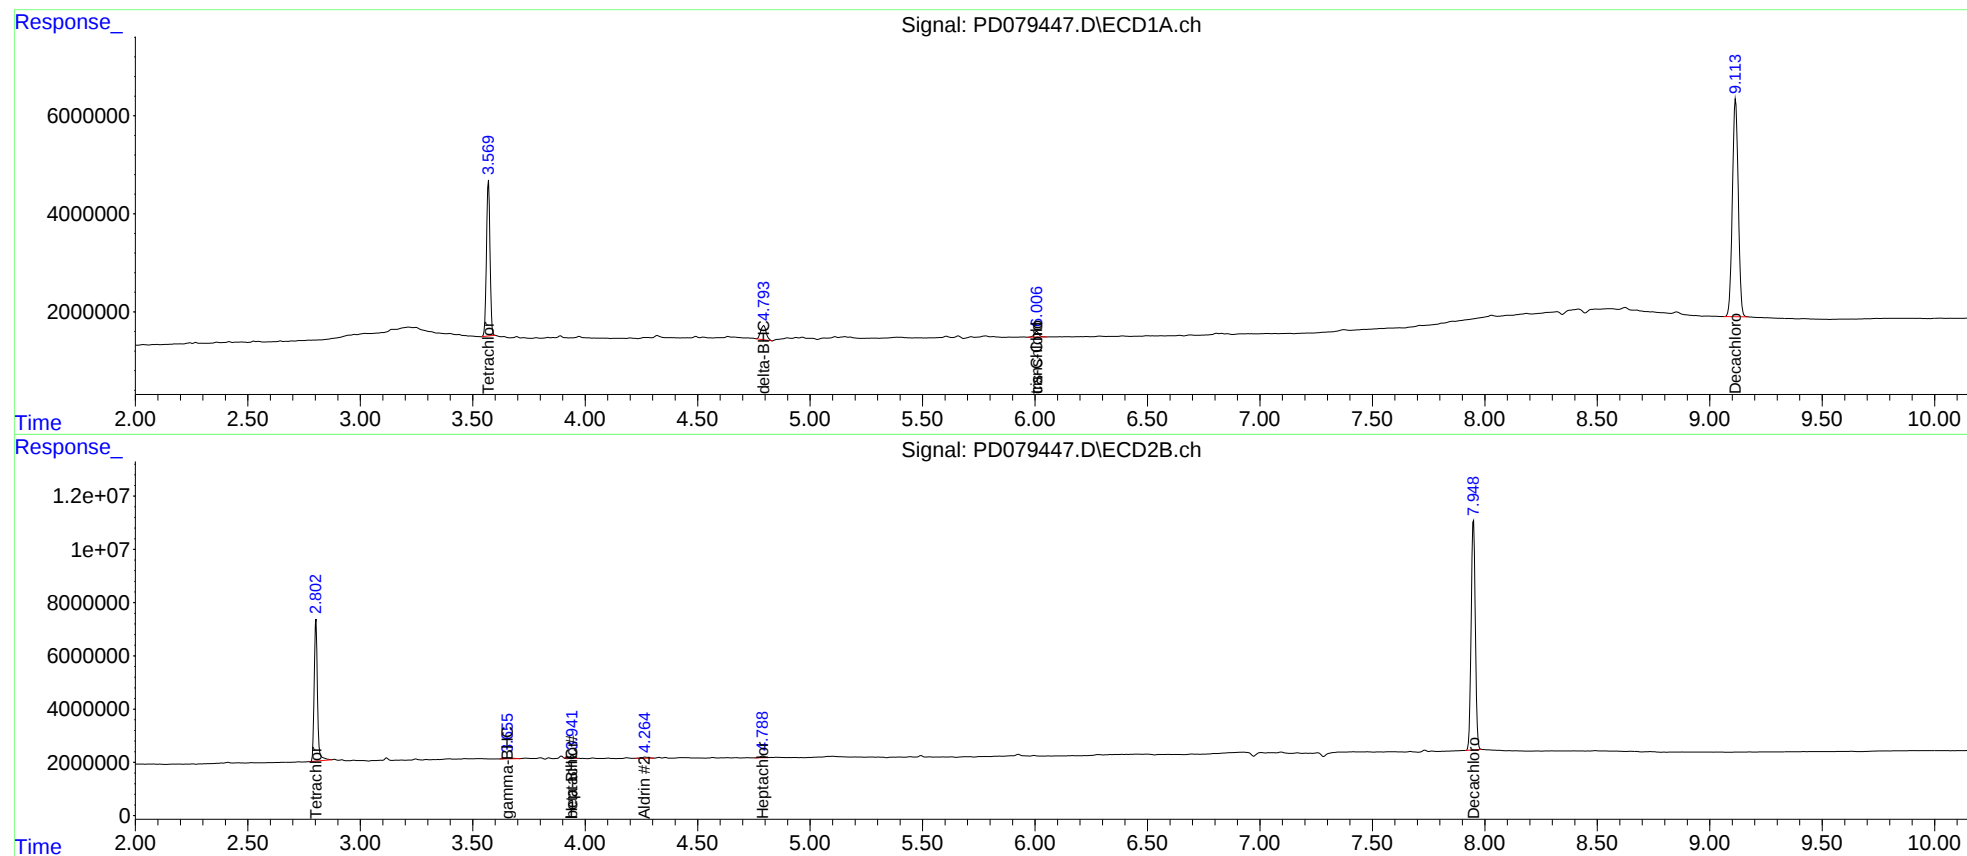

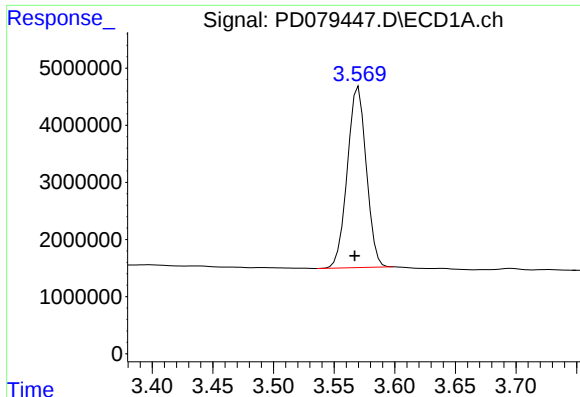


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: 0.003 min
Response: 34497751
Conc: 23.62 ng/ml

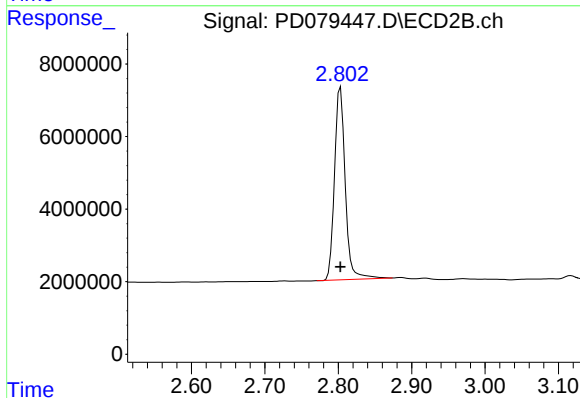


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 54116837
Conc: 23.66 ng/ml

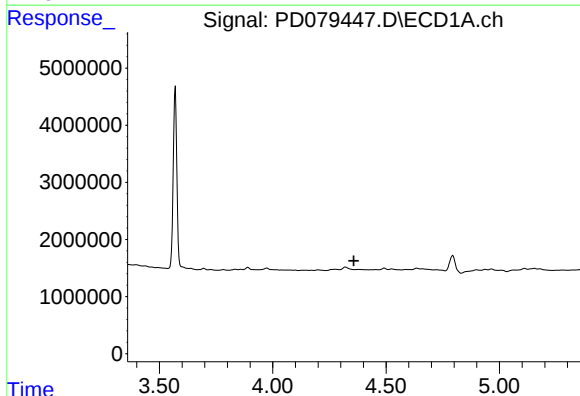


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

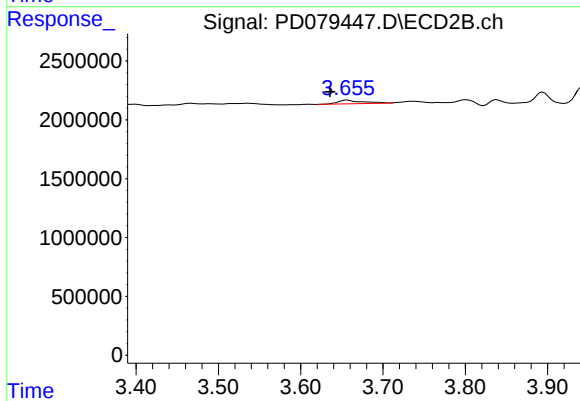


#3 gamma-BHC (Lindane)

R.T.: 3.656 min
Delta R.T.: 0.020 min
Response: 648020
Conc: 0.19 ng/ml

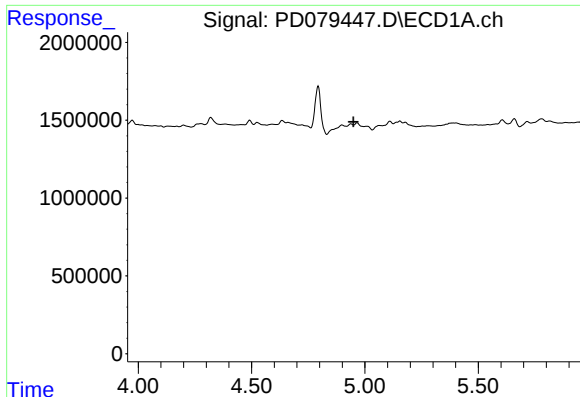


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.950 min
Response: 0
Conc: N.D.

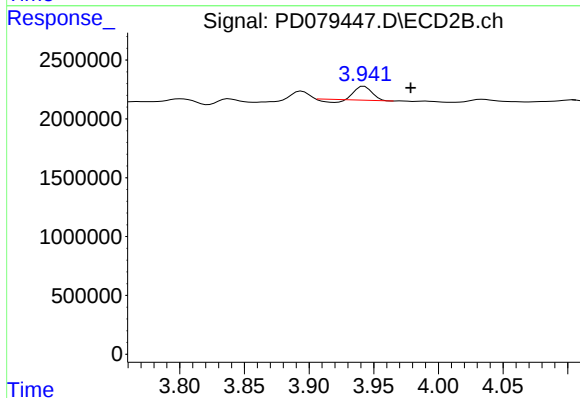


#4 Heptachlor

R.T.: 3.943 min
Delta R.T.: -0.036 min
Response: 978827
Conc: 0.29 ng/ml

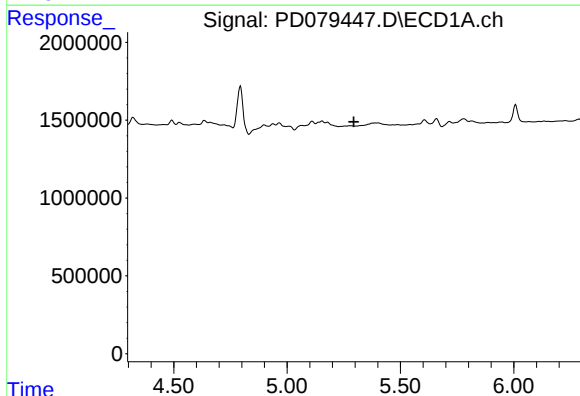


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

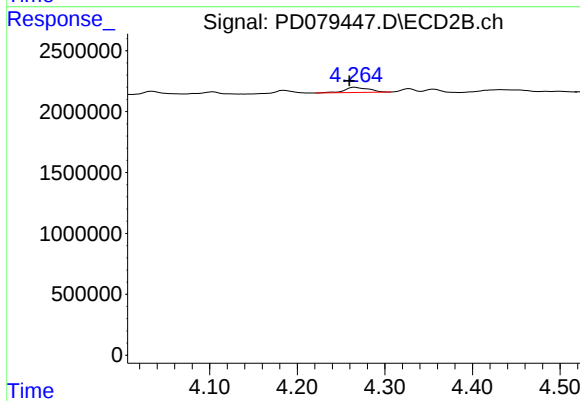


#5 Aldrin

R.T.: 4.266 min
Delta R.T.: 0.006 min
Response: 809564
Conc: 0.25 ng/ml

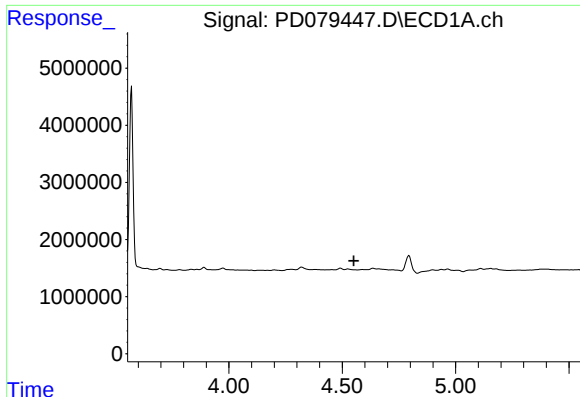


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

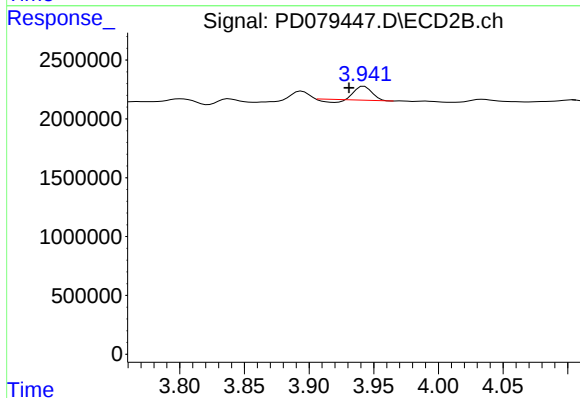


#6 beta-BHC

R.T.: 3.943 min
Delta R.T.: 0.012 min
Response: 978827
Conc: 0.60 ng/ml

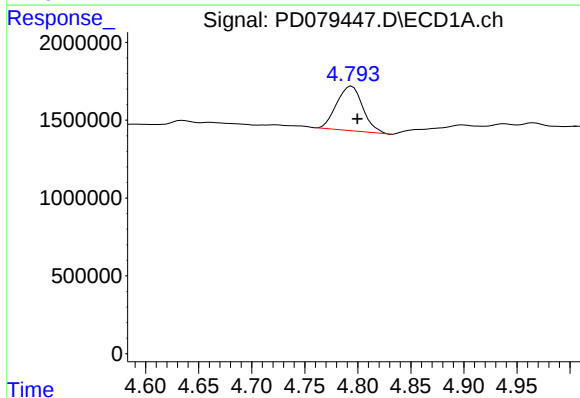


#7 delta-BHC

R.T.: 4.794 min
Delta R.T.: -0.006 min
Response: 4927563
Conc: 1.98 ng/ml

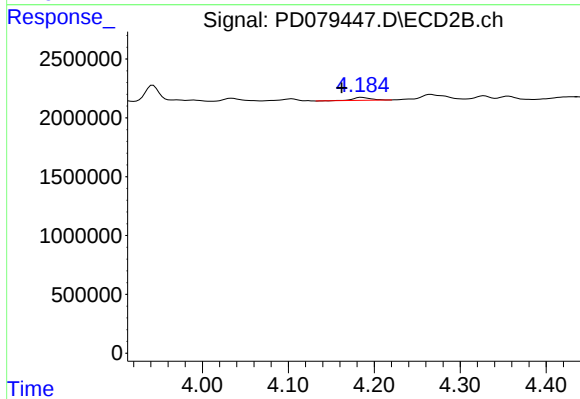


#7 delta-BHC

R.T.: 4.185 min
Delta R.T.: 0.023 min
Response: 326924
Conc: N.D.

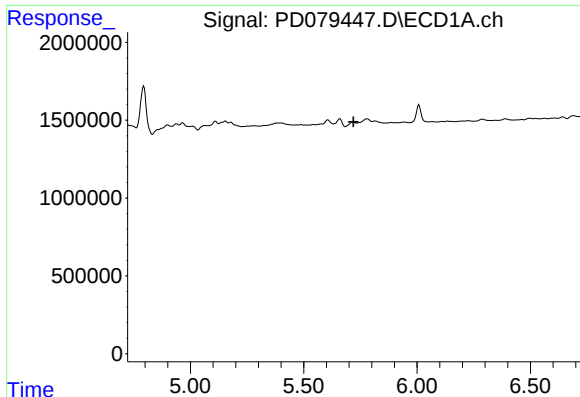


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.720 min
Response: 0
Conc: N.D.

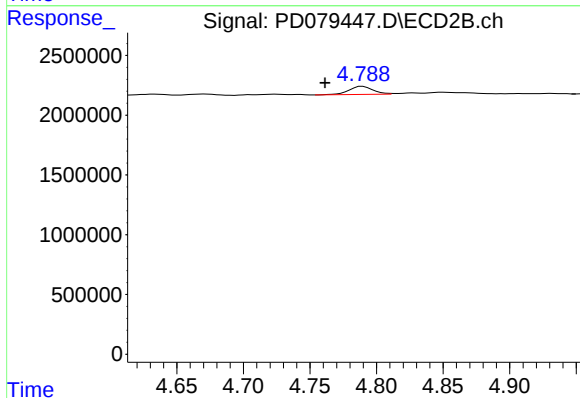


#8 Heptachlor epoxide

R.T.: 4.790 min
Delta R.T.: 0.028 min
Response: 866975
Conc: 0.28 ng/ml

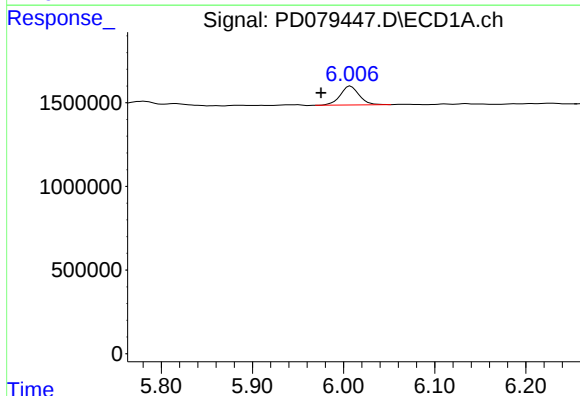


#10 trans-Chlordane

R.T.: 6.008 min
Delta R.T.: 0.032 min
Response: 1625307
Conc: 0.76 ng/ml

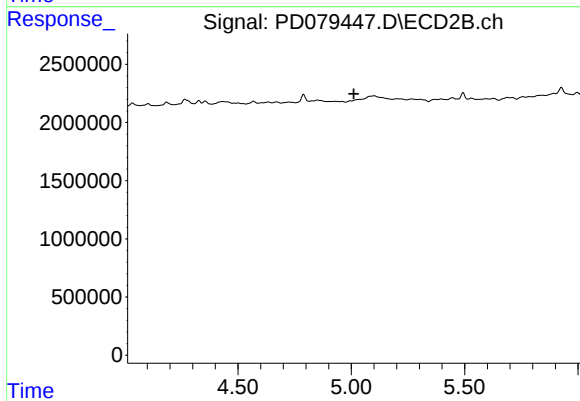


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.011 min
Response: 0
Conc: N.D.

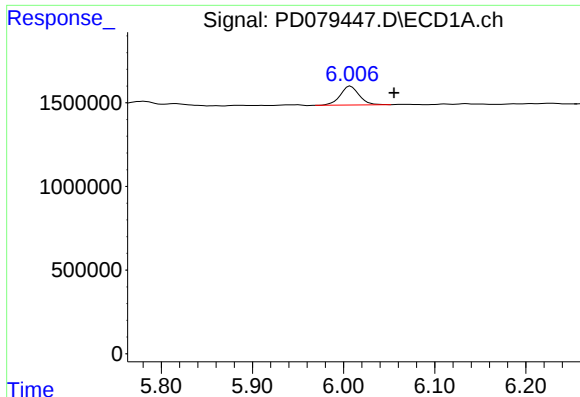


#11 cis-Chlordane

R.T.: 6.008 min
Delta R.T.: -0.048 min
Response: 1625307
Conc: 0.75 ng/ml

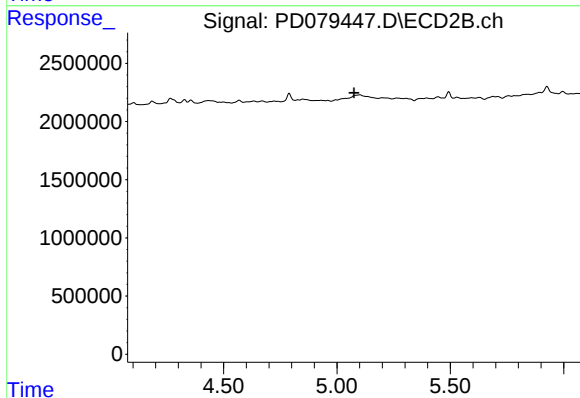


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.076 min
Response: 0
Conc: N.D.

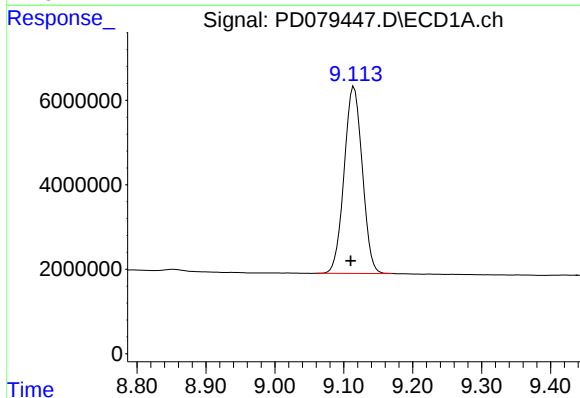

#27 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.004 min
Response: 80958375
Conc: 45.62 ng/ml

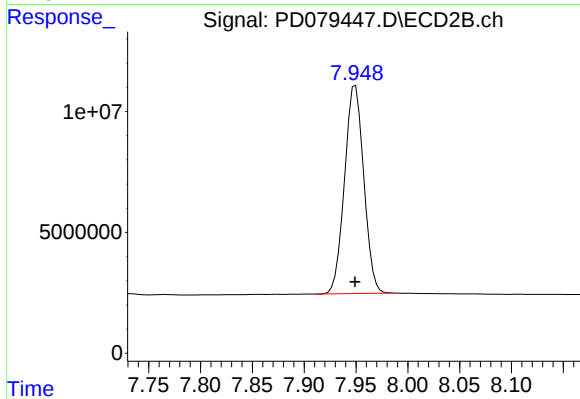

#27 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 111138867
Conc: 46.55 ng/ml