

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
 Data File : PD079479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2023 18:03
 Operator : AR\AJ
 Sample : PIBLK068
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 05:12:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.803	34246481	55780359	23.450	24.387
27)	SA Decachlor...	9.113	7.949	64191759	83890078	36.174	35.138
Target Compounds							
2)	A alpha-BHC	0.000	3.293	0	114234	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.658	0	464861	N.D.	0.135
4)	MA Heptachlor	0.000	3.994	0	146818	N.D.	<MDL
5)	MB Aldrin	0.000	4.267	0	619521	N.D.	0.190
6)	B beta-BHC	0.000	3.943	0	1059411	N.D.	0.647
7)	B delta-BHC	4.791	4.186	4392983	116730	1.763	<MDL #
8)	B Heptachlo...	0.000	4.790	0	787491	N.D.	0.255
10)	B trans-Chl...	6.007	0.000	1660964	0	0.781	N.D. #
11)	B cis-Chlor...	6.007f	0.000	1660964	0	0.763	N.D. #
12)	B 4,4'-DDE	0.000	5.219f	0	120886	N.D.	<MDL
13)	MA Dieldrin	6.382	5.394	1941907	191546	0.883	<MDL #
15)	B Endosulfa...	0.000	5.994	0	174445	N.D.	<MDL
19)	B Endosulfa...	7.234f	6.361	-260470	1709086	N.D.	0.688
20)	A Methoxychlor	7.469f	0.000	267336	0	0.290	N.D. #
23)	Toxaphene-2	0.000	5.373	0	476059	N.D.	28.329


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
Data File : PD079479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2023 18:03
Operator : AR\AJ
Sample : PIBLK068
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 05:12:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

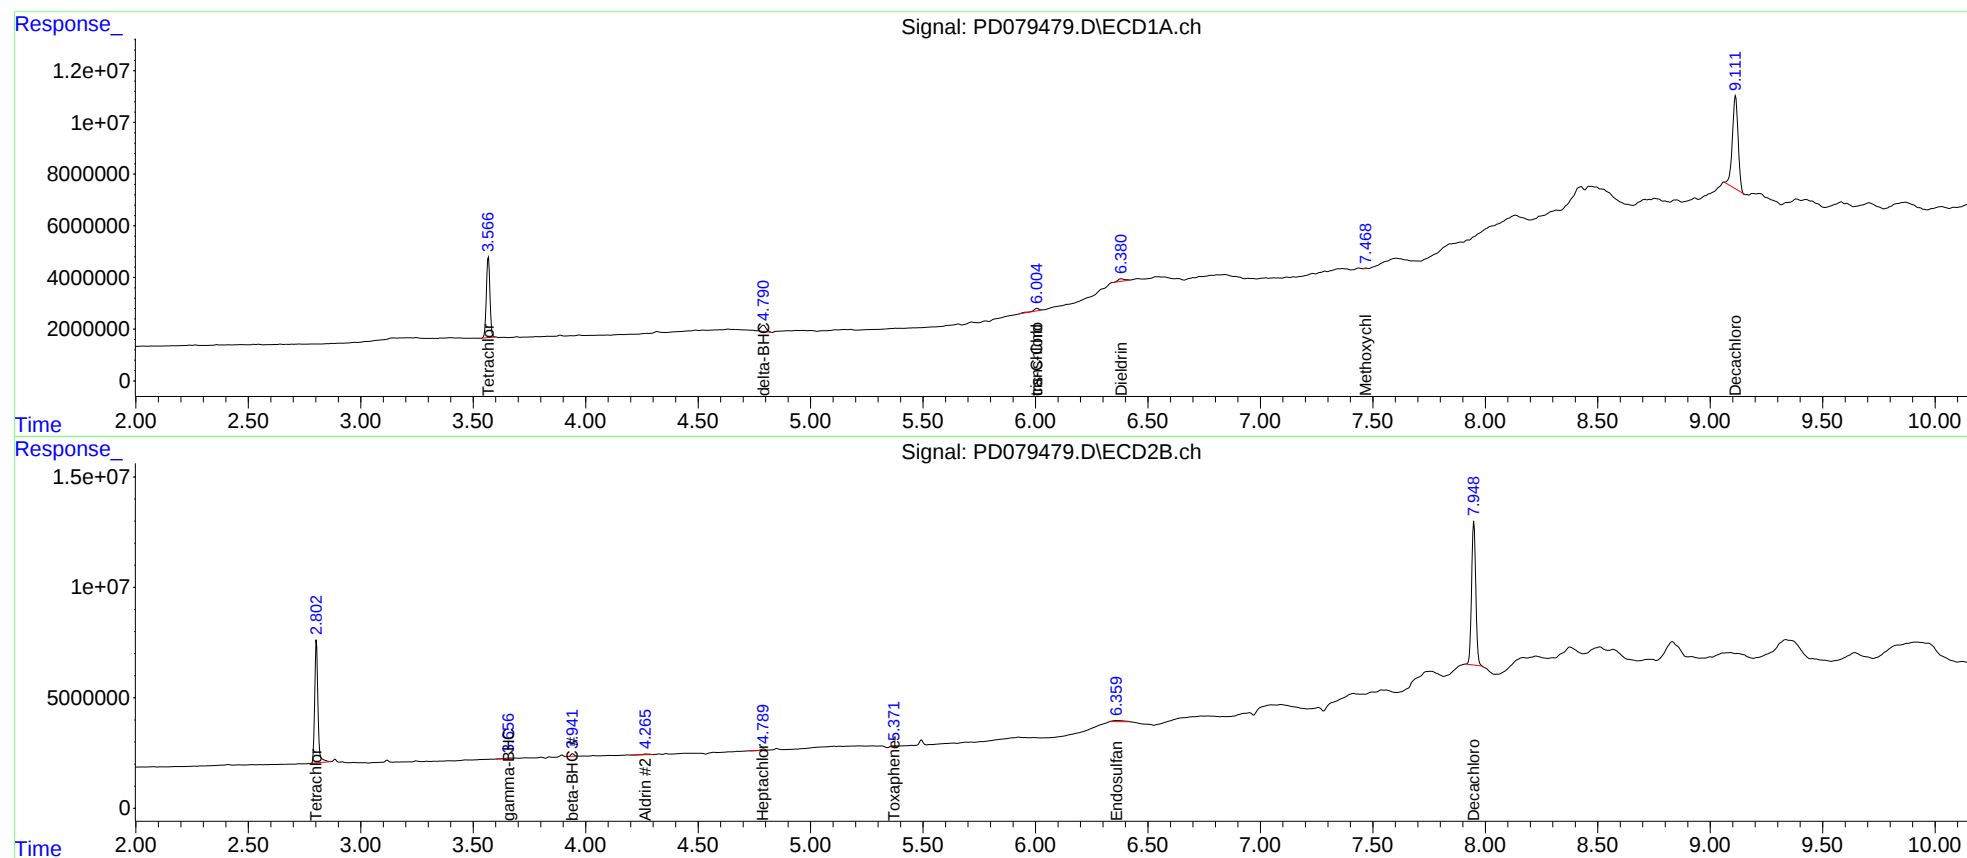

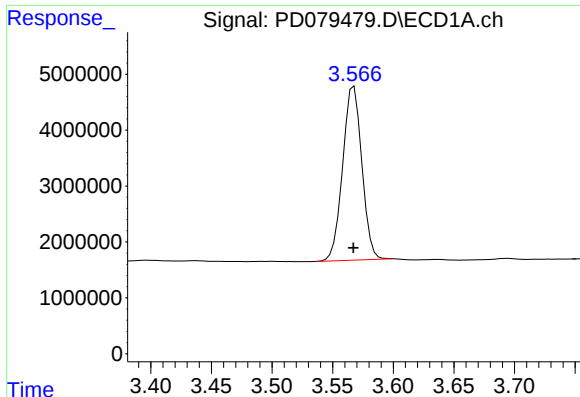


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: 0.000 min
Response: 34246481
Conc: 23.45 ng/ml

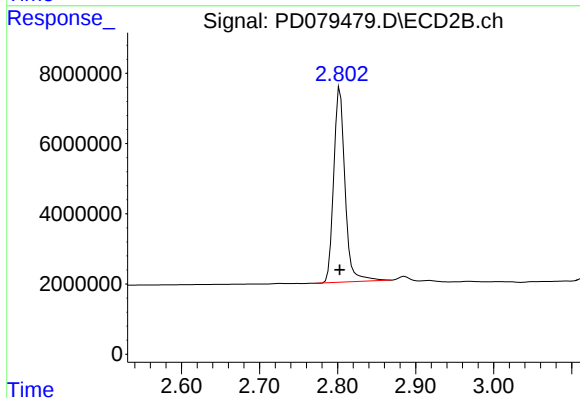


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 55780359
Conc: 24.39 ng/ml

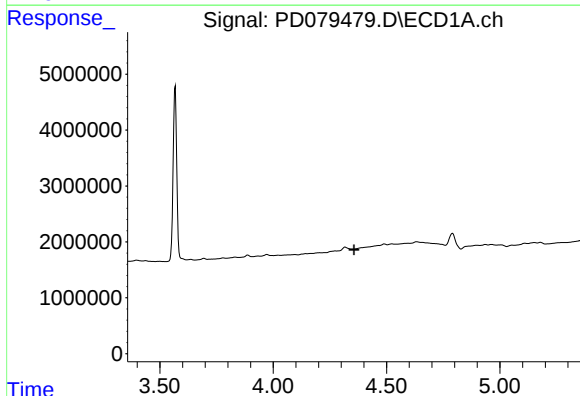


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

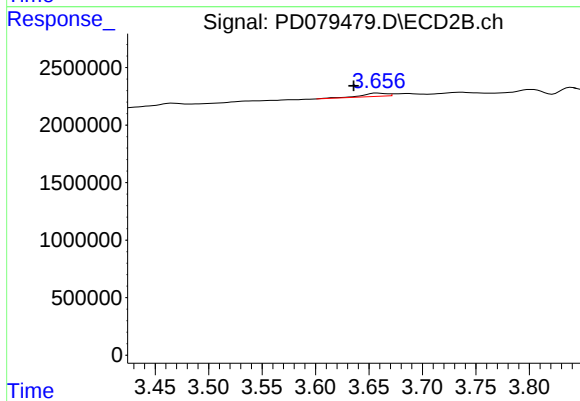


#3 gamma-BHC (Lindane)

R.T.: 3.658 min
Delta R.T.: 0.022 min
Response: 464861
Conc: 0.14 ng/ml

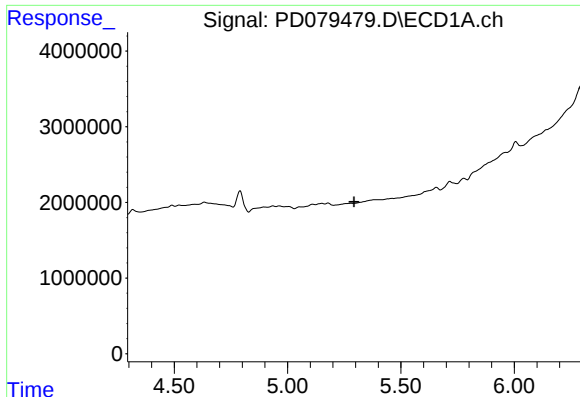


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

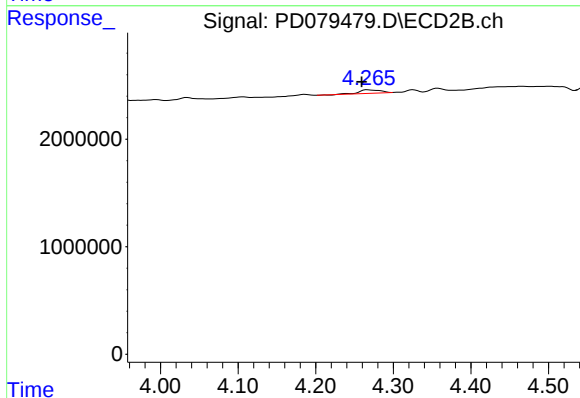


#5 Aldrin

R.T.: 4.267 min
Delta R.T.: 0.007 min
Response: 619521
Conc: 0.19 ng/ml

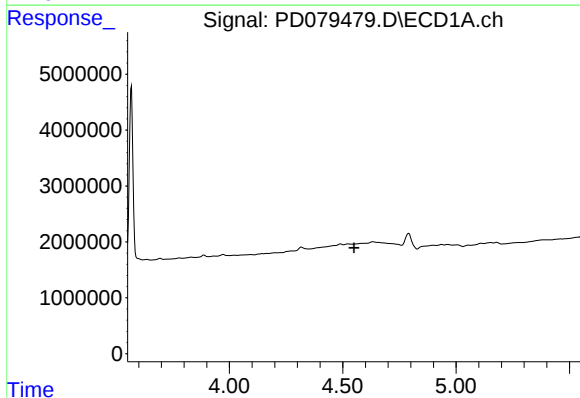


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

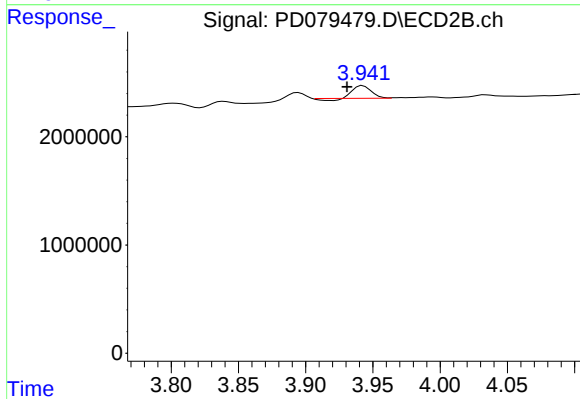


#6 beta-BHC

R.T.: 3.943 min
Delta R.T.: 0.012 min
Response: 1059411
Conc: 0.65 ng/ml

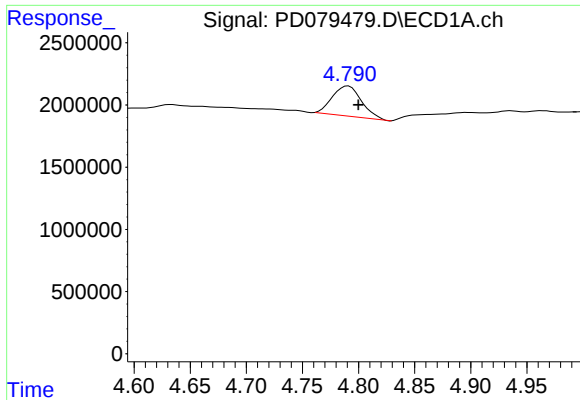


#7 delta-BHC

R.T.: 4.791 min
Delta R.T.: -0.009 min
Response: 4392983
Conc: 1.76 ng/ml

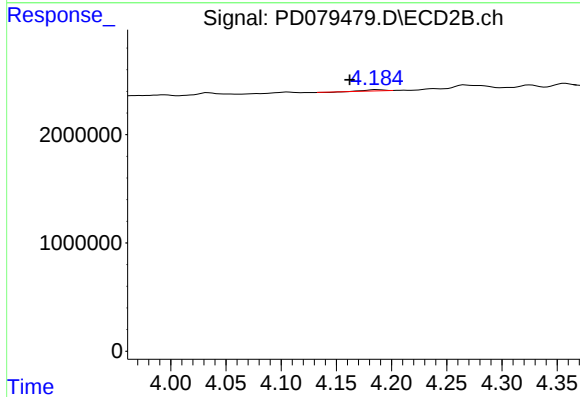


#7 delta-BHC

R.T.: 4.186 min
Delta R.T.: 0.024 min
Response: 116730
Conc: N.D.

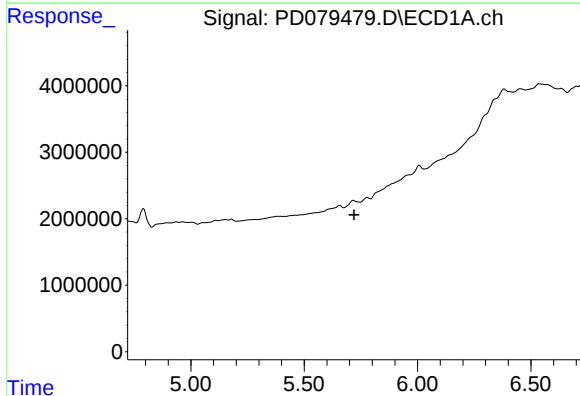


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.720 min
Response: 0
Conc: N.D.

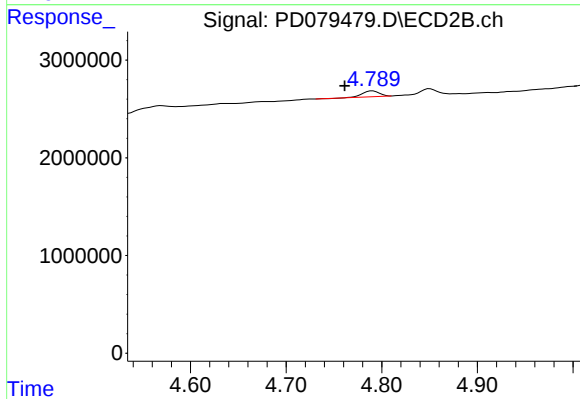


#8 Heptachlor epoxide

R.T.: 4.790 min
Delta R.T.: 0.029 min
Response: 787491
Conc: 0.25 ng/ml

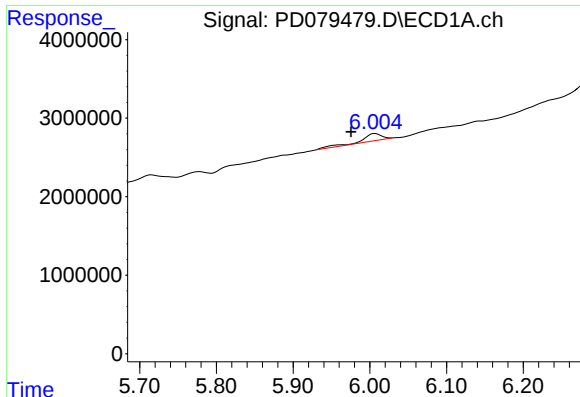


#10 trans-Chlordane

R.T.: 6.007 min
Delta R.T.: 0.031 min
Response: 1660964
Conc: 0.78 ng/ml

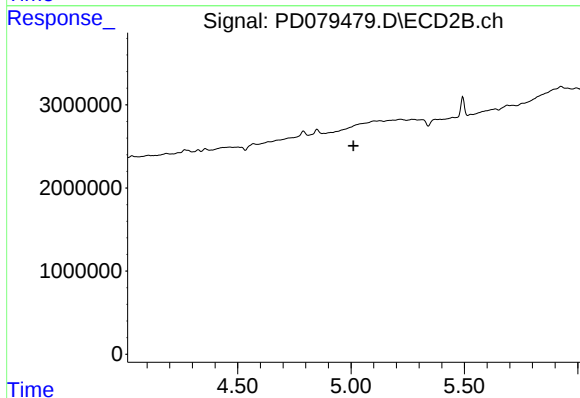


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.011 min
Response: 0
Conc: N.D.

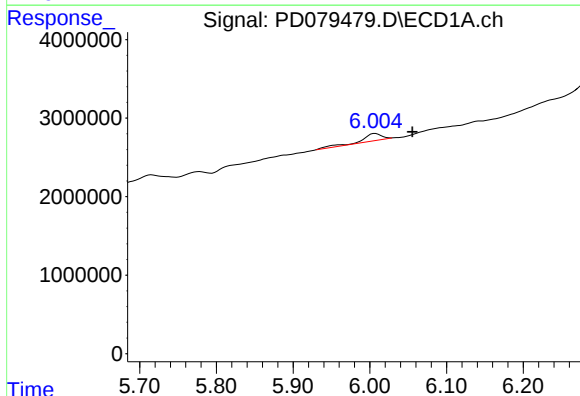


#11 cis-Chlordane

R.T.: 6.007 min
Delta R.T.: -0.049 min
Response: 1660964
Conc: 0.76 ng/ml

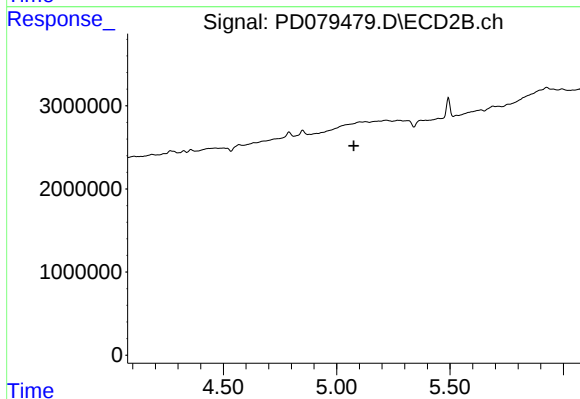


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.076 min
Response: 0
Conc: N.D.

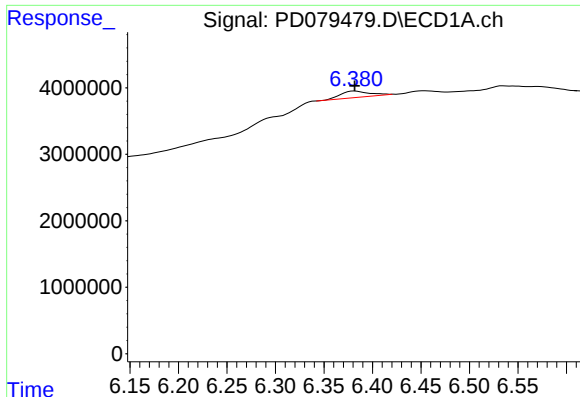


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 1941907
Conc: 0.88 ng/ml

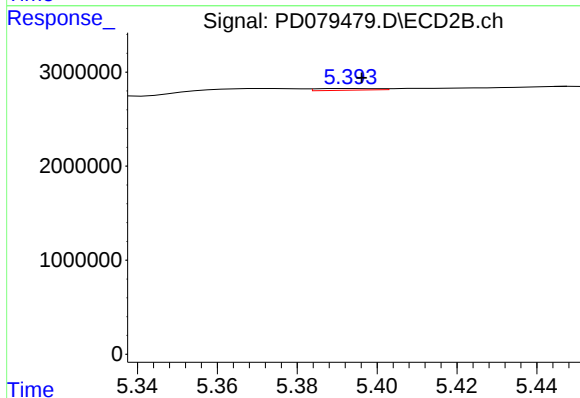


#13 Dieldrin

R.T.: 5.394 min
Delta R.T.: -0.002 min
Response: 191546
Conc: N.D.

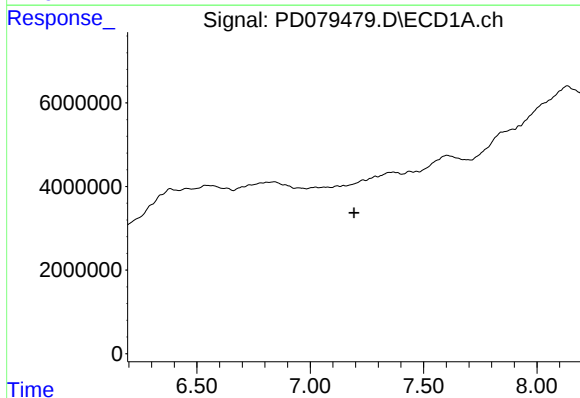


#19 Endosulfan Sulfate

R.T.: 7.234 min
Delta R.T.: 0.040 min
Response: -260470
Conc: N.D.

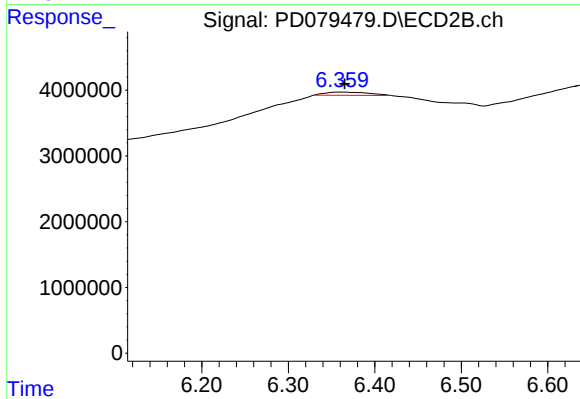


#19 Endosulfan Sulfate

R.T.: 6.361 min
Delta R.T.: -0.005 min
Response: 1709086
Conc: 0.69 ng/ml

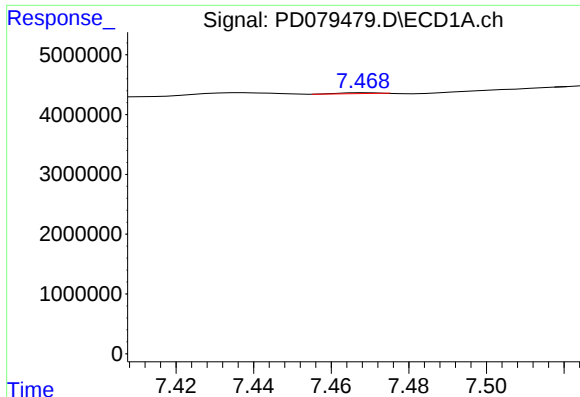


#20 Methoxychlor

R.T.: 7.469 min
Delta R.T.: -0.062 min
Response: 267336
Conc: 0.29 ng/ml

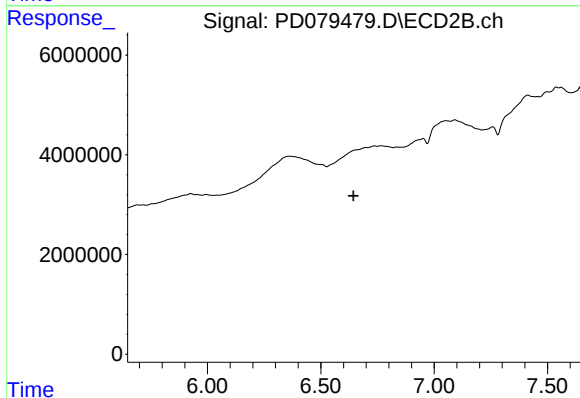


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.645 min
Response: 0
Conc: N.D.

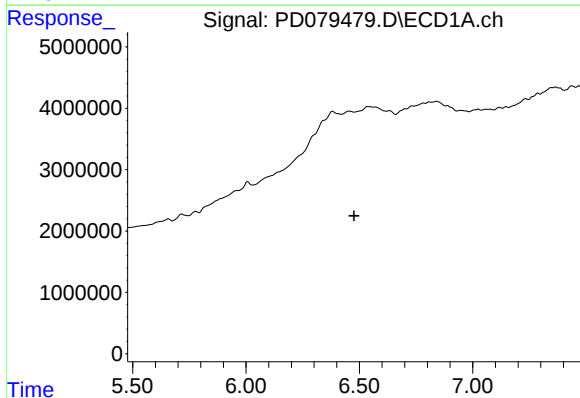


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.477 min
Response: 0
Conc: N.D.

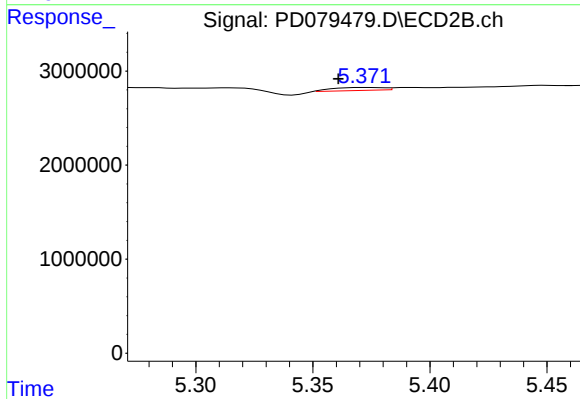


#23 Toxaphene-2

R.T.: 5.373 min
Delta R.T.: 0.012 min
Response: 476059
Conc: 28.33 ng/ml

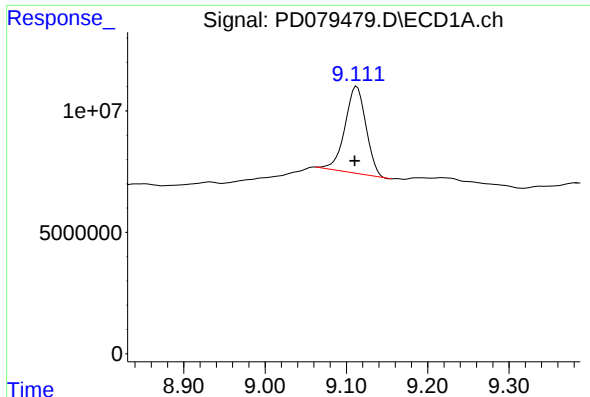

#27 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.003 min
Response: 64191759
Conc: 36.17 ng/ml

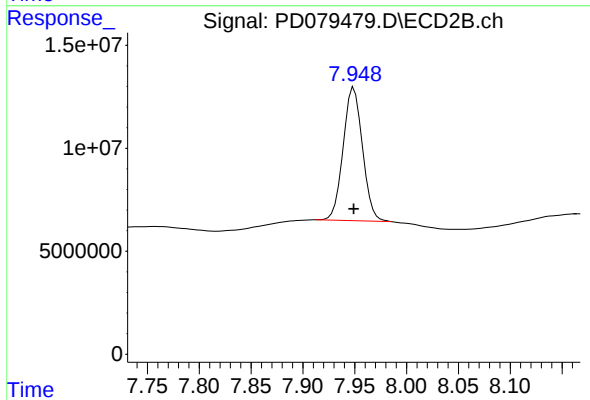

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 83890078
Conc: 35.14 ng/ml