

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
 Data File : PD079469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2023 15:49
 Operator : AR\AJ
 Sample : PB156866BS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS866

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/06/2023
 Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 05:09:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.803	28721988	43629480	19.668	19.075
27)	SA Decachlor...	9.114	7.949	48713812	70701342	27.451	29.613
Target Compounds							
2)	A alpha-BHC	4.024	3.306	12351559	17835720	4.985	4.919
3)	MA gamma-BHC...	4.358	3.636	11245199	17265341	4.760	5.026
4)	MA Heptachlor	4.951	3.979	13811440	17710810	5.514	5.309
5)	MB Aldrin	5.294	4.259	12415033	18341298	5.294	5.637
6)	B beta-BHC	4.551	3.930	6068350	8828853	5.589	5.391m
7)	B delta-BHC	4.799	4.162	9957879	10058029	3.996	2.815 #
8)	B Heptachlo...	5.721	4.761	11650045	17444303	5.255	5.640
9)	A Endosulfan I	6.105	5.132	9402635	15392452	4.548m	5.552
10)	B trans-Chl...	5.975	5.012	9727706	16638173	4.572m	5.605
11)	B cis-Chlor...	6.055	5.076	9989364	16575995	4.587m	5.461
12)	B 4,4'-DDE	6.226	5.265	19601068	30405089	9.928	10.858
13)	MA Dieldrin	6.382	5.396	22963881	33697387	10.439	10.583
14)	MA Endrin	6.613	5.671	18801882	29905765	10.305	10.919
15)	B Endosulfa...	6.831	5.963	21981320	27692916	11.554	10.663
16)	A 4,4'-DDD	6.743	5.818	17484715	25353362	10.793	10.770
17)	MA 4,4'-DDT	7.059	6.070	16933340	24260957	9.939	10.100
18)	B Endrin al...	6.960	6.143	15589309	21826129	10.459	10.786
19)	B Endosulfa...	7.195	6.365	17531091	24544877	9.415	9.878
20)	A Methoxychlor	7.533	6.645	47199864	72154248	51.201	56.135
21)	B Endrin ke...	7.682	6.872	19267106	30606527	9.861	10.766

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
Data File : PD079469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2023 15:49
Operator : AR\AJ
Sample : PB156866BS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 05:09:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

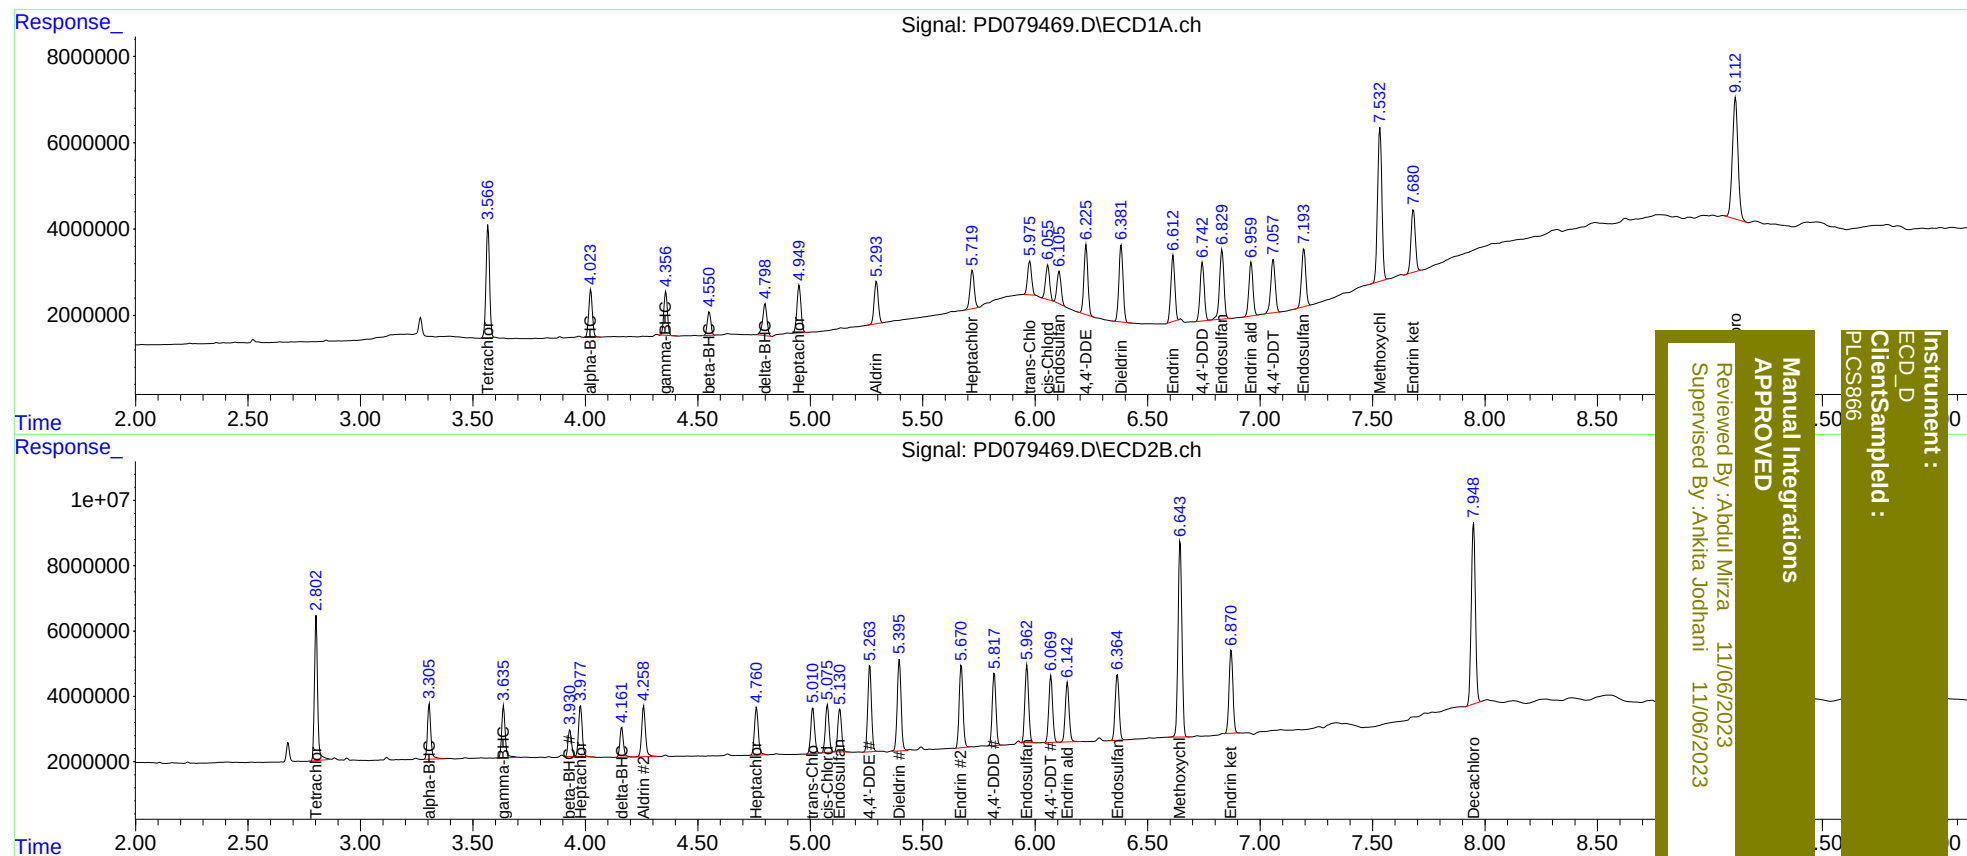

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/06/2023
Supervised By: Ankita Jodhani 11/06/2023

Instrument :
ECD_D
ClientSampled :
PLCS866