

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
 Data File : PD079475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2023 17:09
 Operator : AR\AJ
 Sample : 05174-20MS
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COAN6MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/06/2023
 Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 05:11:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.803	20326338	33393213	13.919	14.599
27)	SA Decachlor...	9.109	7.949	44025479	58402757	24.809	24.462
Target Compounds							
2)	A alpha-BHC	4.023	3.306	110.5E6	163.3E6	44.590m	45.047
3)	MA gamma-BHC...	4.356	3.636	100.4E6	159.1E6	42.507m	46.308
4)	MA Heptachlor	4.951	3.978	102.7E6	148.5E6	41.013	44.520
5)	MB Aldrin	5.294	4.259	95018430	140.4E6	40.520	43.141
6)	B beta-BHC	4.552	3.931	35456569	63440490	32.655	38.738
7)	B delta-BHC	4.801	4.162	101.4E6	153.6E6	40.679	42.980
8)	B Heptachlo...	5.721	4.761	83720437	129.6E6	37.764	41.884
9)	A Endosulfan I	6.107	5.132	81721195	96756851	39.532	34.902m
10)	B trans-Chl...	5.975	5.012	79218292	125.8E6	37.232m	42.387
11)	B cis-Chlor...	6.056	5.076	91553758	122.4E6	42.036	40.321
12)	B 4,4'-DDE	6.226	5.265	128.6E6	245.2E6	65.121	87.561 #
13)	MA Dieldrin	6.383	5.396	171.2E6	268.7E6	77.810	84.376
14)	MA Endrin	6.613	5.671	138.8E6	230.6E6	76.057	84.189
15)	B Endosulfa...	6.831	5.964	140.1E6	204.9E6	73.656	78.906
16)	A 4,4'-DDD	6.744	5.819	132.2E6	189.8E6	81.599	80.637
17)	MA 4,4'-DDT	7.059	6.070	136.3E6	182.1E6	80.002	75.826
18)	B Endrin al...	6.960	6.142	91383714	120.2E6	61.310	59.418m
19)	B Endosulfa...	7.195	6.365	139.6E6	182.8E6	74.946	73.577
20)	A Methoxychlor	7.532	6.645	367.9E6	494.7E6	399.128	384.863
21)	B Endrin ke...	7.682	6.871	152.0E6	185.8E6	77.815	65.354

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
Data File : PD079475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2023 17:09
Operator : AR\AJ
Sample : 05174-20MS
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 05:11:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

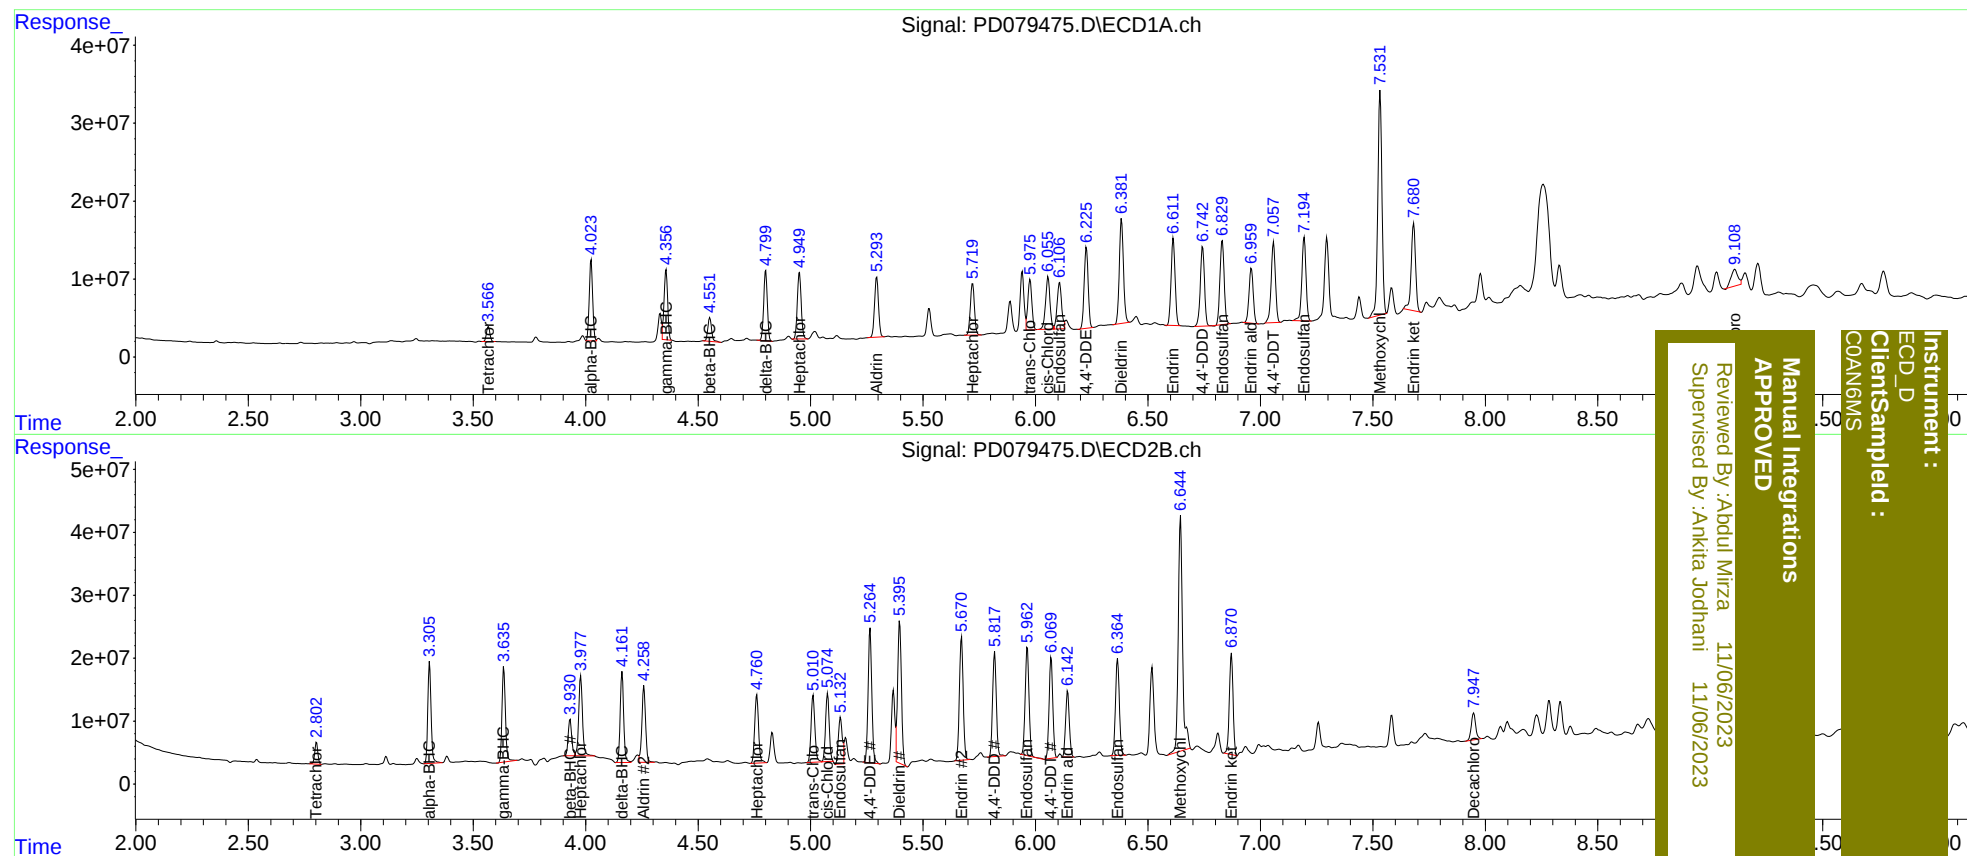

Instrument :
ECD_D
ClientSampled :
COAN6MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/06/2023
Supervised By: Ankita Jodhani 11/06/2023