

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
 Data File : PD079454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2023 12:28
 Operator : AR\AJ
 Sample : 04922-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAQ9

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/06/2023
 Supervised By :Ankita Jodhani 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 05:04:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.576	2.818	14323874	25077678	9.808m	10.964m
27) SA Decachlor...	9.115	7.963	12147078	87721132	6.845m	36.742 #
Target Compounds						
8) B Heptachlo...	5.725	4.769	59978183	323.5E6	27.055m	104.592m#
13) MA Dieldrin	6.367	5.409	288.3E6	192.9E6	131.037	60.588 #
15) B Endosulfa...	6.817	5.976	651.1E6	322.5E6	342.233	124.182m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110723\
Data File : PD079454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2023 12:28
Operator : AR\AJ
Sample : 04922-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 05:04:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

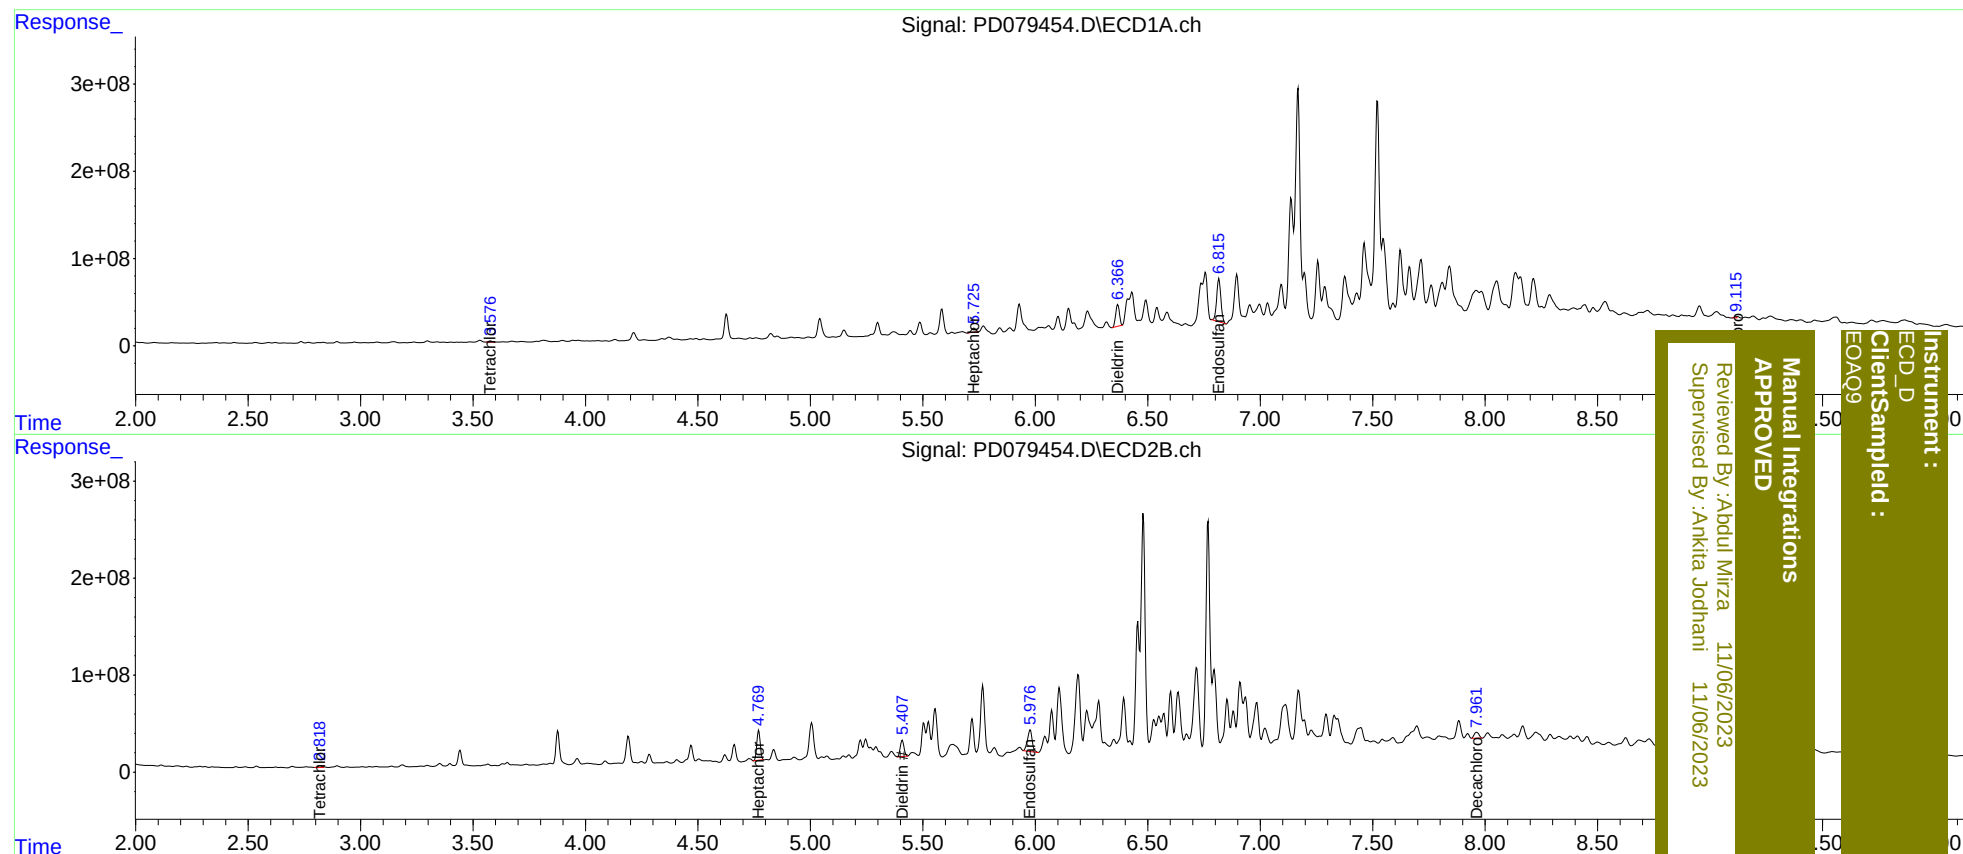

Instrument :
ECD_D
ClientSampled :
EOAQ9

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/06/2023
Supervised By : Ankita Jodhani 11/06/2023