

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110724\
 Data File : PD086417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 12:25
 Operator : AR\AJ
 Sample : PEST/SPIK/EPA 50/100PPB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEST/SPIK/EPA 50/100PPB

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/08/2024
 Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 00:54:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
2) A	alpha-BHC	4.015	3.401	136.3E6	740.9E6	54.734
3) MA	gamma-BHC...	4.347	3.738	134.4E6	686.7E6	54.001
4) MA	Heptachlor	4.948	4.094	130.4E6	637.1E6	52.747
5) MB	Aldrin	5.291	4.381	126.5E6	667.9E6	52.198
6) B	beta-BHC	4.530	4.033	51004984	281.1E6	45.927
7) B	delta-BHC	4.780	4.270	139.2E6	694.8E6	53.766
8) B	Heptachlo...	5.711	4.884	116.2E6	601.2E6	50.852
9) A	Endosulfan I	6.095	5.261	107.5E6	563.4E6	53.070
10) B	trans-Chl...	5.966	5.140	112.0E6	634.8E6	50.776
11) B	cis-Chlor...	6.048	5.204	117.0E6	617.7E6	52.900
12) B	4,4'-DDE	6.216	5.391	222.5E6	1137.9E6	104.169
13) MA	Dieldrin	6.368	5.526	248.4E6	1194.4E6	108.898
14) MA	Endrin	6.594	5.803	207.5E6	969.8E6	110.381m
15) B	Endosulfa...	6.805	6.094	205.9E6	1026.7E6	102.725m
16) A	4,4'-DDD	6.724	5.945	181.9E6	972.2E6	112.262m
17) MA	4,4'-DDT	7.041	6.199	177.8E6	865.7E6	106.669m
18) B	Endrin al...	6.935	6.273	153.7E6	778.9E6	103.006
19) B	Endosulfa...	7.170	6.498	180.1E6	1047.7E6	97.682
20) A	Methoxychlor	7.515	6.773	464.2E6	1888.9E6	493.225
21) B	Endrin ke...	7.651	7.007	222.9E6	1078.0E6	108.182

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110724\
Data File : PD086417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 12:25
Operator : AR\AJ
Sample : PEST/SPIK/EPA 50/100PPB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 00:54:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

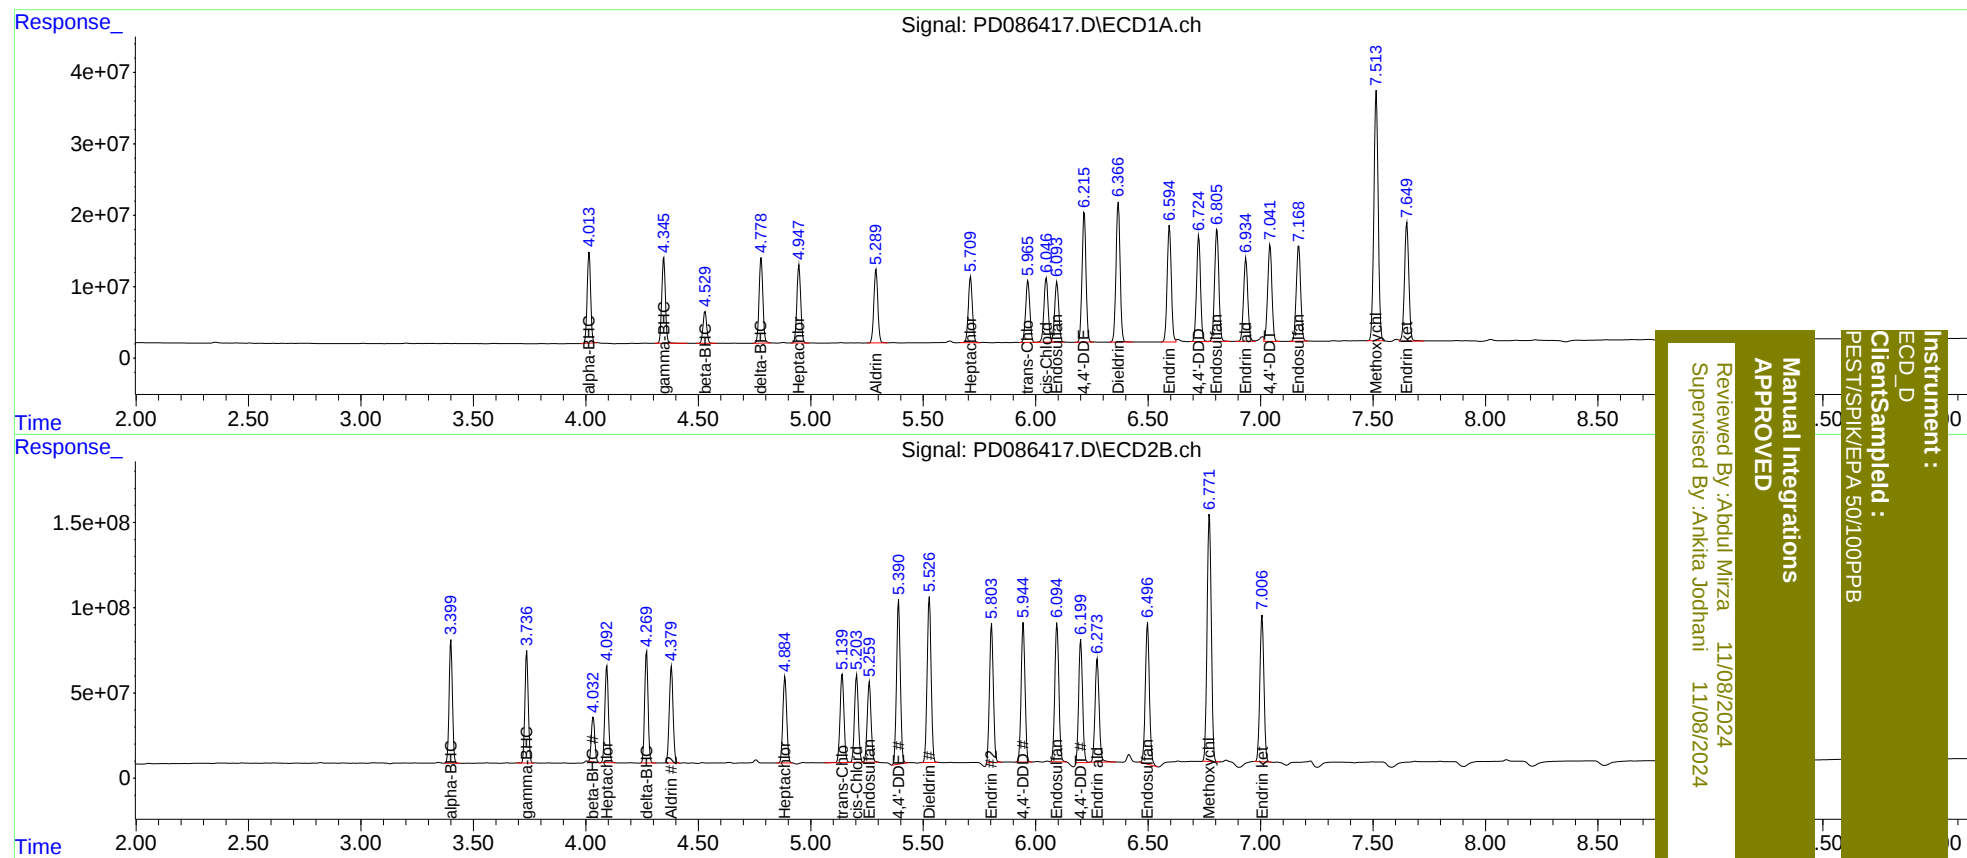

Reviewed By: Abdul Mirza 11/08/2024
Supervised By: Ankita Jodhani 11/08/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
PEST/SPIK/EPA 50/100PPB