

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110724\
 Data File : PD086439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 19:34
 Operator : AR\AJ
 Sample : P4621-11MS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6N6MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/08/2024
 Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:00:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.888	24802203	191.6E6	18.838	20.657
27)	SA Decachlor...	9.096	8.093	36963874	214.2E6	20.618	22.649
Target Compounds							
2)	A alpha-BHC	4.009	3.402	149.8E6	794.7E6	60.160	55.309
3)	MA gamma-BHC...	4.341	3.738	146.5E6	739.4E6	58.863	54.821
4)	MA Heptachlor	4.942	4.093	128.7E6	674.4E6	52.075	49.360m
5)	MB Aldrin	5.284	4.380	124.2E6	655.4E6	51.243	48.306m
6)	B beta-BHC	4.524	4.033	55119226	302.0E6	49.632	48.170
7)	B delta-BHC	4.773	4.271	151.7E6	747.2E6	58.596	53.254
8)	B Heptachlo...	5.704	4.885	124.9E6	654.8E6	54.673	52.217m
9)	A Endosulfan I	6.088	5.261	117.6E6	607.5E6	58.052	52.913
10)	B trans-Chl...	5.959	5.140	121.5E6	673.4E6	55.067	51.193
11)	B cis-Chlor...	6.041	5.205	124.1E6	660.1E6	56.141	51.972
12)	B 4,4'-DDE	6.209	5.391	244.3E6	1259.4E6	114.389	102.710
13)	MA Dieldrin	6.361	5.526	271.4E6	1298.6E6	119.006	105.259m
14)	MA Endrin	6.588	5.804	214.7E6	1138.3E6	114.226	101.287
15)	B Endosulfa...	6.799	6.096	224.1E6	1120.9E6	111.773	101.601
16)	A 4,4'-DDD	6.719	5.946	196.6E6	1067.7E6	121.328	108.766
17)	MA 4,4'-DDT	7.034	6.201	194.2E6	1068.6E6	116.483m	104.138
18)	B Endrin al...	6.929	6.274	166.9E6	843.2E6	111.862	101.584
19)	B Endosulfa...	7.163	6.498	211.3E6	1093.3E6	114.654	103.711
20)	A Methoxychlor	7.508	6.772	507.9E6	2236.6E6	539.635	470.531
21)	B Endrin ke...	7.644	7.007	237.8E6	1199.9E6	115.378	104.863

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110724\
Data File : PD086439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 19:34
Operator : AR\AJ
Sample : P4621-11MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:00:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

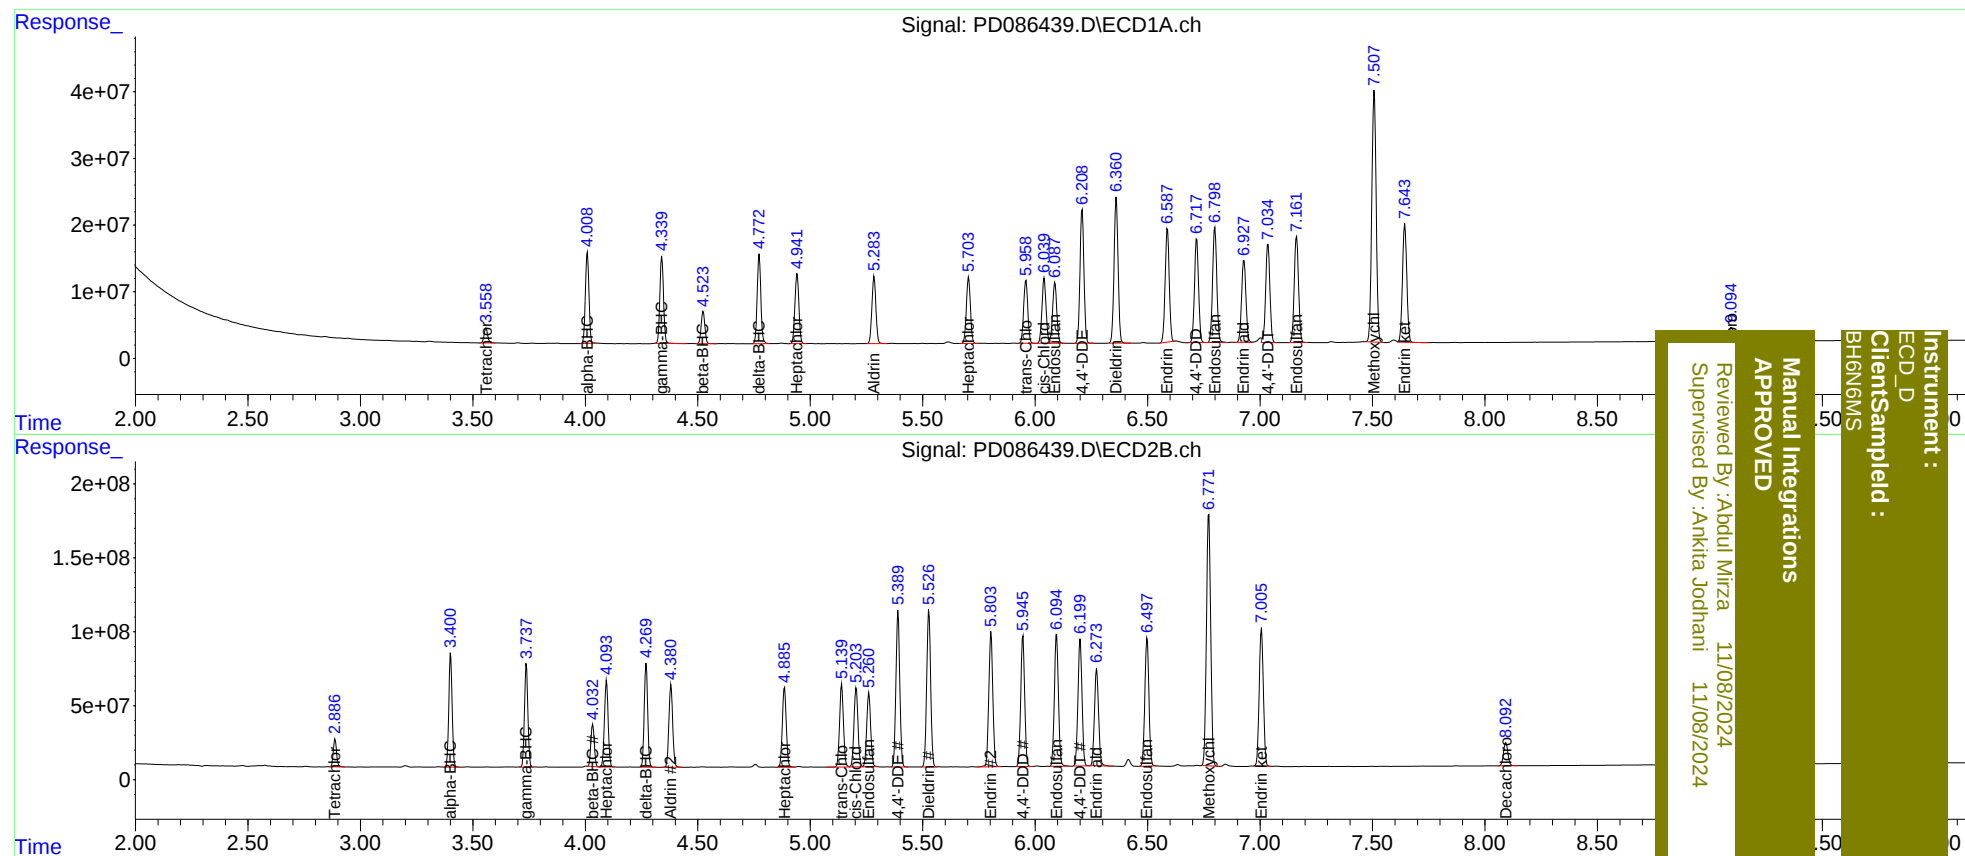

Instrument :
ECD_D
ClientSampled :
BH6N6MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 11/08/2024
Supervised By: Ankita Jodhani 11/08/2024