

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110724\
 Data File : PD086440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 19:48
 Operator : AR\AJ
 Sample : P4621-12MSD
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6N6MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/08/2024
 Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:01:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.887	24565557	190.0E6	18.659	20.485
27)	SA Decachlor...	9.095	8.093	36397282	212.9E6	20.302	22.511
Target Compounds							
2)	A alpha-BHC	4.009	3.401	146.2E6	777.8E6	58.743	54.137
3)	MA gamma-BHC...	4.340	3.738	144.4E6	724.4E6	58.034m	53.708
4)	MA Heptachlor	4.942	4.093	126.7E6	669.6E6	51.234	49.012m
5)	MB Aldrin	5.284	4.380	122.0E6	646.5E6	50.356	47.653m
6)	B beta-BHC	4.525	4.033	53903208	295.8E6	48.537	47.183
7)	B delta-BHC	4.773	4.270	148.7E6	732.4E6	57.445	52.195
8)	B Heptachlo...	5.704	4.884	122.0E6	641.5E6	53.381	51.161m
9)	A Endosulfan I	6.088	5.261	114.9E6	601.0E6	56.737	52.343
10)	B trans-Chl...	5.959	5.140	118.8E6	662.4E6	53.819	50.354
11)	B cis-Chlor...	6.040	5.204	121.5E6	650.0E6	54.953	51.176
12)	B 4,4'-DDE	6.209	5.391	238.2E6	1237.6E6	111.510	100.938
13)	MA Dieldrin	6.361	5.526	265.1E6	1275.1E6	116.218	103.350m
14)	MA Endrin	6.588	5.803	210.9E6	1123.2E6	112.185	99.946
15)	B Endosulfa...	6.799	6.095	219.7E6	1101.3E6	109.596	99.816
16)	A 4,4'-DDD	6.718	5.945	192.2E6	1049.3E6	118.587	106.893
17)	MA 4,4'-DDT	7.033	6.198	190.5E6	1062.1E6	114.275m	103.501m
18)	B Endrin al...	6.928	6.273	164.1E6	830.6E6	109.974	100.060
19)	B Endosulfa...	7.162	6.497	207.4E6	1079.6E6	112.508	102.414
20)	A Methoxychlor	7.507	6.772	499.6E6	2209.3E6	530.830	464.785
21)	B Endrin ke...	7.644	7.006	232.7E6	1181.3E6	112.931	103.235

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110724\
Data File : PD086440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 19:48
Operator : AR\AJ
Sample : P4621-12MSD
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:01:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

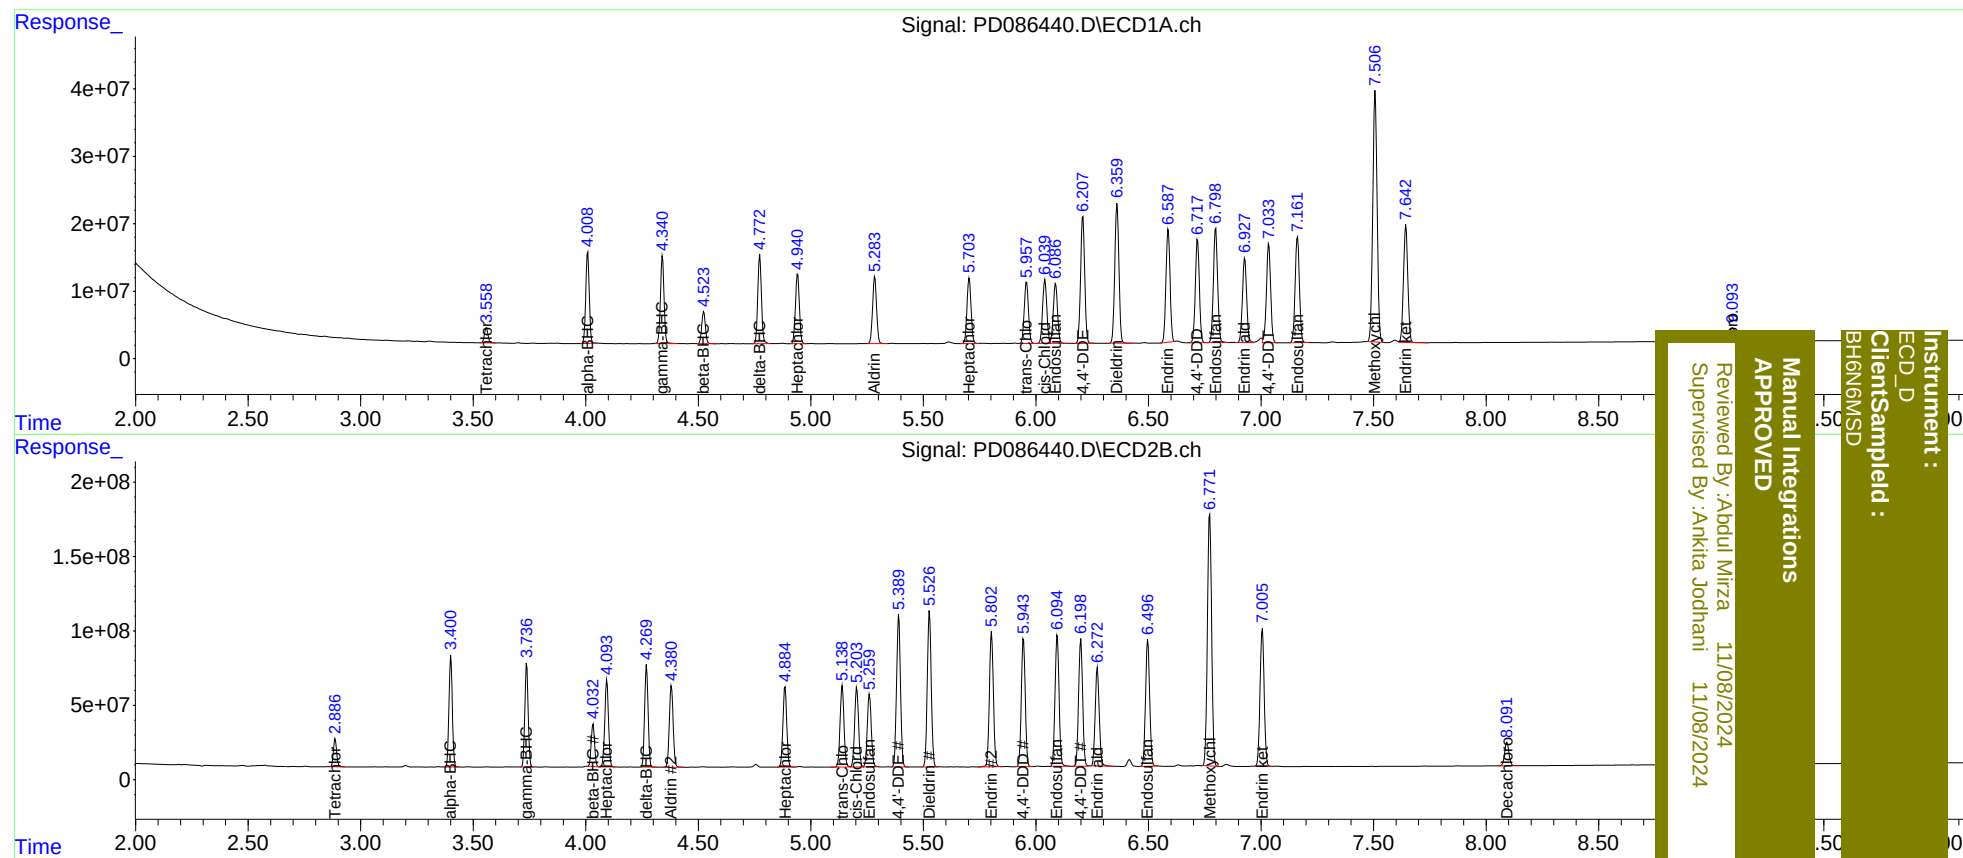

Instrument :
ECD_D
ClientSampled :
BH6N6MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/08/2024
Supervised By: Ankita Jodhani 11/08/2024