Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110725\
Data File : PD091022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2025 11:20
Operator : AR\AJ
Sample : Q3541-01RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
N48969RE

Manual Integrations APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 02:44:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	3.543	2.874	39847213	434.2E6	12.795m	14.582
28)	SA Decachlor...	9.063	8.057	30532676	192.0E6	6.527m	6.337m
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110725\
Data File : PD091022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2025 11:20
Operator : AR\AJ
Sample : Q3541-01RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
N48969RE

Manual Integrations APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 02:44:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

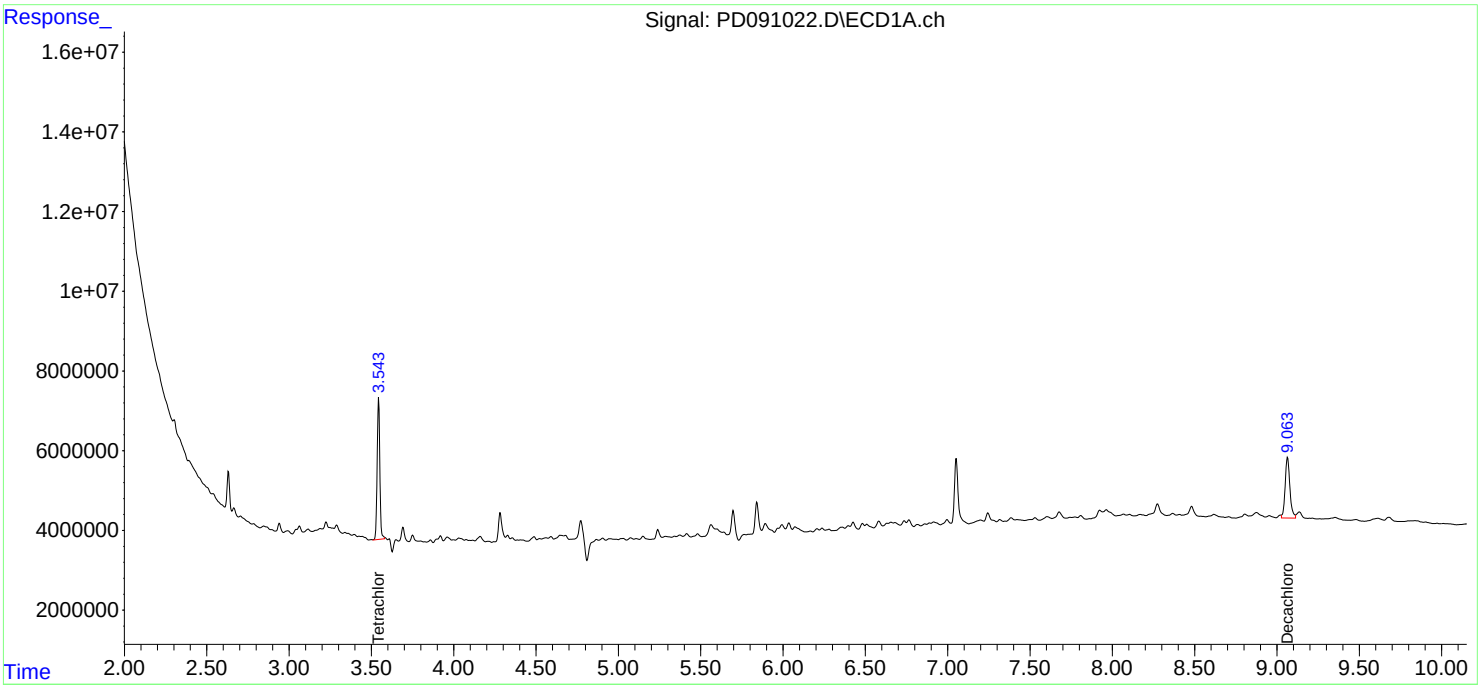

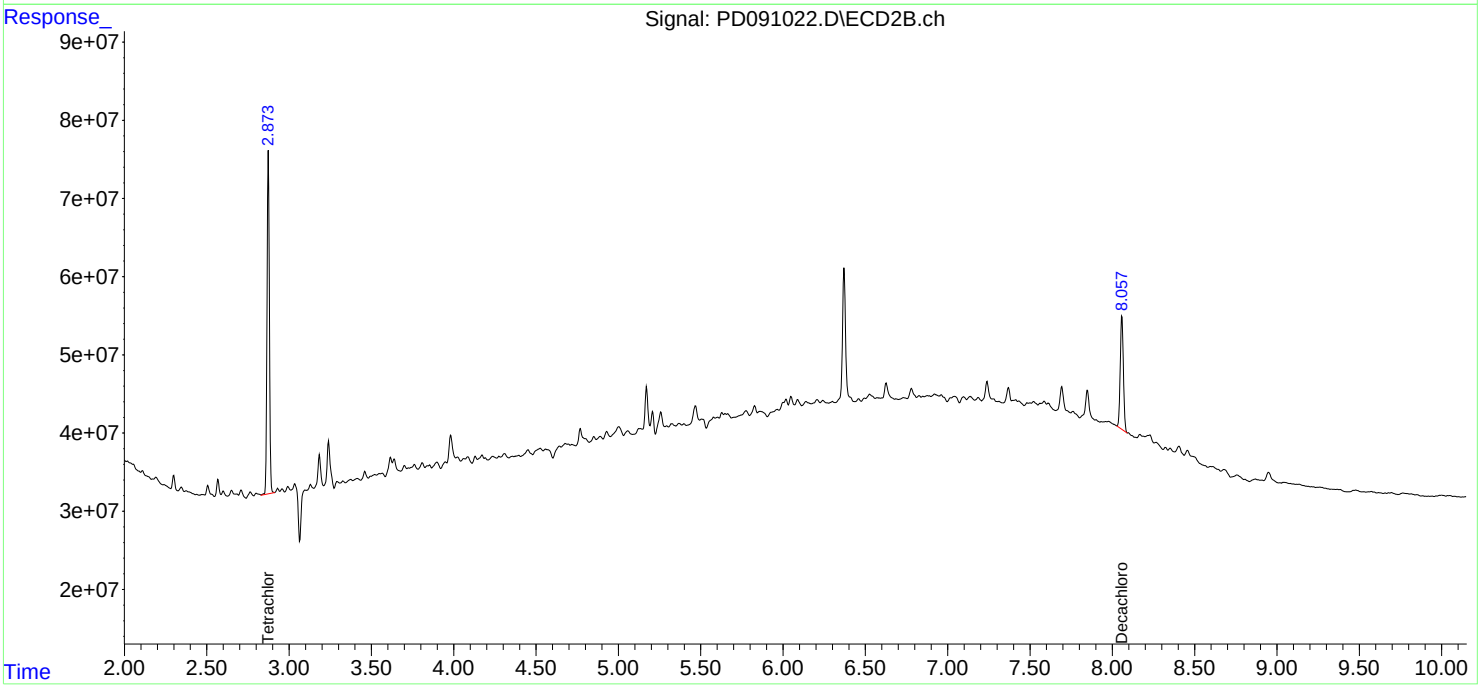

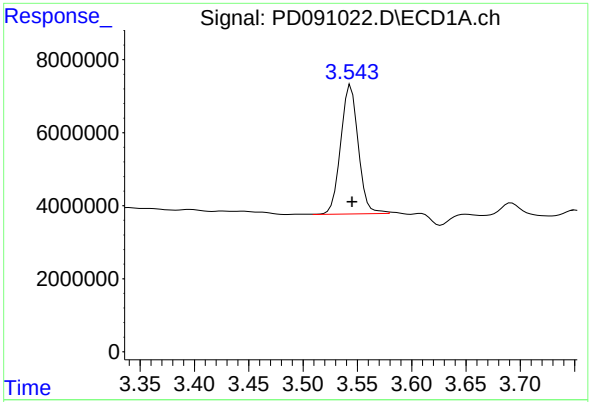

#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.002 min
Response: 39847213
Conc: 12.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
N48969RE

Manual Integrations APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

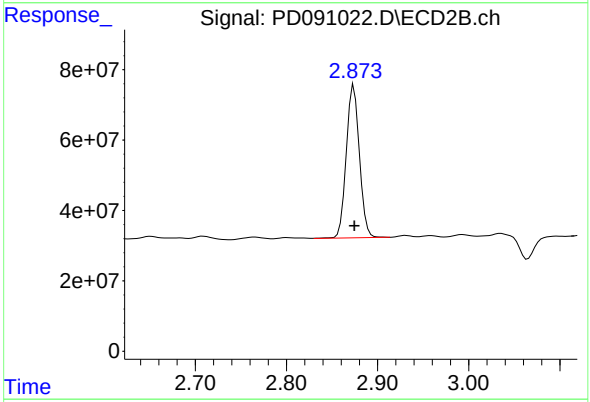

#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: 0.000 min
Response: 434203213
Conc: 14.58 ng/ml

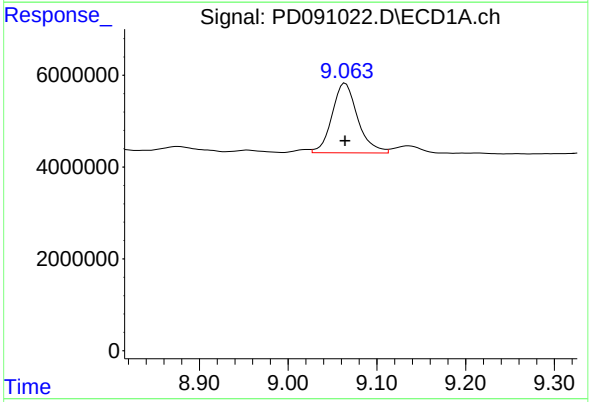

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: -0.001 min
Response: 30532676
Conc: 6.53 ng/ml m

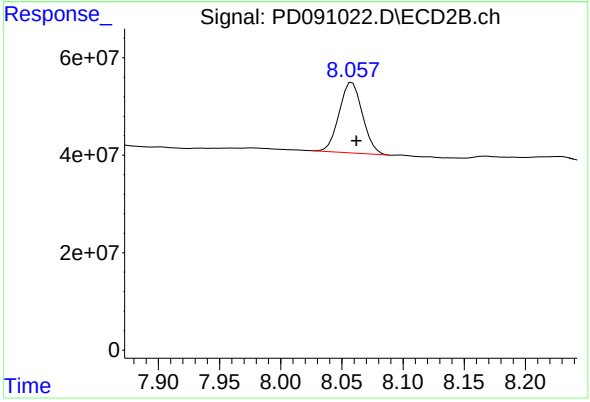

#28 Decachlorobiphenyl

R.T.: 8.057 min
Delta R.T.: -0.005 min
Response: 191967965
Conc: 6.34 ng/ml m