

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110818\
 Data File : PD050222.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2018 12:37
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 18:12:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103018.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 03:08:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.232	4.059	13977673	645.9E6	22.296	23.194
28)	SA Decachlor...	9.017	9.167	15106945	454.8E6	25.131	26.461
Target Compounds							
2)	A alpha-BHC	4.617f	4.519f	71155	56827865	0.075	1.297 #
6)	B beta-BHC	5.164f	4.952f	506694	8189848	1.338	0.512 #
7)	B delta-BHC	0.000	5.125	0	457891	N.D.	0.012 #
9)	A Endosulfan I	6.301f	0.000	1314283	0	1.757	N.D. #
11)	B alpha-Chl...	6.301	0.000	1314283	0	1.604	N.D. #
12)	B 4,4'-DDE	0.000	6.397	0	370438	N.D.	0.012 #
23)	Chlordane-1	5.164	5.125	506694	457891	17.285	0.328 #
26)	Chlordane-4	6.301	0.000	1314283	0	18.141	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110818\
Data File : PD050222.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2018 12:37
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 18:12:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103018.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 03:08:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

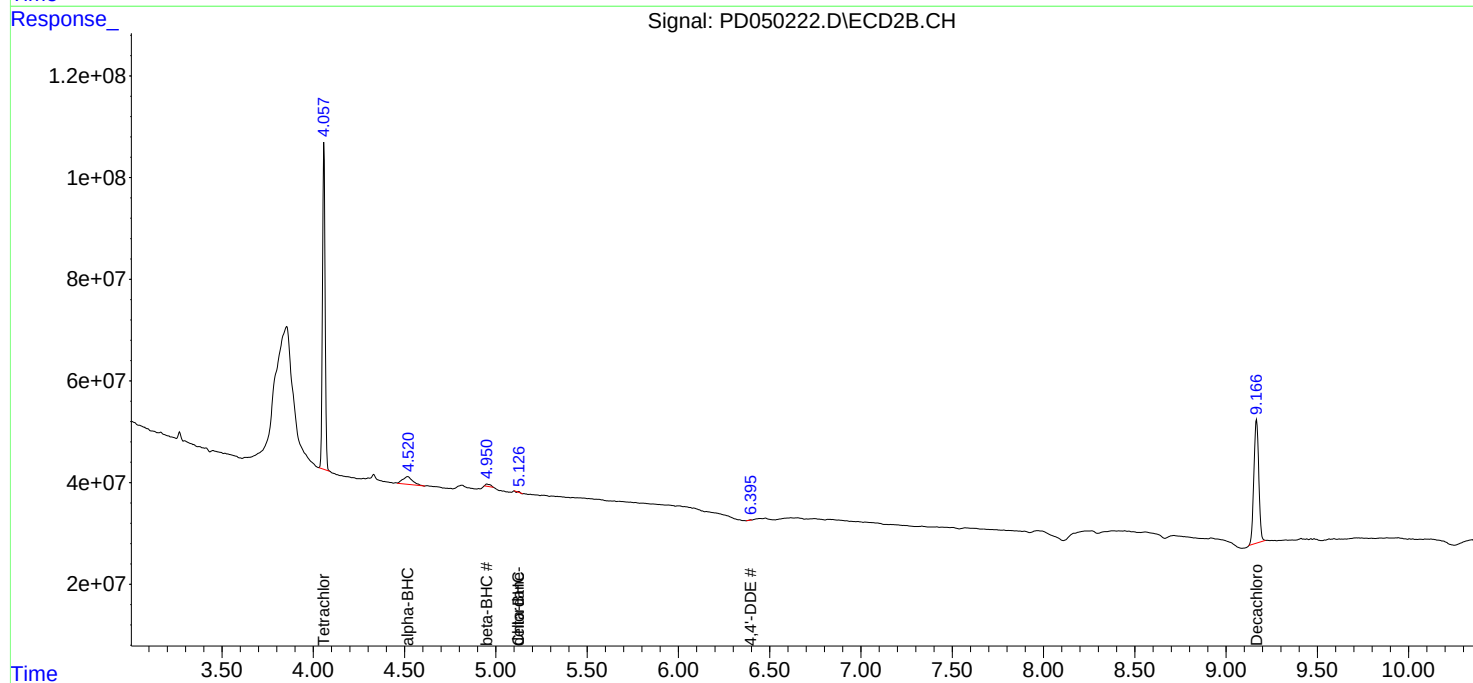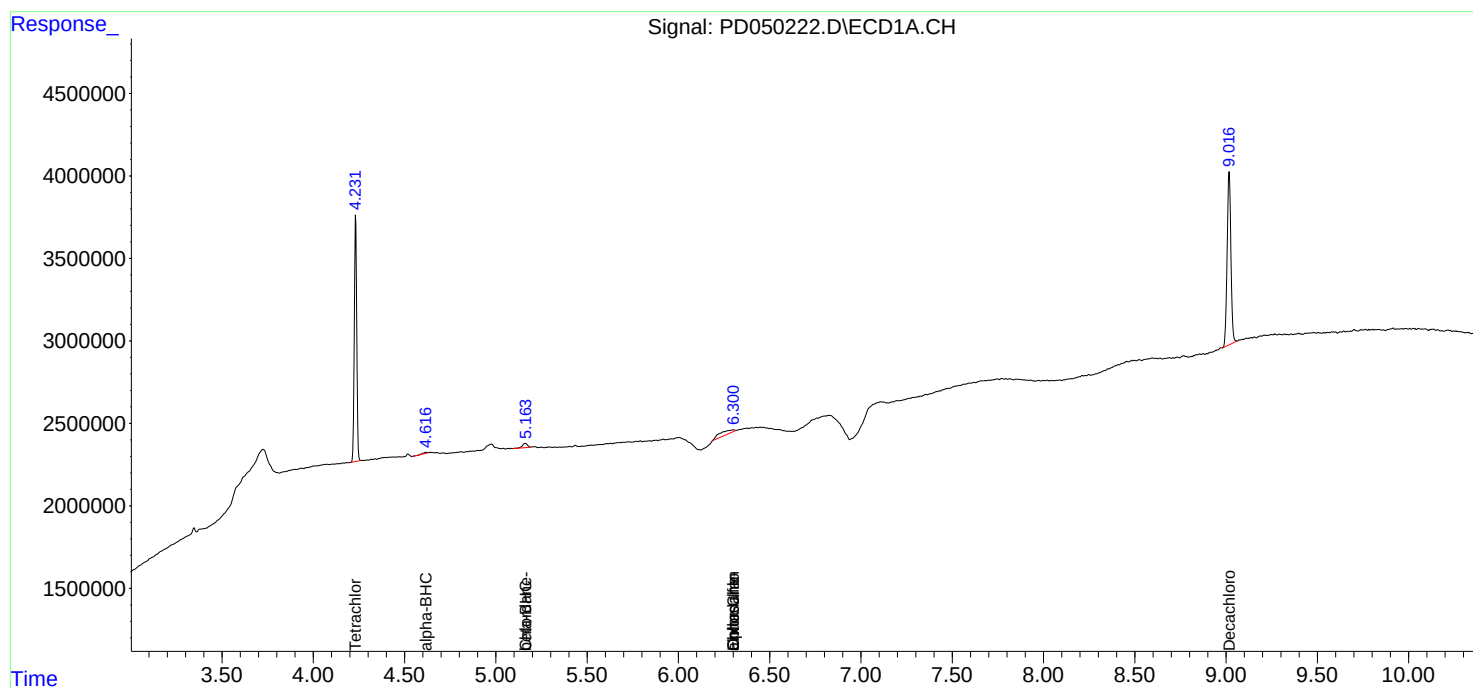


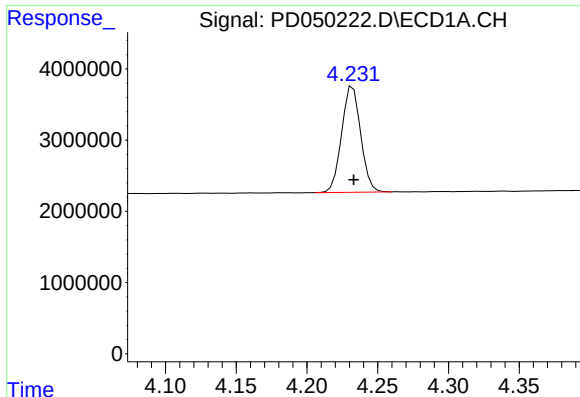

#1 Tetrachloro-m-xylene


R.T.: 4.232 min
Delta R.T.: 0.000 min
Response: 13977673
Conc: 22.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

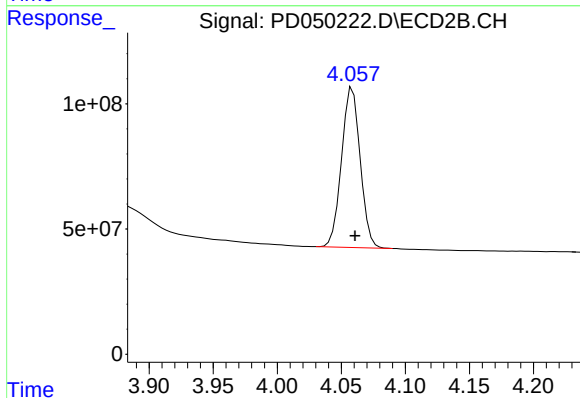


#1 Tetrachloro-m-xylene

R.T.: 4.059 min
Delta R.T.: -0.002 min
Response: 645937316
Conc: 23.19 ng/ml

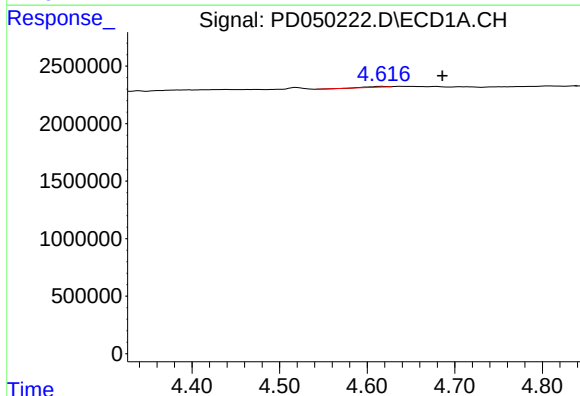


#2 alpha-BHC

R.T.: 4.617 min
Delta R.T.: -0.069 min
Response: 71155
Conc: 0.07 ng/ml

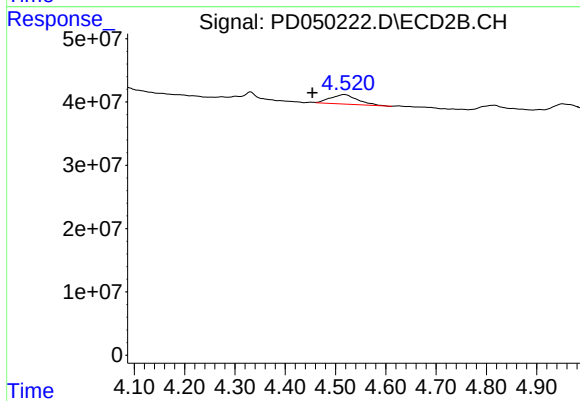

#2 alpha-BHC


R.T.: 4.519 min
Delta R.T.: 0.064 min
Response: 56827865
Conc: 1.30 ng/ml

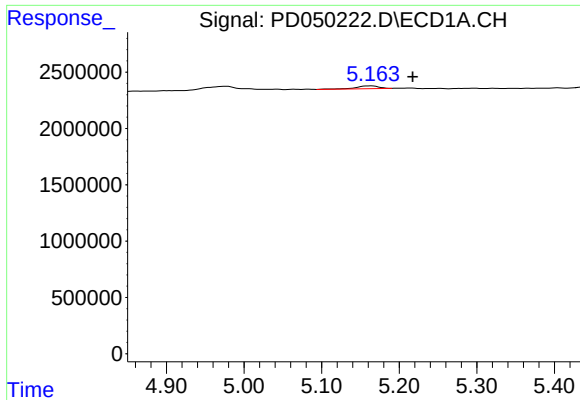

#6 beta-BHC


R.T.: 5.164 min
Delta R.T.: -0.054 min
Response: 506694
Conc: 1.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

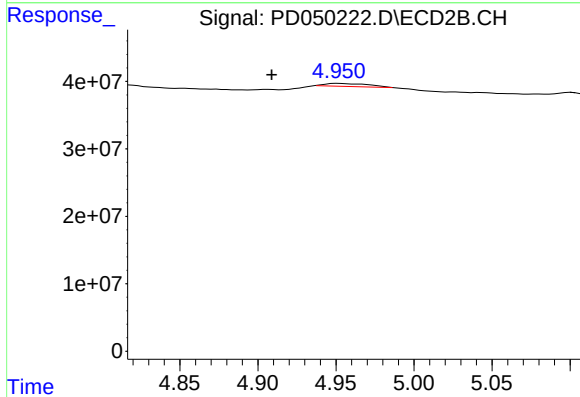


#6 beta-BHC

R.T.: 4.952 min
Delta R.T.: 0.043 min
Response: 8189848
Conc: 0.51 ng/ml

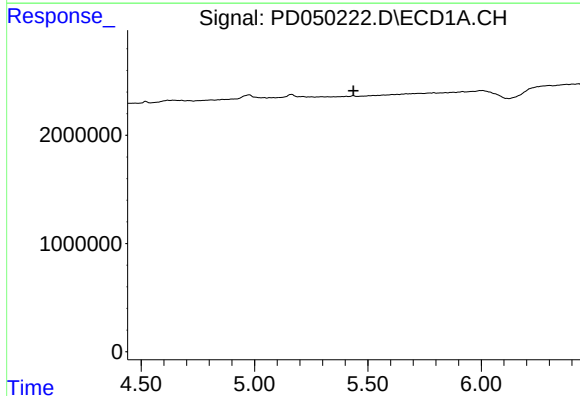


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.437 min
Response: 0
Conc: N.D.

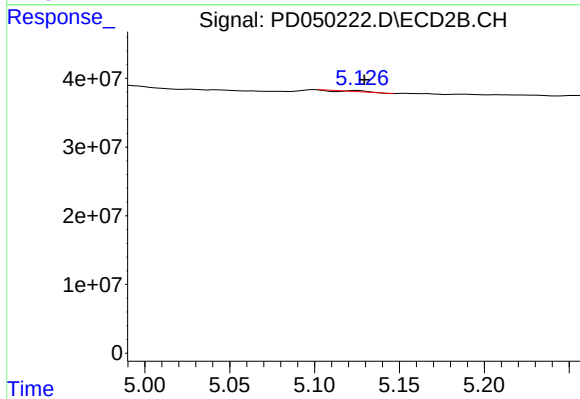

#7 delta-BHC


R.T.: 5.125 min
Delta R.T.: -0.004 min
Response: 457891
Conc: 0.01 ng/ml

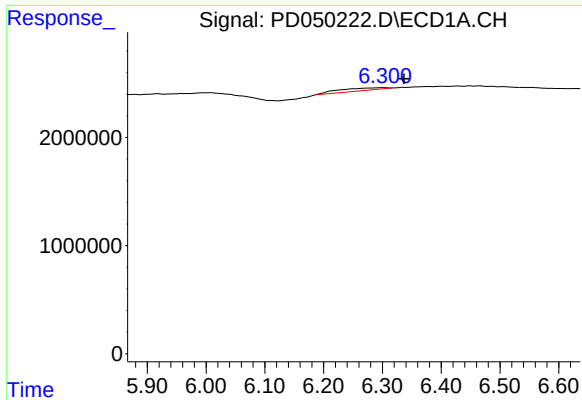

#9 Endosulfan I


R.T.: 6.301 min
Delta R.T.: -0.035 min
Response: 1314283
Conc: 1.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

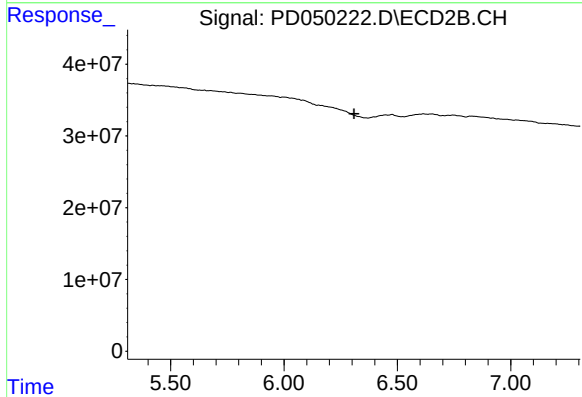


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

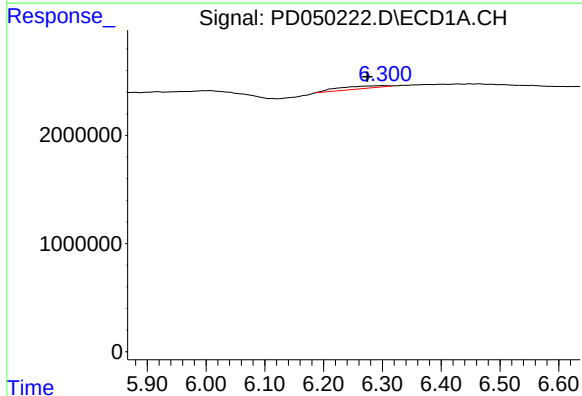


#11 alpha-Chlordane

R.T.: 6.301 min
Delta R.T.: 0.027 min
Response: 1314283
Conc: 1.60 ng/ml

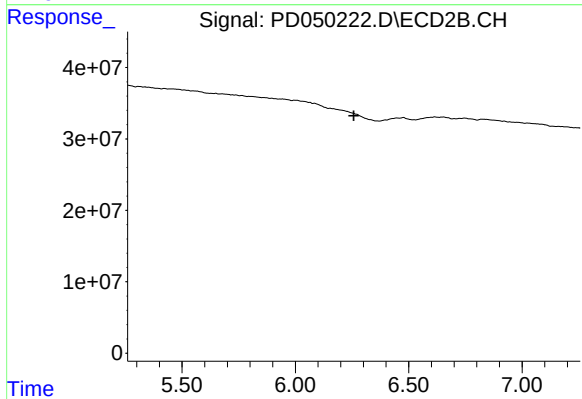

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.258 min
Response: 0
Conc: N.D.

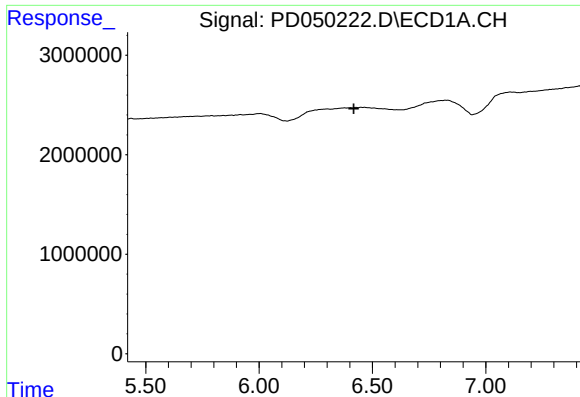

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

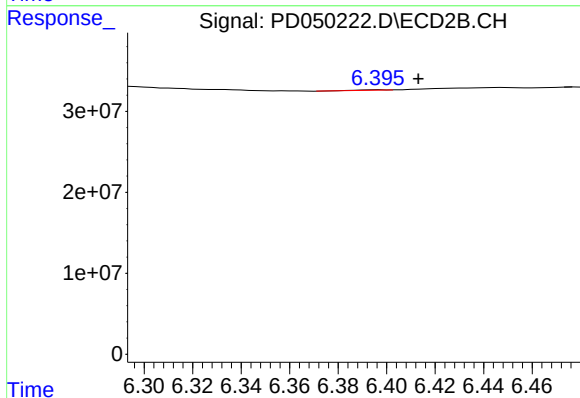


#12 4,4'-DDE

R.T.: 6.397 min
Delta R.T.: -0.016 min
Response: 370438
Conc: 0.01 ng/ml

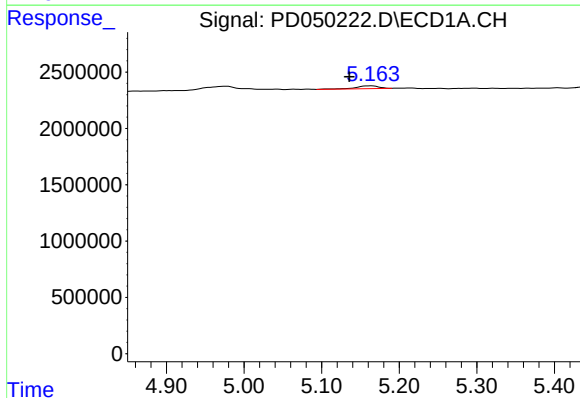


#23 Chlordane-1

R.T.: 5.164 min
Delta R.T.: 0.028 min
Response: 506694
Conc: 17.28 ng/ml

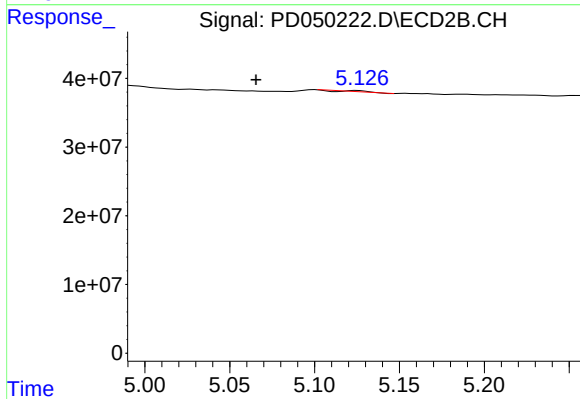

#23 Chlordane-1


R.T.: 5.125 min
Delta R.T.: 0.060 min
Response: 457891
Conc: 0.33 ng/ml

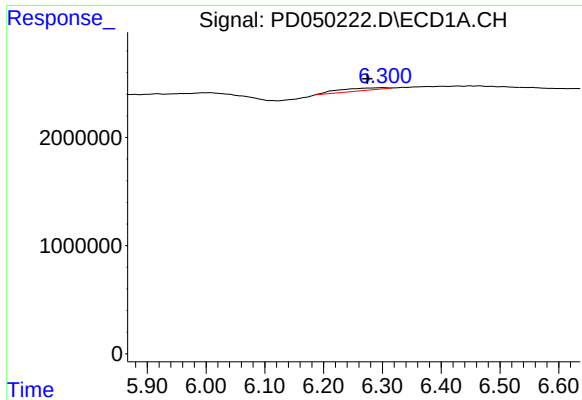

#26 Chlordane-4


R.T.: 6.301 min
Delta R.T.: 0.027 min
Response: 1314283
Conc: 18.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

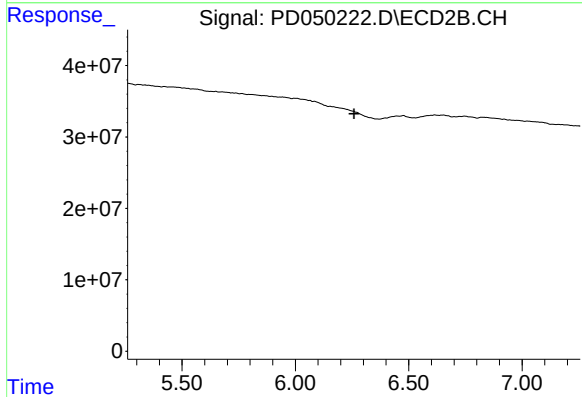


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.260 min
Response: 0
Conc: N.D.

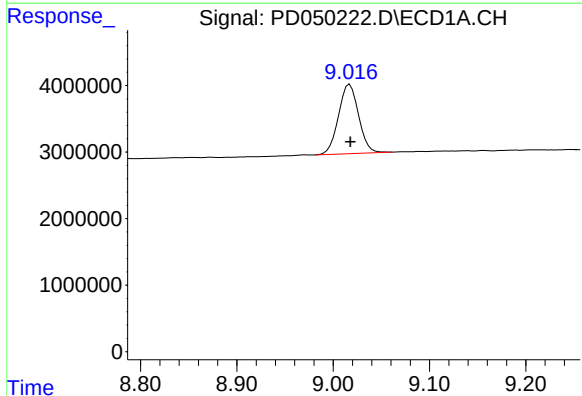

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: 0.000 min
Response: 15106945
Conc: 25.13 ng/ml

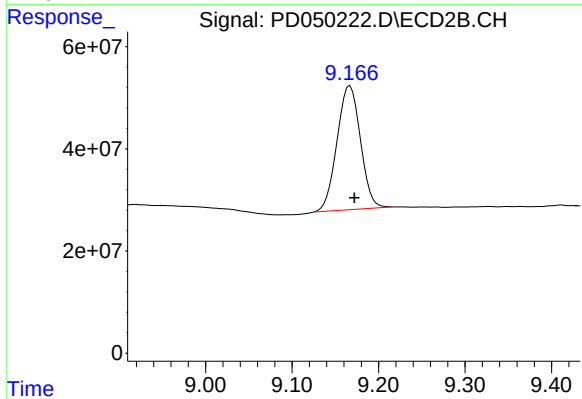

#28 Decachlorobiphenyl

R.T.: 9.167 min
Delta R.T.: -0.005 min
Response: 454826871
Conc: 26.46 ng/ml