

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110818\
 Data File : PD050228.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2018 14:43
 Operator : AJ\SJ
 Sample : J5768-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OK-02-110718-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 18:13:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103018.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 03:08:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.232	4.059	10076640	392.0E6	16.074	14.075
28) SA Decachlor...	9.016	9.167	9544630	288.9E6	15.878	16.808
Target Compounds						
10) B gamma-Chl...	6.216	6.180	727287	35327071	0.880m	1.090m
11) B alpha-Chl...	6.272	6.255	1356696	110.5E6	1.656m	3.567m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110818\
Data File : PD050228.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2018 14:43
Operator : AJ\SJ
Sample : J5768-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
OK-02-110718-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 18:13:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103018.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 03:08:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

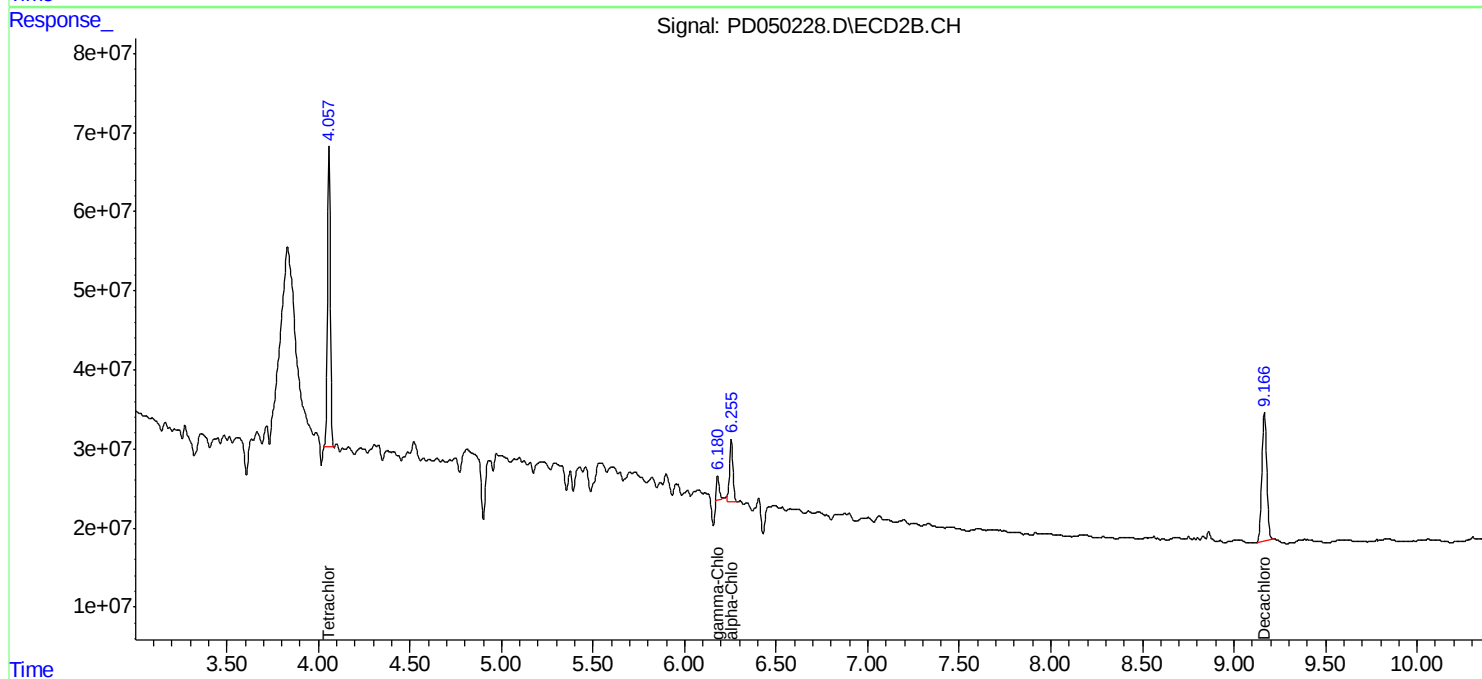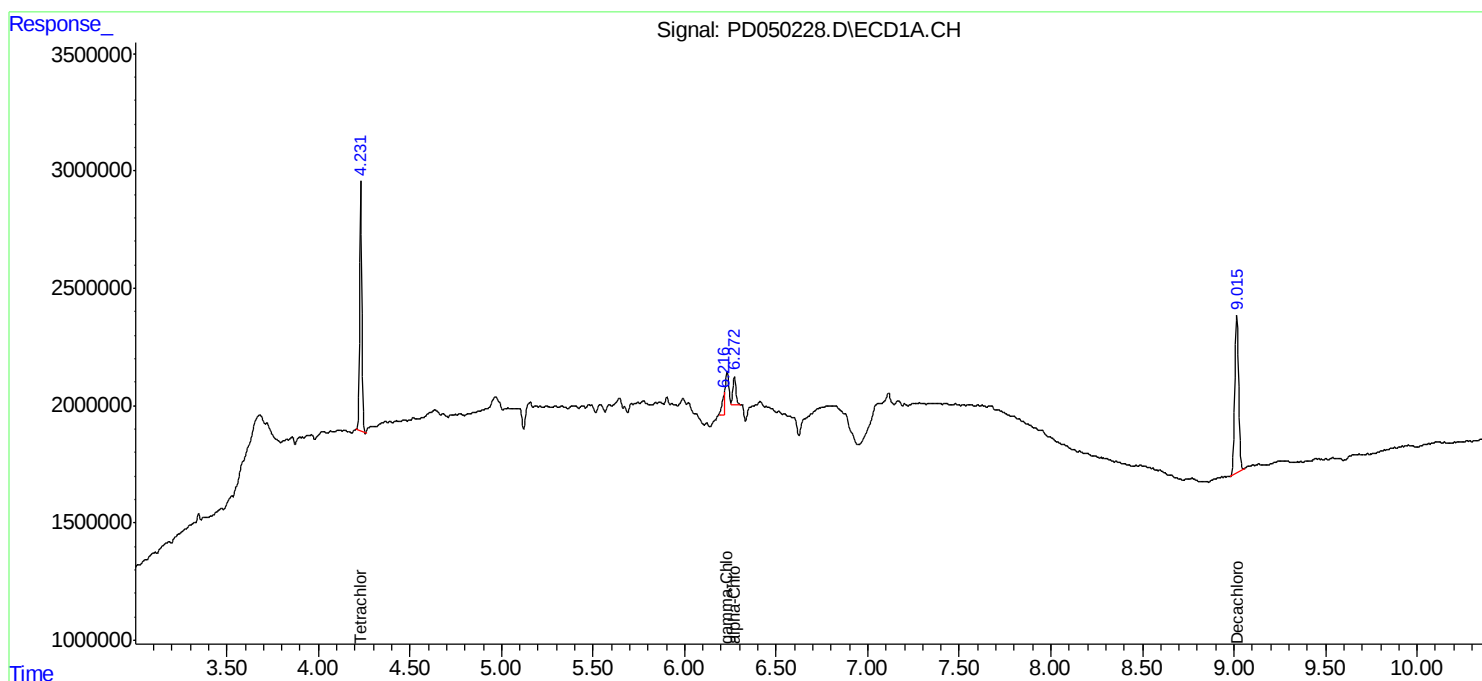


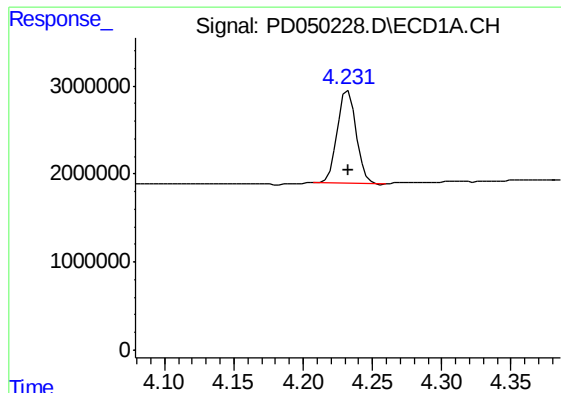

#1 Tetrachloro-m-xylene


R.T.: 4.232 min
Delta R.T.: 0.000 min
Response: 10076640
Conc: 16.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-02-110718-B

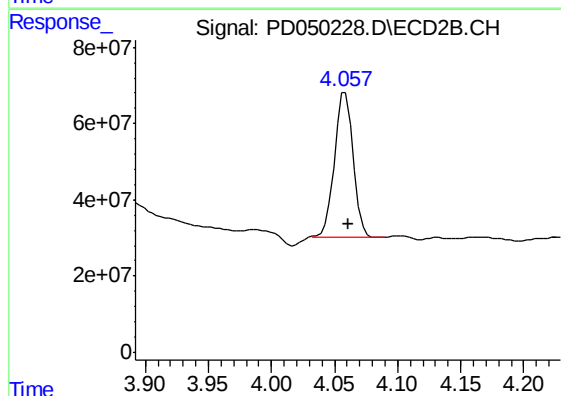


#1 Tetrachloro-m-xylene

R.T.: 4.059 min
Delta R.T.: -0.002 min
Response: 391991714
Conc: 14.08 ng/ml

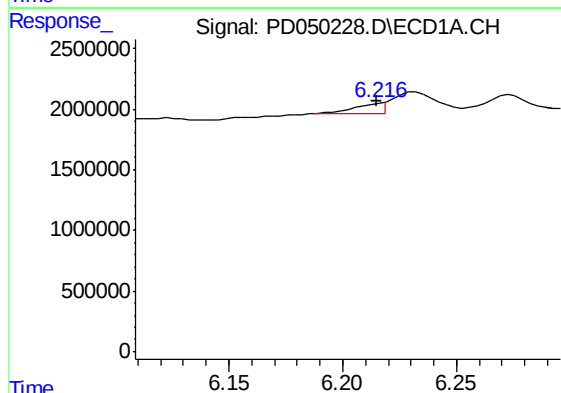


#10 gamma-Chlordane

R.T.: 6.216 min
Delta R.T.: 0.000 min
Response: 727287
Conc: 0.88 ng/ml m

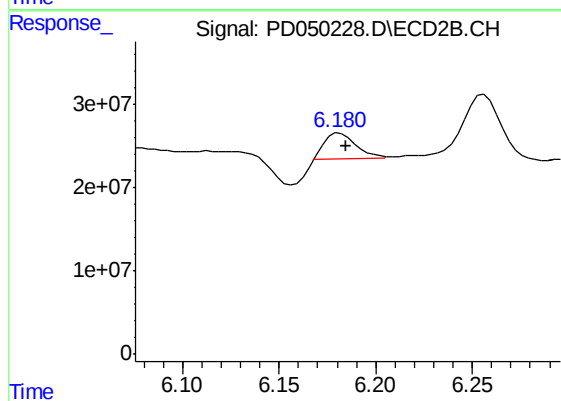

#10 gamma-Chlordane


R.T.: 6.180 min
Delta R.T.: -0.005 min
Response: 35327071
Conc: 1.09 ng/ml m

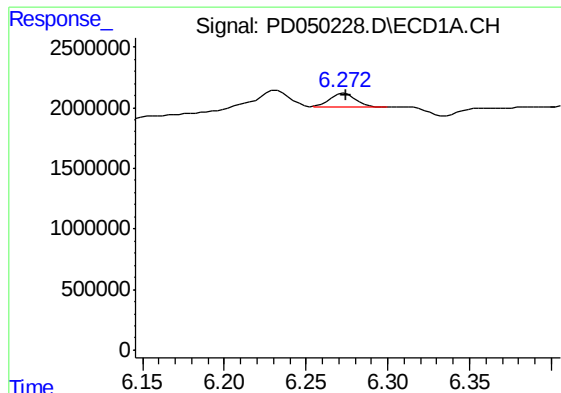

#11 alpha-Chlordane


R.T.: 6.272 min
Delta R.T.: -0.002 min
Response: 1356696
Conc: 1.66 ng/ml m

Instrument :
ECD_D
ClientSampleId :
OK-02-110718-B

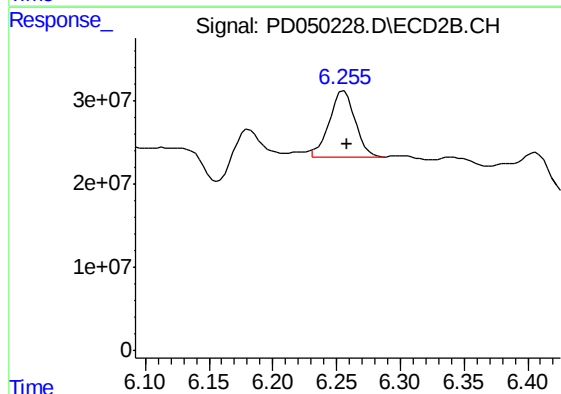


#11 alpha-Chlordane

R.T.: 6.255 min
Delta R.T.: -0.004 min
Response: 110502705
Conc: 3.57 ng/ml m

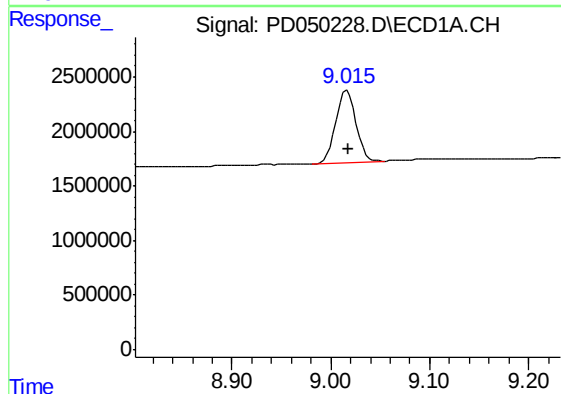

#28 Decachlorobiphenyl

R.T.: 9.016 min
Delta R.T.: -0.001 min
Response: 9544630
Conc: 15.88 ng/ml

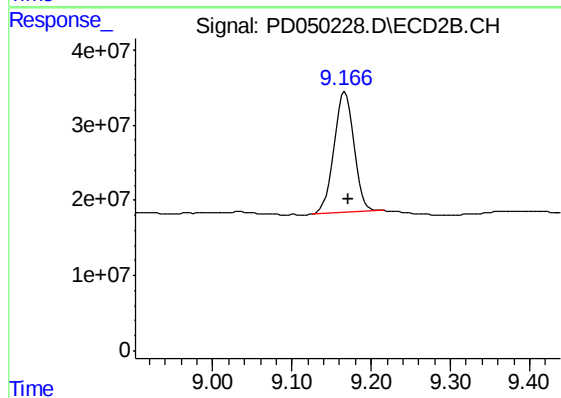

#28 Decachlorobiphenyl

R.T.: 9.167 min
Delta R.T.: -0.005 min
Response: 288908811
Conc: 16.81 ng/ml