

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
 Data File : PD072846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 12:39
 Operator : AR\AJ
 Sample : TOXAPH501
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 15:14:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 15:12:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.701	3.462	174.7E6	3044.5E6	81.108	72.787
27)	SA Decachlor...	7.830	8.912	288.9E6	1407.0E6	156.755	148.813
Target Compounds							
22)	Toxaphene-1	5.247	5.769	116.4E6	526.6E6	8751.455	7103.101
23)	Toxaphene-2	5.606	6.146	123.2E6	979.2E6	8891.897	7425.705
24)	Toxaphene-3	5.891	6.967	165.5E6	2555.0E6	8592.590	7803.995
25)	Toxaphene-4	6.650	7.057	712.3E6	2147.6E6	8913.026	7886.770
26)	Toxaphene-5	6.960	7.485	396.4E6	1375.2E6	9057.031	8114.870

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
Data File : PD072846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 12:39
Operator : AR\AJ
Sample : TOXAPH501
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 15:14:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 15:12:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

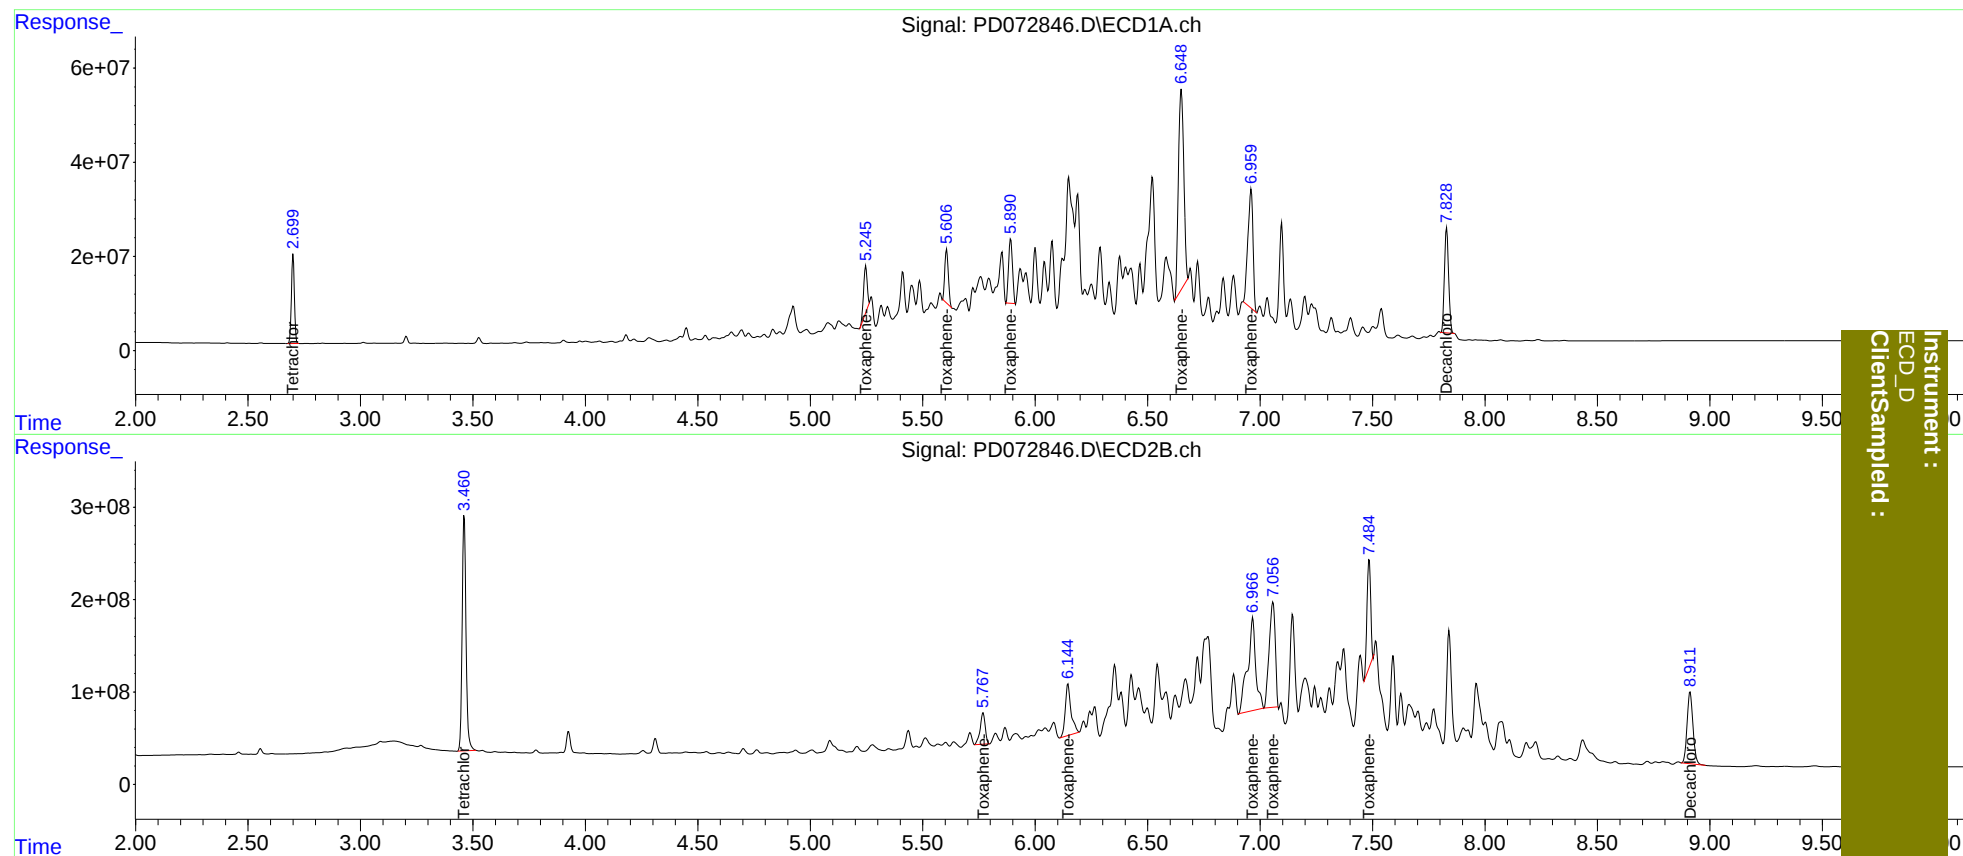

Instrument :
ECD_D
ClientSampled :
0