

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
 Data File : PD072855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 14:39
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 15:42:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 15:38:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.700	3.462	178.6E6	2961.0E6	75.324	66.719
27)	SA Decachlor...	7.830	8.912	333.0E6	1498.6E6	143.244	137.747
Target Compounds							
2)	A alpha-BHC	3.204	3.926	300.6E6	3965.5E6	82.993	68.727
3)	MA gamma-BHC...	3.534	4.260	271.4E6	3061.4E6	81.452	67.269
4)	MA Heptachlor	3.867	4.825	269.1E6	2057.4E6	79.542	65.537
9)	A Endosulfan I	5.019	5.981	217.5E6	1332.8E6	76.930	67.044
13)	MA Dieldrin	5.285	6.257	496.0E6	2840.0E6	159.263	140.095
14)	MA Endrin	5.562	6.489	439.8E6	2377.9E6	158.192	140.158
16)	A 4,4'-DDD	5.709	6.623	389.7E6	2112.9E6	157.990	140.184
17)	MA 4,4'-DDT	5.957	6.931	399.5E6	2121.6E6	165.152	144.979
20)	A Methoxychlor	6.541	7.411	991.5E6	4538.4E6	733.970	691.395

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
Data File : PD072855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 14:39
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 15:42:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 15:38:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

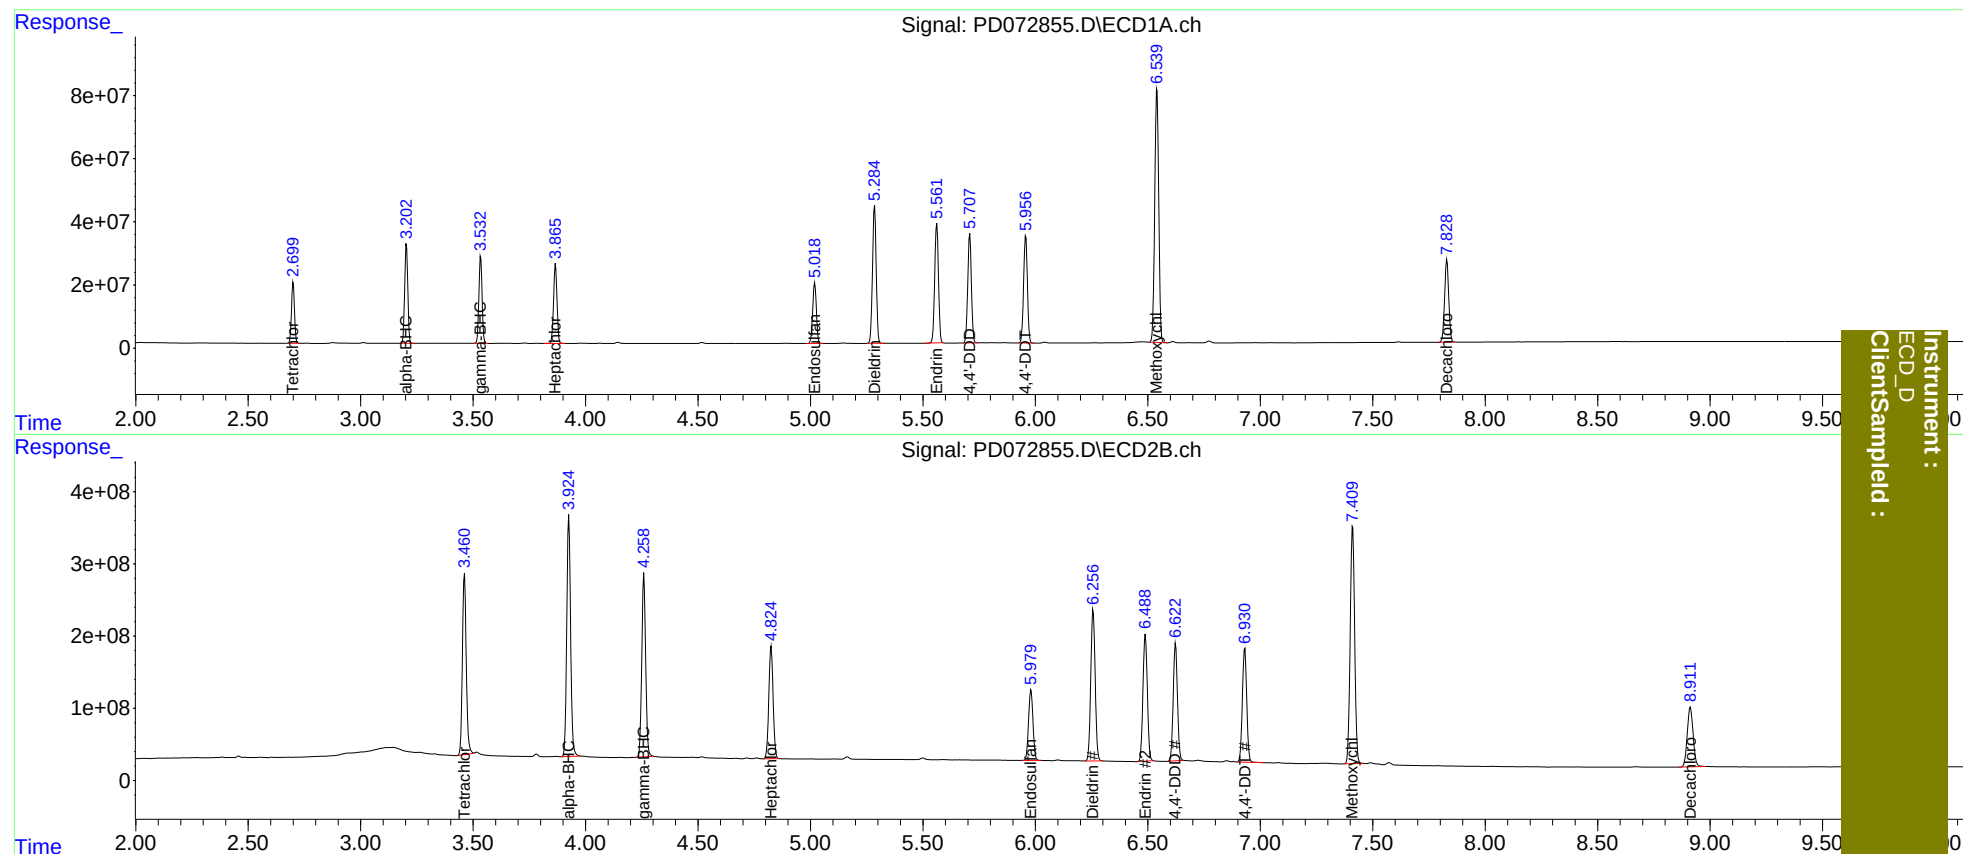


Instrument :
ECD_D
ClientSampled :
0

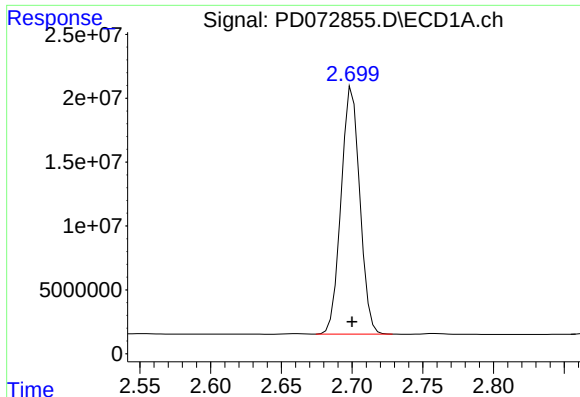

#1 Tetrachloro-m-xylene


R.T.: 2.700 min
Delta R.T.: 0.000 min
Response: 178645509
Conc: 75.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

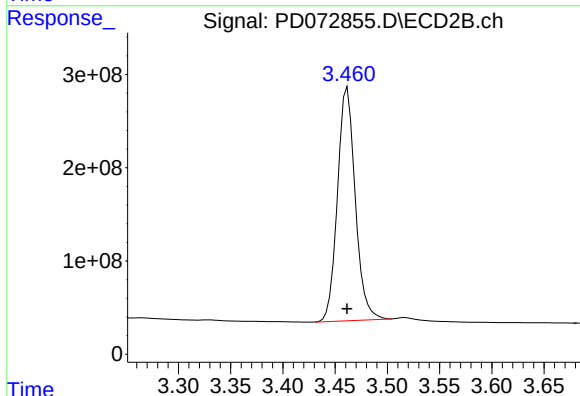


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: 0.000 min
Response: 2961013199
Conc: 66.72 ng/ml

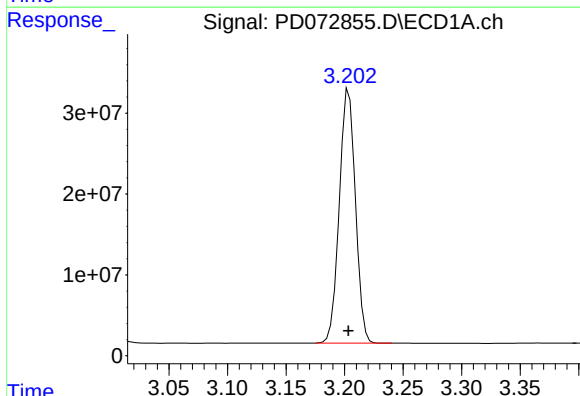


#2 alpha-BHC

R.T.: 3.204 min
Delta R.T.: 0.000 min
Response: 300633128
Conc: 82.99 ng/ml

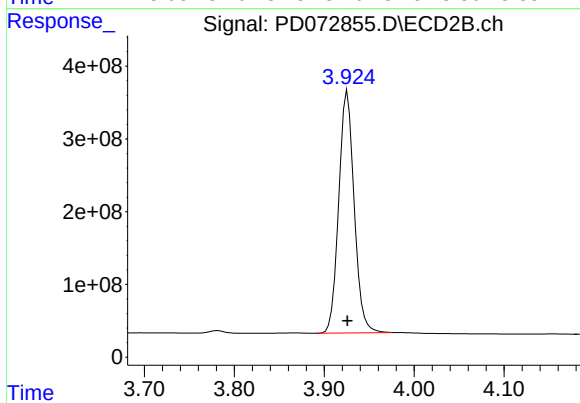

#2 alpha-BHC


R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 3965458014
Conc: 68.73 ng/ml

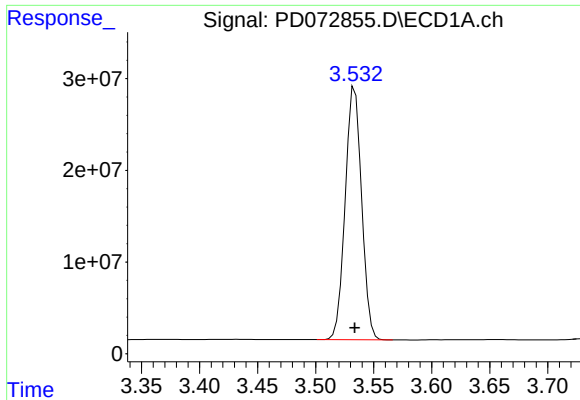

#3 gamma-BHC (Lindane)


R.T.: 3.534 min
Delta R.T.: 0.000 min
Response: 271389177
Conc: 81.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

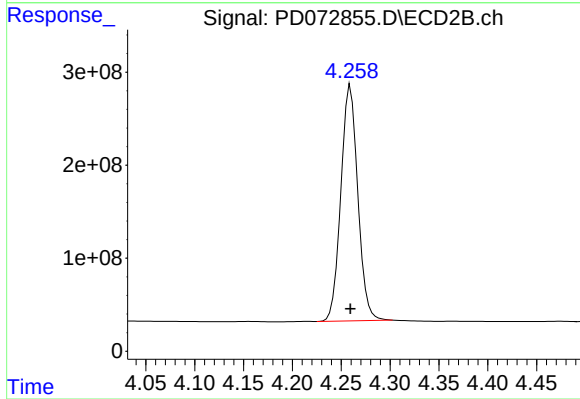


#3 gamma-BHC (Lindane)

R.T.: 4.260 min
Delta R.T.: 0.000 min
Response: 3061398612
Conc: 67.27 ng/ml

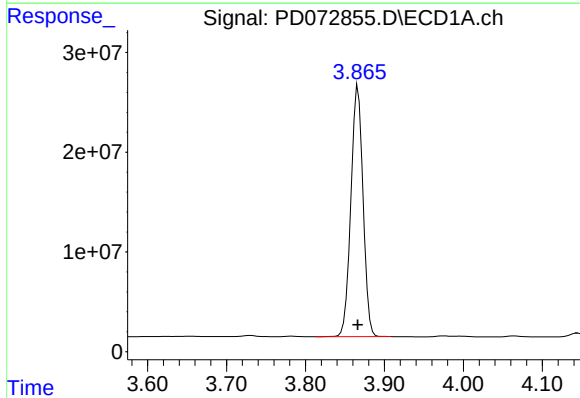


#4 Heptachlor

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 269128652
Conc: 79.54 ng/ml

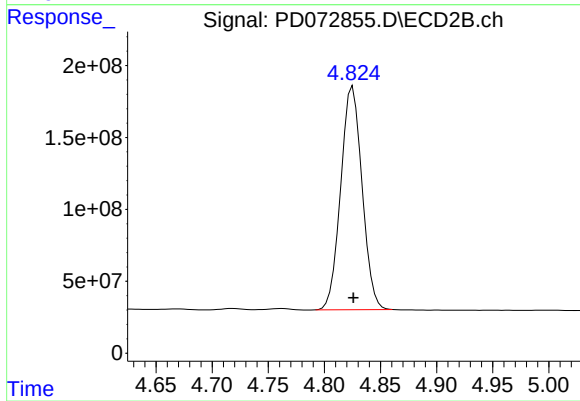

#4 Heptachlor


R.T.: 4.825 min
Delta R.T.: 0.000 min
Response: 2057371000
Conc: 65.54 ng/ml

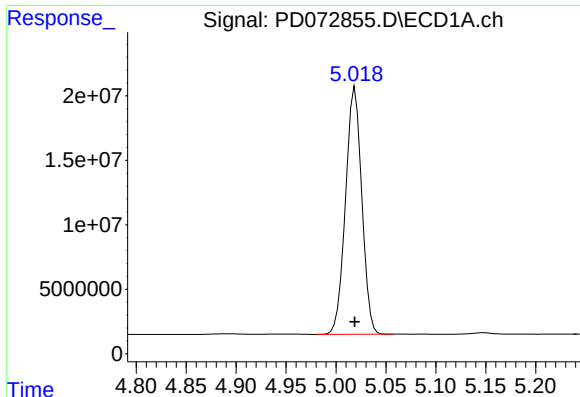

#9 Endosulfan I


R.T.: 5.019 min
Delta R.T.: 0.000 min
Response: 217481090
Conc: 76.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

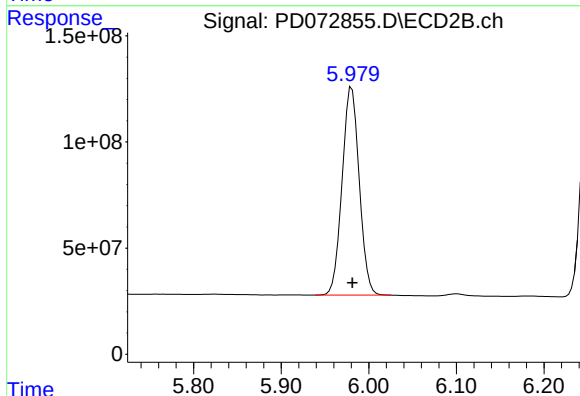


#9 Endosulfan I

R.T.: 5.981 min
Delta R.T.: 0.000 min
Response: 1332816287
Conc: 67.04 ng/ml

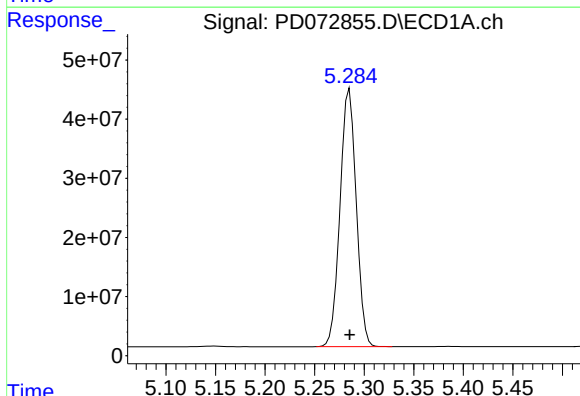


#13 Dieldrin

R.T.: 5.285 min
Delta R.T.: 0.000 min
Response: 496049259
Conc: 159.26 ng/ml

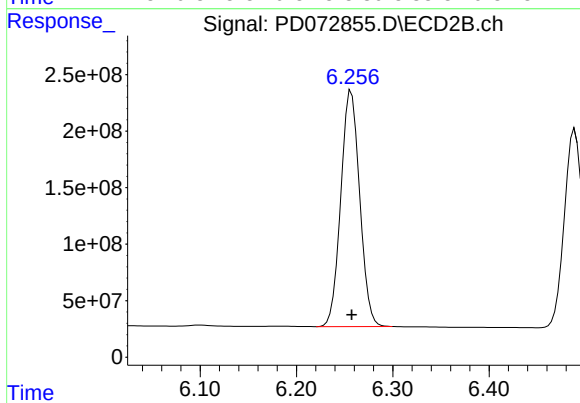

#13 Dieldrin


R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 2840004319
Conc: 140.09 ng/ml

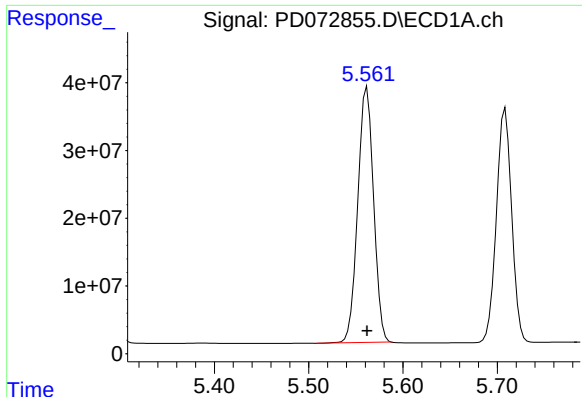

#14 Endrin


R.T.: 5.562 min
Delta R.T.: 0.000 min
Response: 439765072
Conc: 158.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

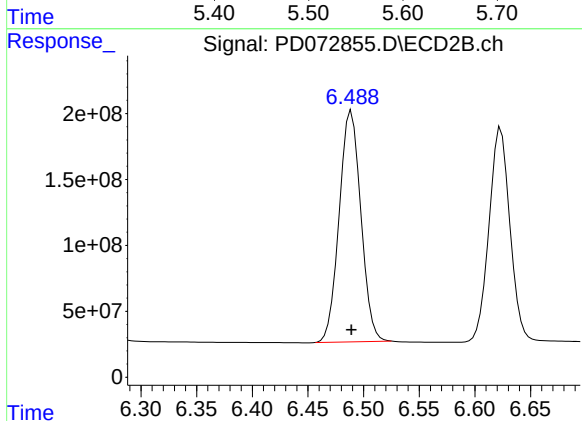


#14 Endrin

R.T.: 6.489 min
Delta R.T.: 0.000 min
Response: 2377893137
Conc: 140.16 ng/ml

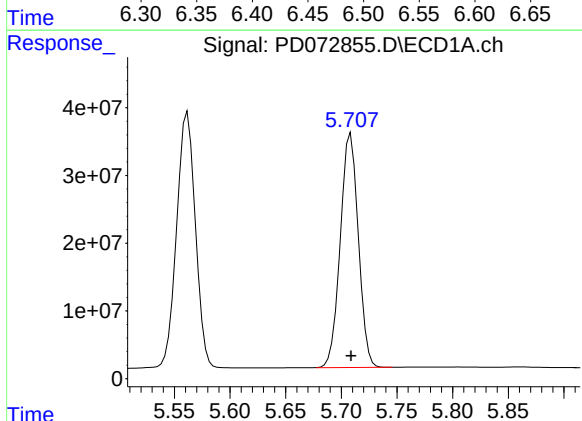


#16 4,4'-DDD

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 389710187
Conc: 157.99 ng/ml

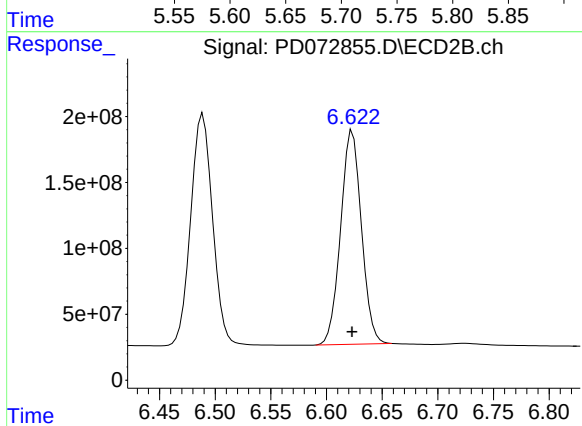

#16 4,4'-DDD


R.T.: 6.623 min
Delta R.T.: 0.000 min
Response: 2112909444
Conc: 140.18 ng/ml

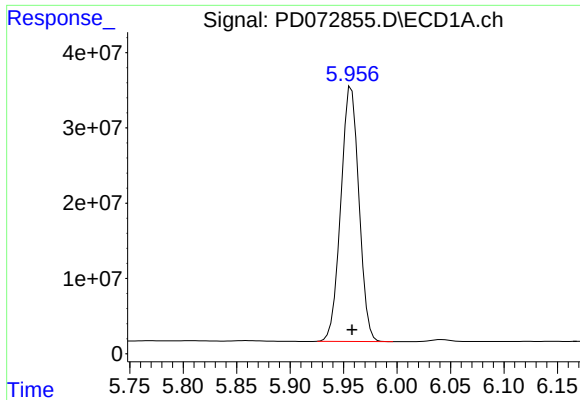

#17 4,4'-DDT


R.T.: 5.957 min
Delta R.T.: 0.000 min
Response: 399540795
Conc: 165.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

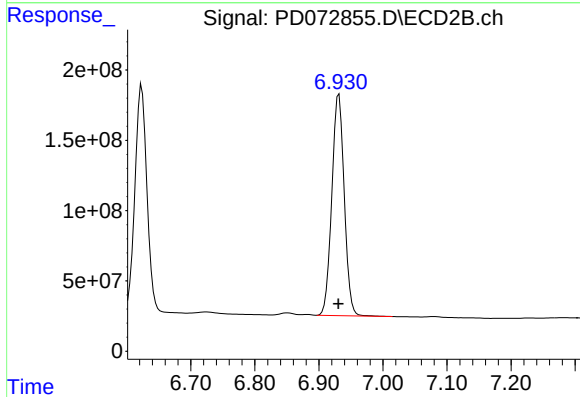


#17 4,4'-DDT

R.T.: 6.931 min
Delta R.T.: 0.000 min
Response: 2121603587
Conc: 144.98 ng/ml

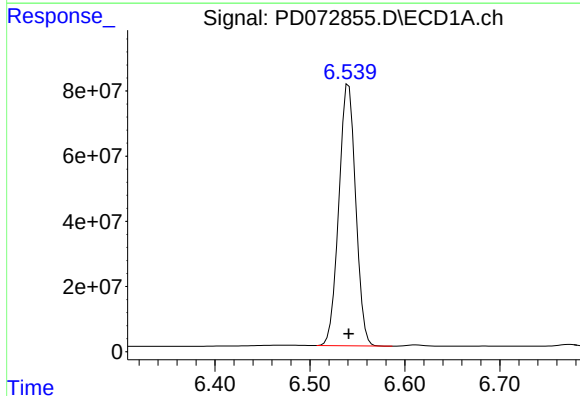


#20 Methoxychlor

R.T.: 6.541 min
Delta R.T.: 0.000 min
Response: 991451662
Conc: 733.97 ng/ml

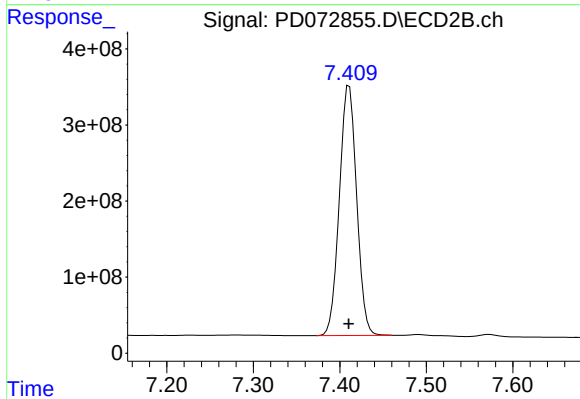

#20 Methoxychlor

R.T.: 7.411 min
Delta R.T.: 0.000 min
Response: 4538439298
Conc: 691.40 ng/ml

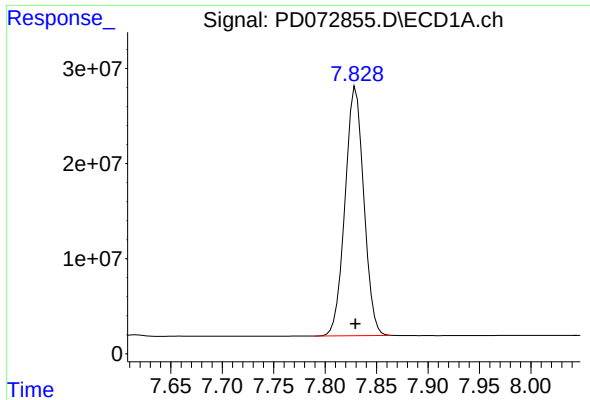

#27 Decachlorobiphenyl


R.T.: 7.830 min

Delta R.T.: 0.000 min

Response: 332961966

Conc: 143.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

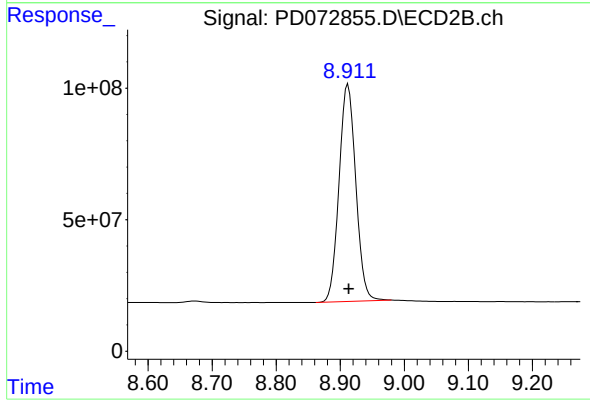

#27 Decachlorobiphenyl

R.T.: 8.912 min

Delta R.T.: 0.000 min

Response: 1498573199

Conc: 137.75 ng/ml