

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
 Data File : PD072853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 14:12
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4078

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 15:42:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 15:38:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.700	3.462	88102063	1611.8E6	37.147	36.317
27)	SA Decachlor...	7.830	8.914	162.5E6	753.7E6	69.920	69.282
Target Compounds							
2)	A alpha-BHC	3.204	3.926	140.7E6	2057.8E6	38.852	35.664
3)	MA gamma-BHC...	3.534	4.259	127.9E6	1587.2E6	38.388	34.876
4)	MA Heptachlor	3.866	4.826	126.4E6	1079.8E6	37.366	34.396
9)	A Endosulfan I	5.019	5.981	104.3E6	692.5E6	36.897	34.833
13)	MA Dieldrin	5.286	6.258	233.3E6	1438.5E6	74.919	70.961
14)	MA Endrin	5.562	6.490	205.5E6	1194.4E6	73.912	70.398
16)	A 4,4'-DDD	5.709	6.623	183.4E6	1068.1E6	74.370	70.864
17)	MA 4,4'-DDT	5.958	6.932	181.1E6	1045.3E6	74.876	71.433
20)	A Methoxychlor	6.541	7.411	478.9E6	2290.3E6	354.547	348.910

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
Data File : PD072853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 14:12
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 15:42:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 15:38:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

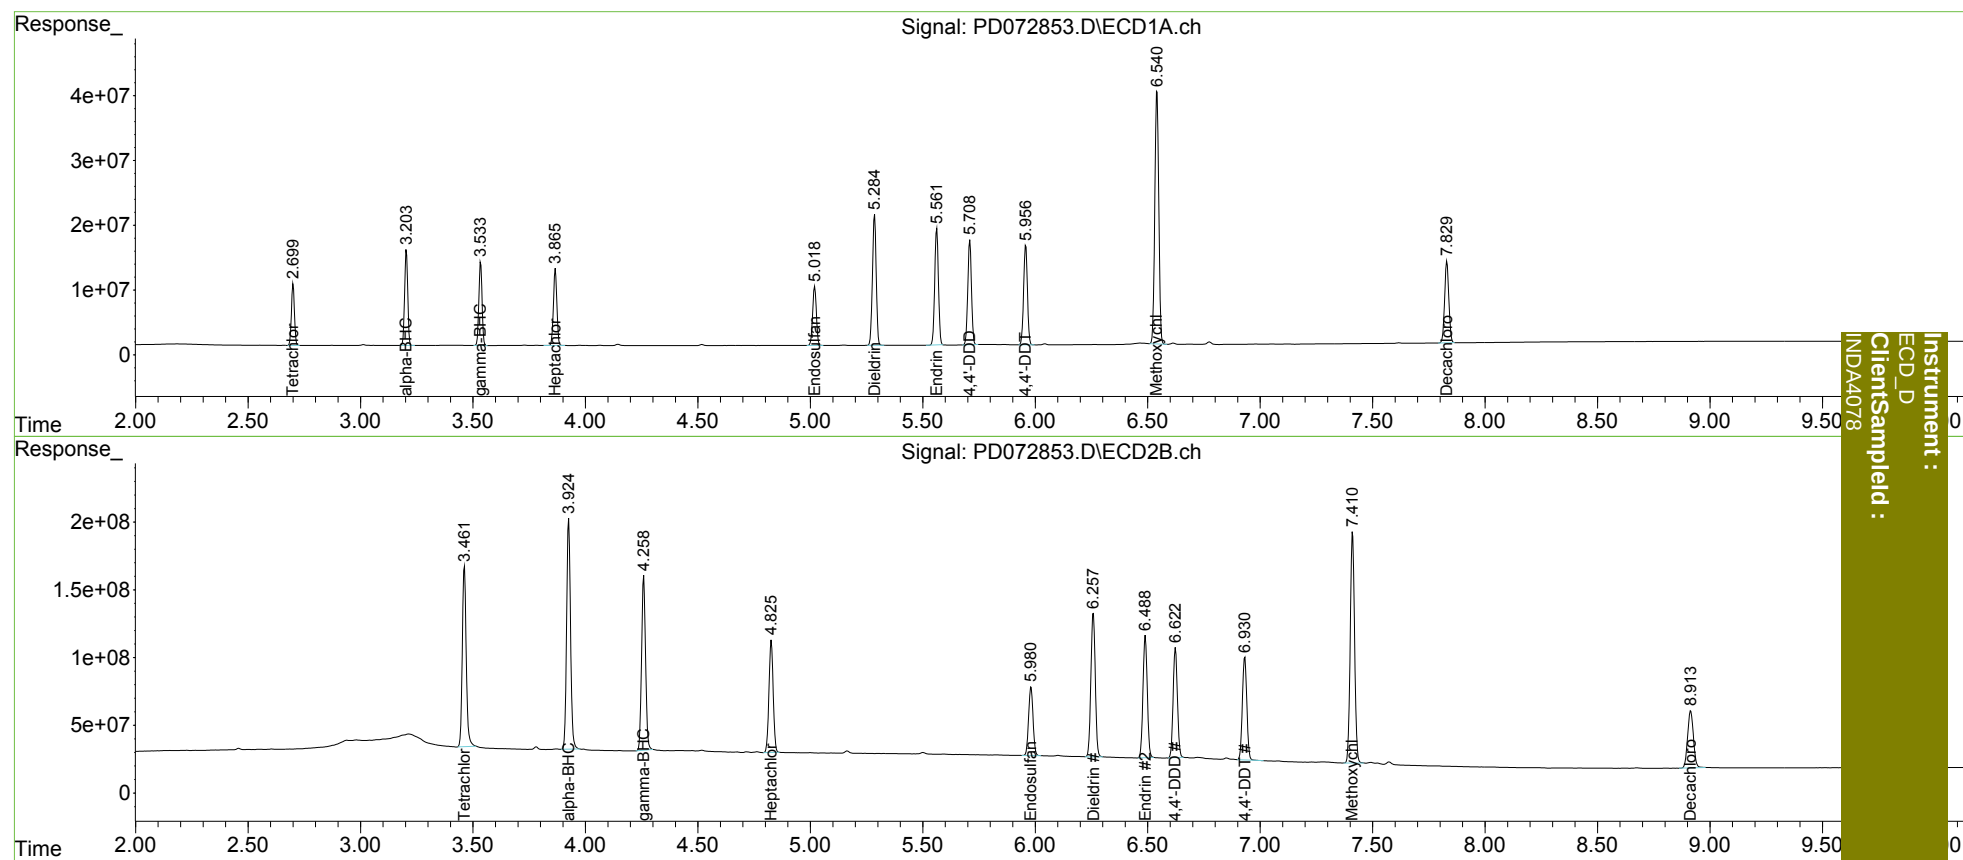

Instrument :
ECD_D
ClientSampled :
INDA4078