

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
 Data File : PD072871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 20:08
 Operator : AR\AJ
 Sample : INDA374
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3218

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 02:13:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 16:13:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.700	3.461	46578411	863.5E6	19.958	19.809
27)	SA Decachlor...	7.829	8.912	85220887	414.9E6	37.518	39.421
Target Compounds							
2)	A alpha-BHC	3.204	3.925	70495243	1119.5E6	19.974	19.784
3)	MA gamma-BHC...	3.534	4.259	65350268	880.0E6	20.101	19.658
4)	MA Heptachlor	3.866	4.825	65135451	594.9E6	19.825	19.323
9)	A Endosulfan I	5.019	5.980	52601328	371.6E6	19.007	19.258
13)	MA Dieldrin	5.285	6.257	115.7E6	770.6E6	38.608	38.848
14)	MA Endrin	5.561	6.489	101.5E6	640.6E6	37.978	38.793
16)	A 4,4'-DDD	5.708	6.623	90365756	574.7E6	38.210	39.182
17)	MA 4,4'-DDT	5.957	6.930	86823883	548.3E6	37.567	38.530
20)	A Methoxychlor	6.540	7.410	243.4E6	1232.1E6	189.477	194.483

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
Data File : PD072871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 20:08
Operator : AR\AJ
Sample : INDA374
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 02:13:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 16:13:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

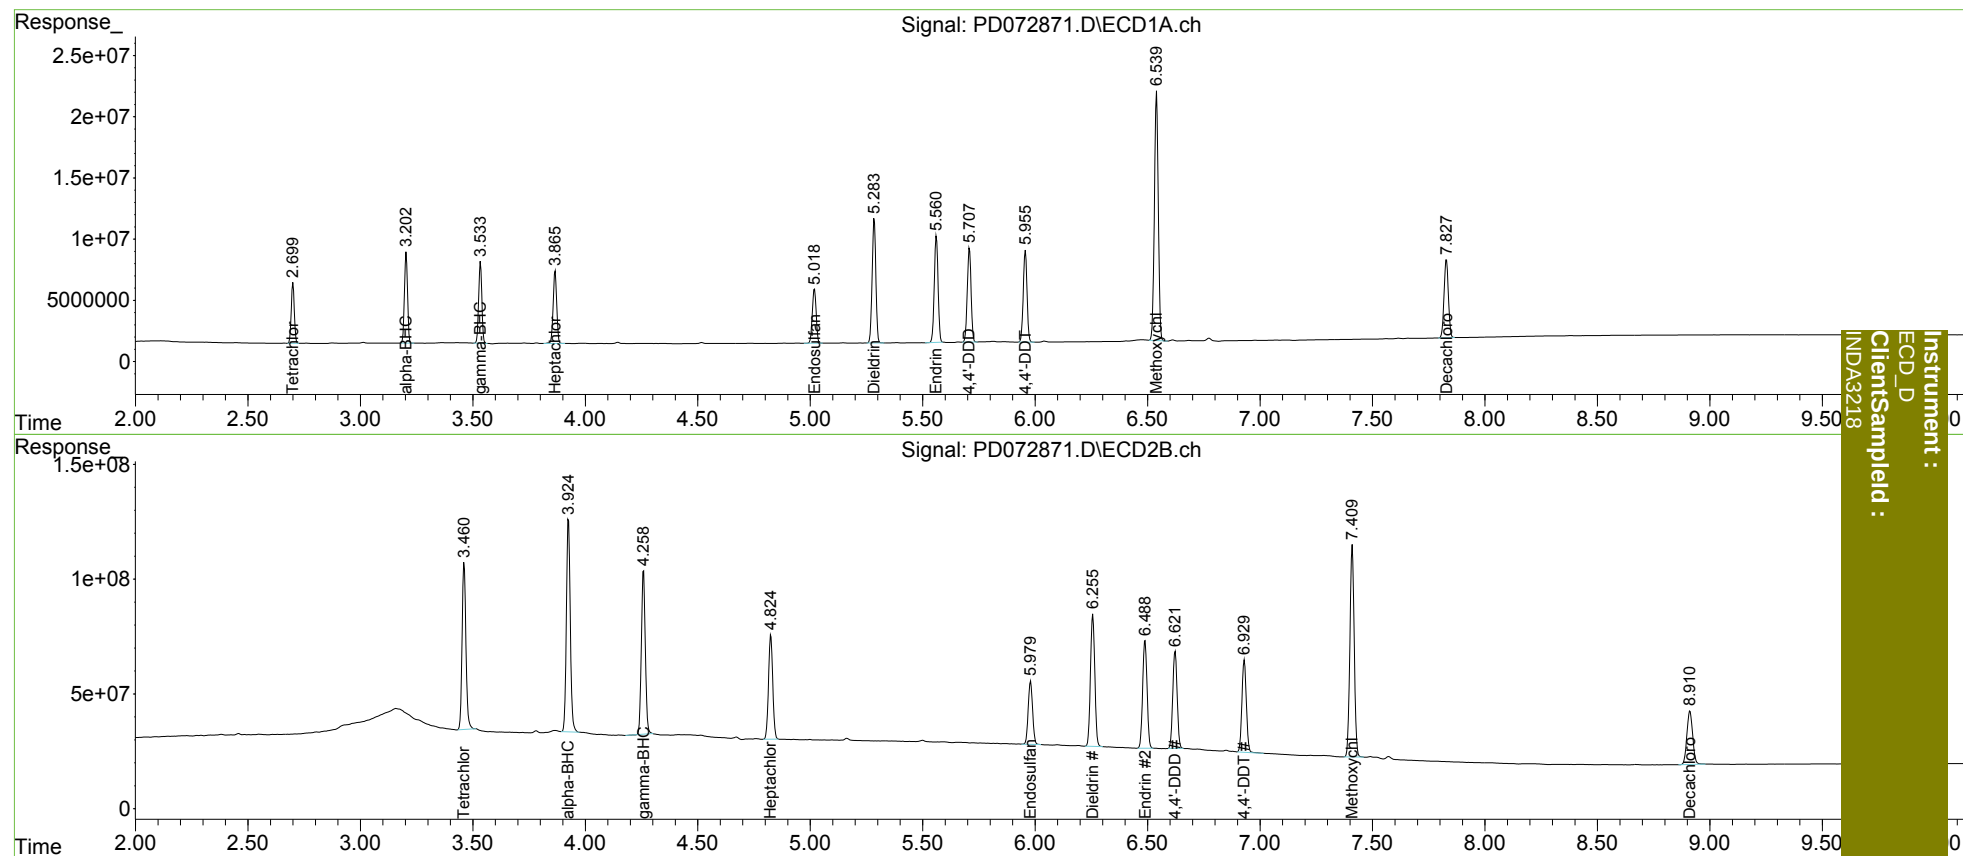

Instrument :
ECD_D
ClientSampled :
INDA3218